


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102720\
 Data File : BN012402.D
 Acq On : 27 Oct 2020 09:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN102620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 27 11:36:24 2020

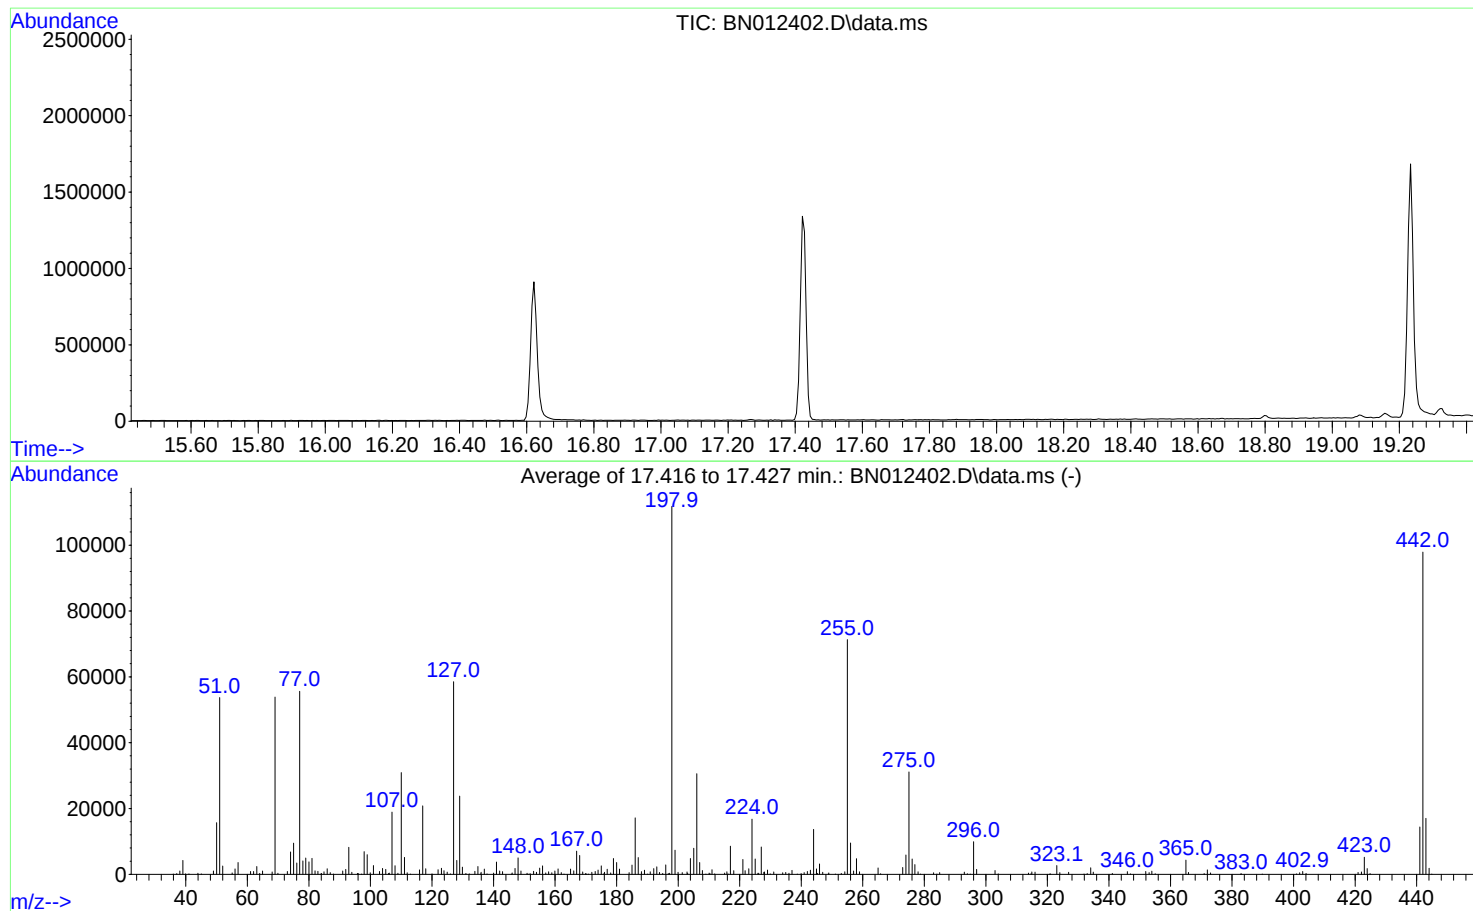

AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.1	53720	PASS
68	69	0.00	2	1.3	722	PASS
69	198	0.00	100	48.2	53872	PASS
70	69	0.00	2	0.6	342	PASS
127	198	10	80	52.4	58549	PASS
197	198	0.00	2	0.3	344	PASS
198	198	100	100	100.0	111749	PASS
199	198	5	9	6.6	7330	PASS
275	198	10	60	27.8	31109	PASS
365	198	1	100	3.9	4339	PASS
441	198	0.01	100	12.9	14370	PASS
442	442	100	100	100.0	97899	PASS
443	442	15	24	17.4	17038	PASS