

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102721\
 Data File : BN017162.D
 Acq On : 28 Oct 2021 19:00
 Operator : CG/JU
 Sample : M4205-02
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AZ8

Quant Time: Oct 29 02:49:53 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 28 12:50:34 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.531	152	5313	0.400	ng/ul	0.00
4) Naphthalene-d8	10.306	136	19839	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.180	164	12279	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.936	188	26552	0.400	ng/ul	0.00
17) Chrysene-d12	21.148	240	25535	0.400	ng/ul	0.00
23) Perylene-d12	23.348	264	26249	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.063	96	176	0.030	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.906	152	4058	0.140	ng/ul	0.00
18) Fluoranthene-d10	18.976	212	11101	0.166	ng/ul	0.00
Target Compounds						
					Qvalue	
19) Fluoranthene	19.009	202	2592	0.028	ng/ul#	93
20) Pyrene	19.371	202	2350	0.025	ng/ul#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102721\
Data File : BN017162.D
Acq On : 28 Oct 2021 19:00
Operator : CG/JU
Sample : M4205-02
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AZ8

Quant Time: Oct 29 02:49:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 28 12:50:34 2021
Response via : Initial Calibration




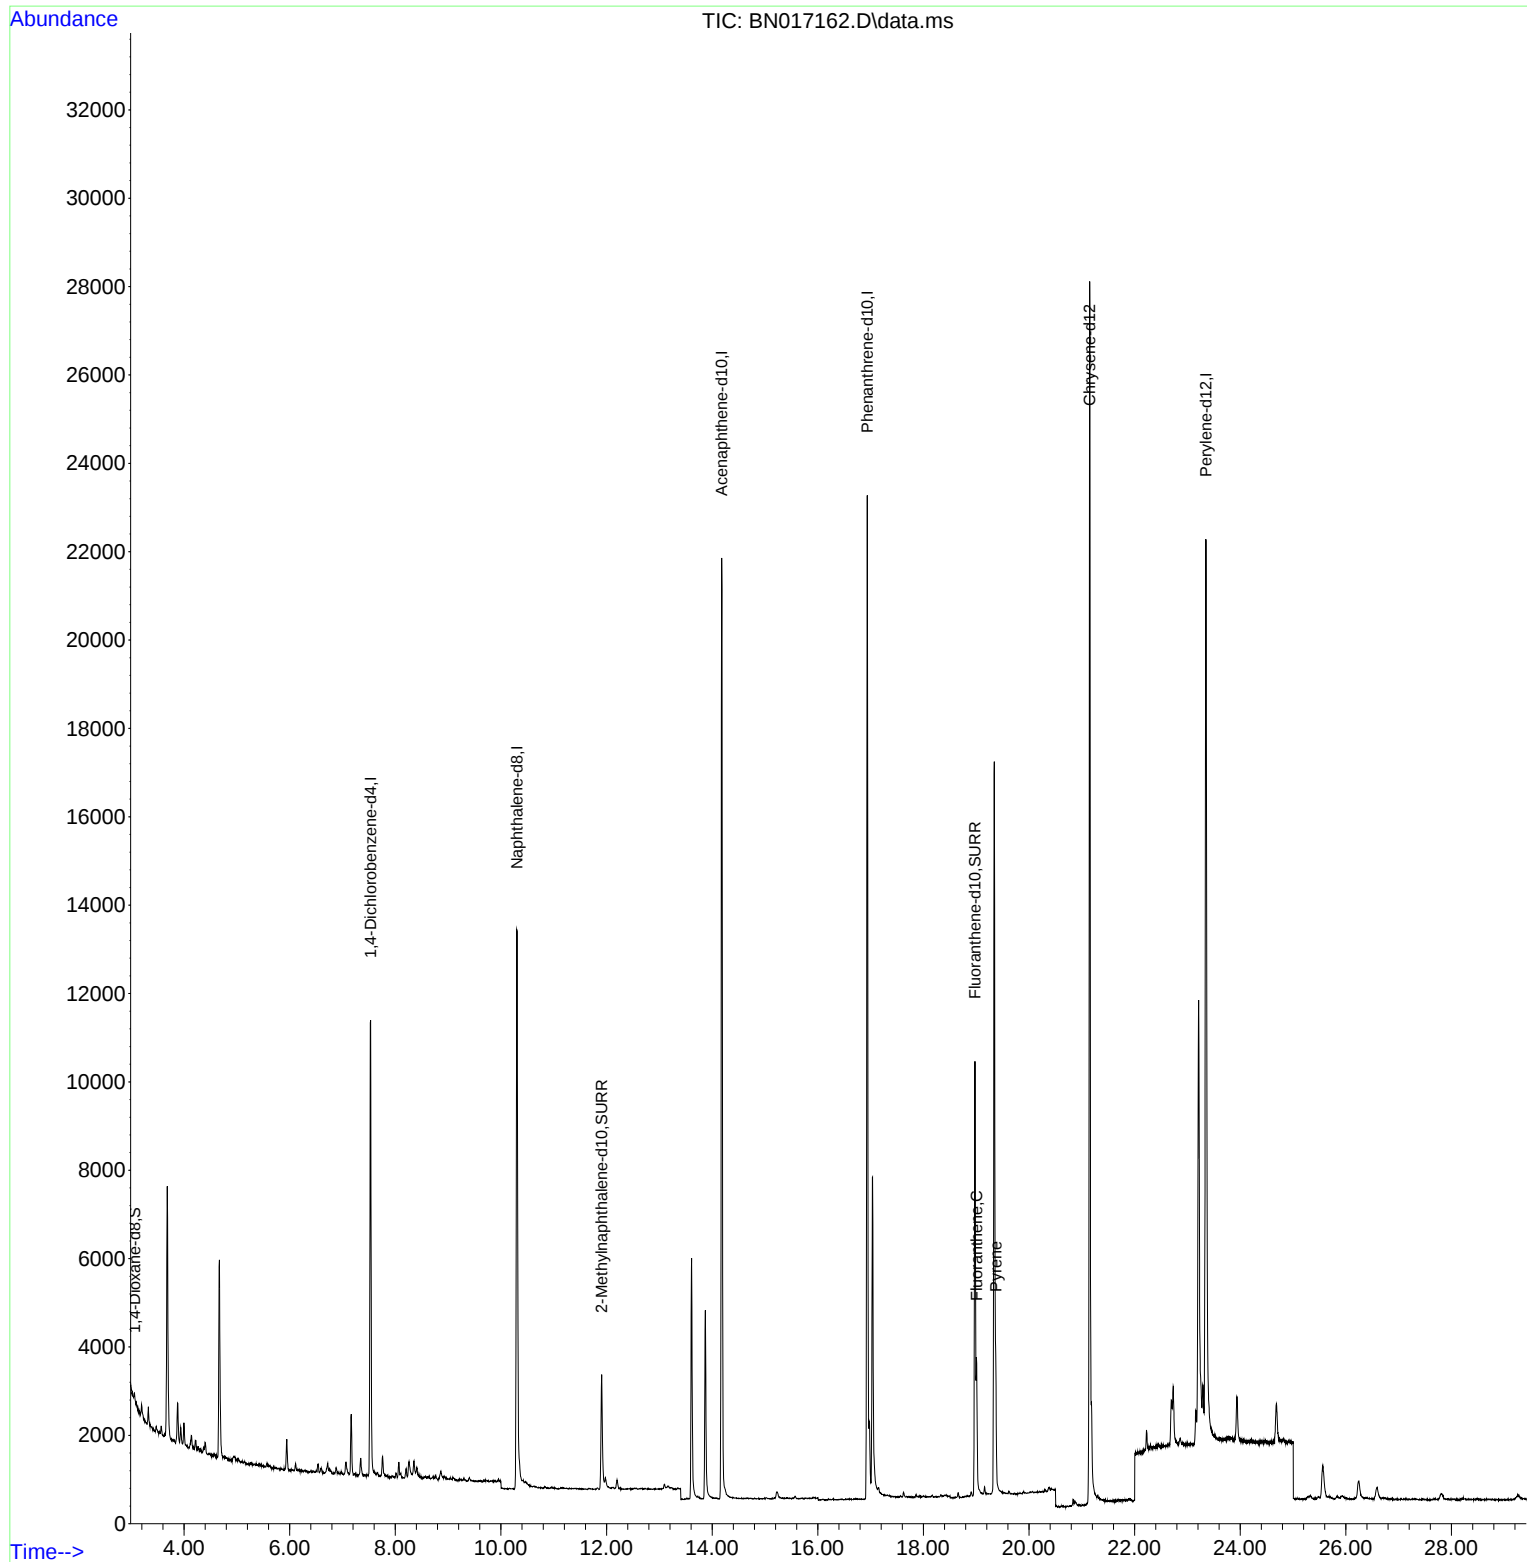


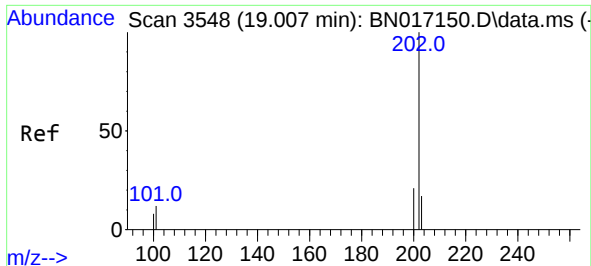

#19
Fluoranthene
Concen: 0.028 ng/u1
RT: 19.009 min Scan# 3548
Delta R.T. 0.001 min
Lab File: BN017162.D
Acq: 28 Oct 2021 19:00

Instrument :
BNA_N
ClientSampleId :
C0AZ8

Tgt Ion:202 Resp: 2592
Ion Ratio Lower Upper
202 100
101 15.2 9.7 14.5#
100 11.1 7.2 10.8#

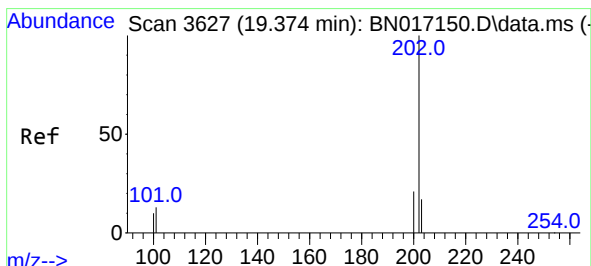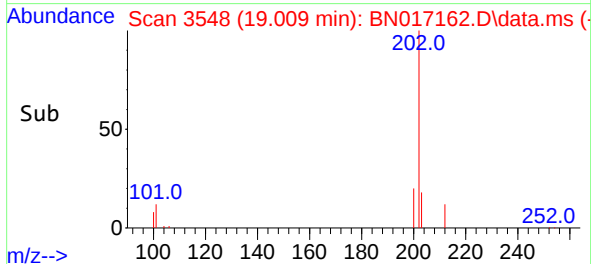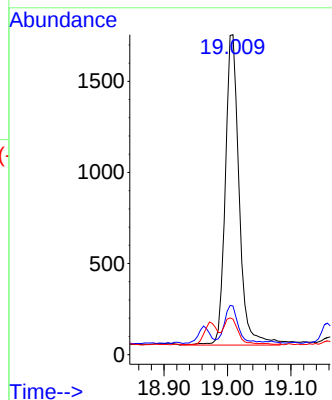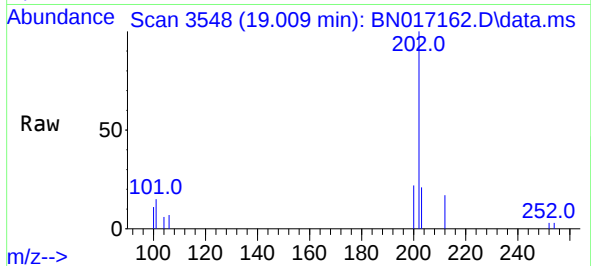

#20
Pyrene
Concen: 0.025 ng/u1
RT: 19.371 min Scan# 3626
Delta R.T. -0.003 min
Lab File: BN017162.D
Acq: 28 Oct 2021 19:00

Tgt Ion:202 Resp: 2350
Ion Ratio Lower Upper
202 100
101 16.2 10.3 15.5#
100 13.0 8.2 12.2#

