


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102722\
 Data File : BN022338.D
 Acq On : 26 Oct 2022 16:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN102722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 27 07:14:22 2022

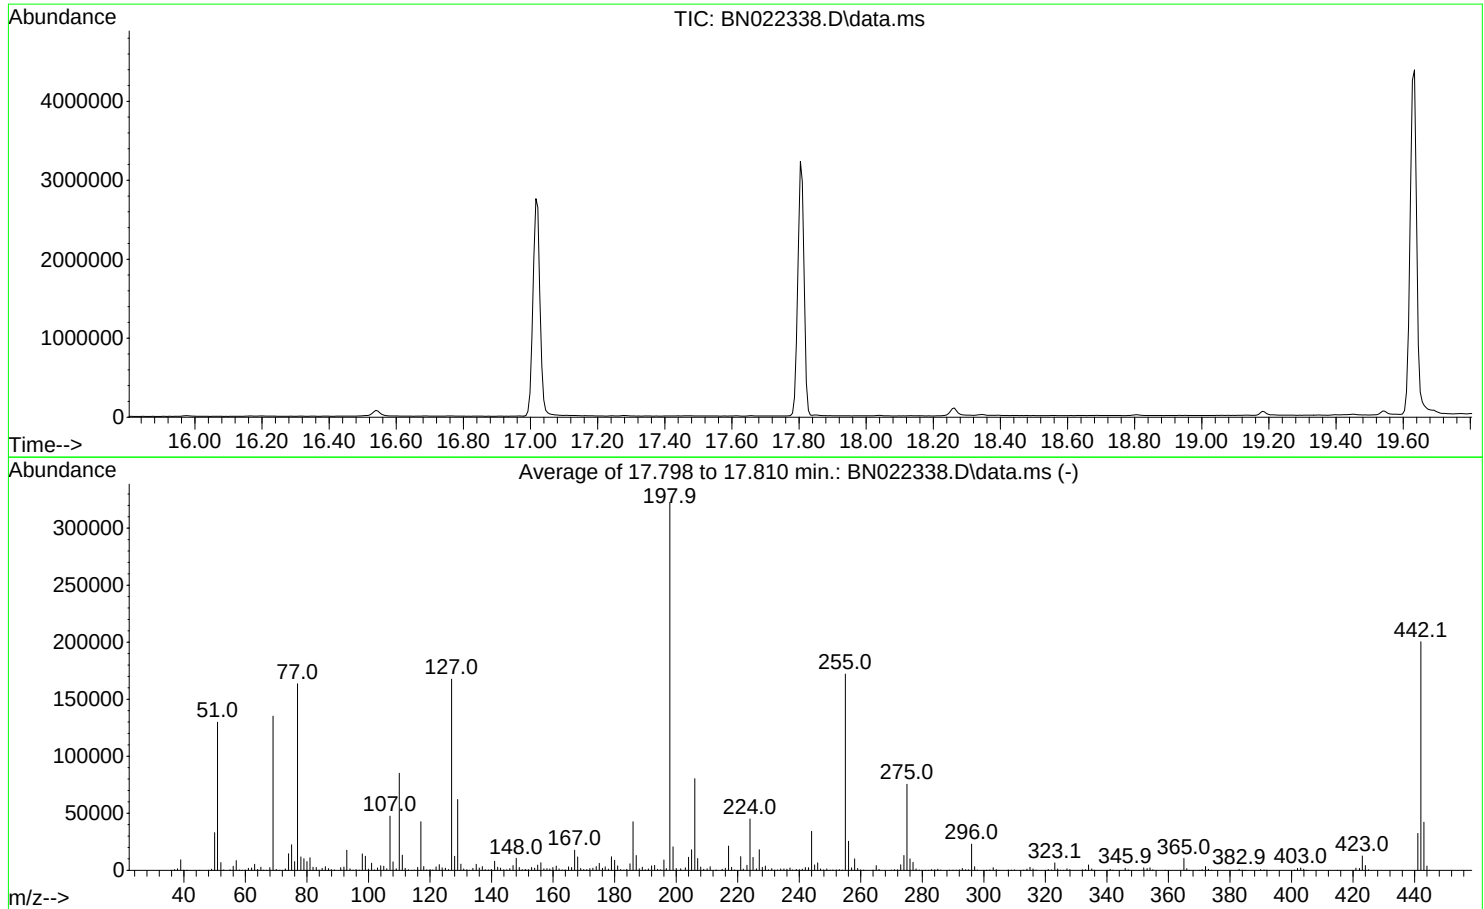

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2511

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	129897	PASS
68	69	0.00	2	1.7	2301	PASS
69	198	0.00	100	41.9	135202	PASS
70	69	0.00	2	0.6	802	PASS
127	198	10	80	52.0	167659	PASS
197	198	0.00	2	0.5	1467	PASS
198	198	100	100	100.0	322603	PASS
199	198	5	9	6.4	20560	PASS
275	198	10	60	23.4	75379	PASS
365	198	1	100	3.2	10431	PASS
441	198	0.01	100	10.0	32299	PASS
442	442	50	100	100.0	200405	PASS
443	442	15	24	21.1	42205	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/27/2022	BNA_N	<u>BN022338.D</u>
Compound Name	Response	Retention Time
DDT	1047380	20.857
DDD	5801	20.469
DDE	290	19.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6091	1053471	0.58

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102722\
 Data File : BN022338.D
 Acq On : 26 Oct 2022 16:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Oct 28 09:00:12 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 28 09:00:04 2022
 Response via : Initial Calibration

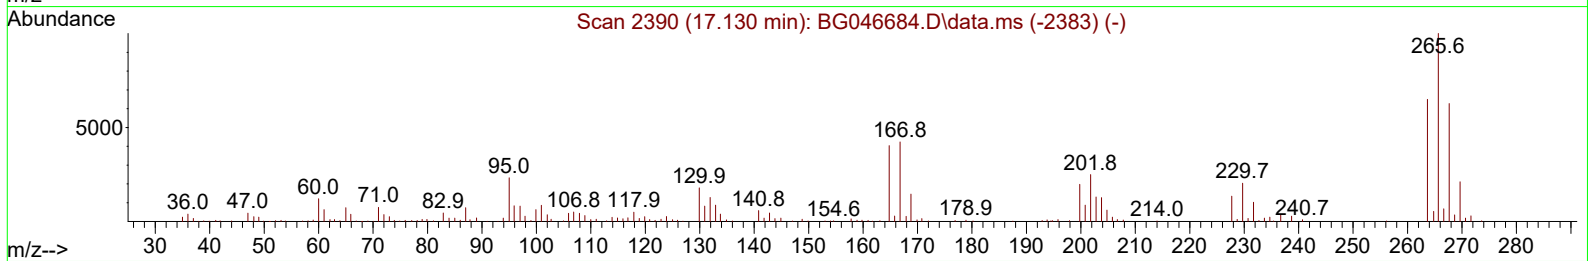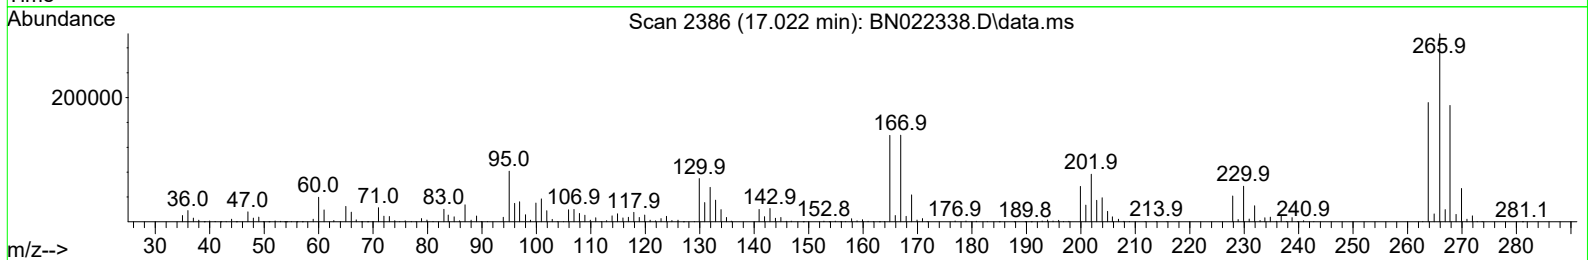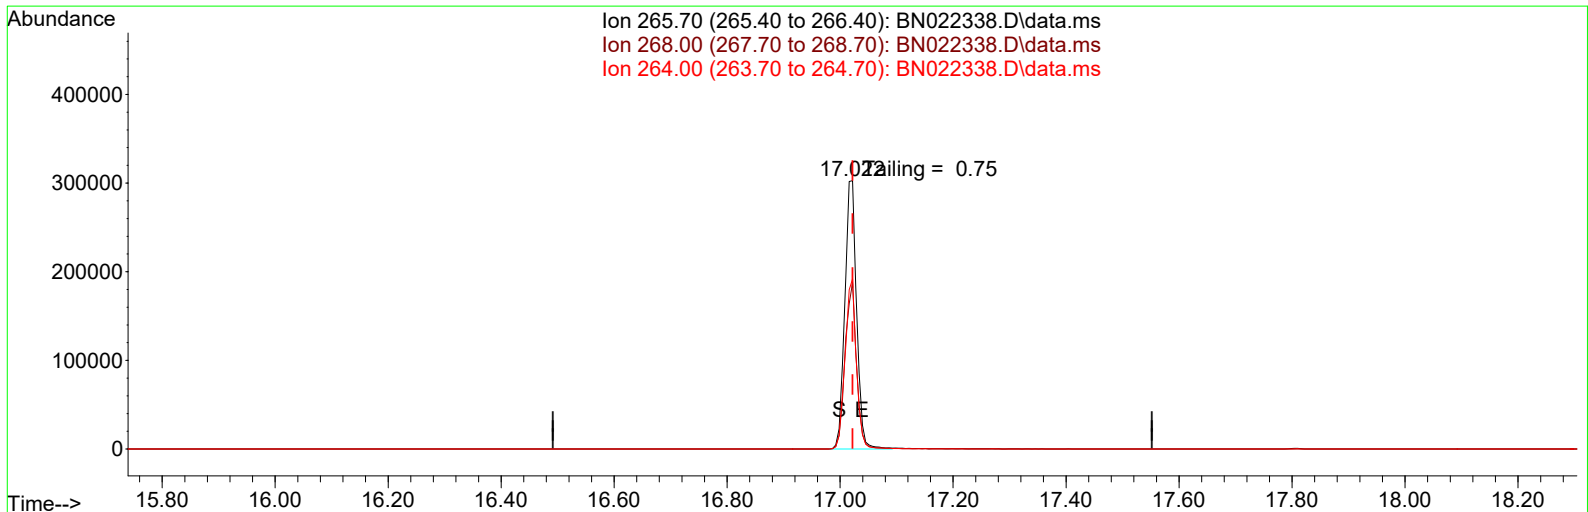

TIC: BN022338.D\data.ms

(70) Pentachlorophenol (C)

17.022min (0.000) 26904.37 ng




response 441280

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.93
264.00	61.60	63.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102722\
Data File : BN022338.D
Acq On : 26 Oct 2022 16:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 28 09:00:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 28 09:00:04 2022
Response via : Initial Calibration

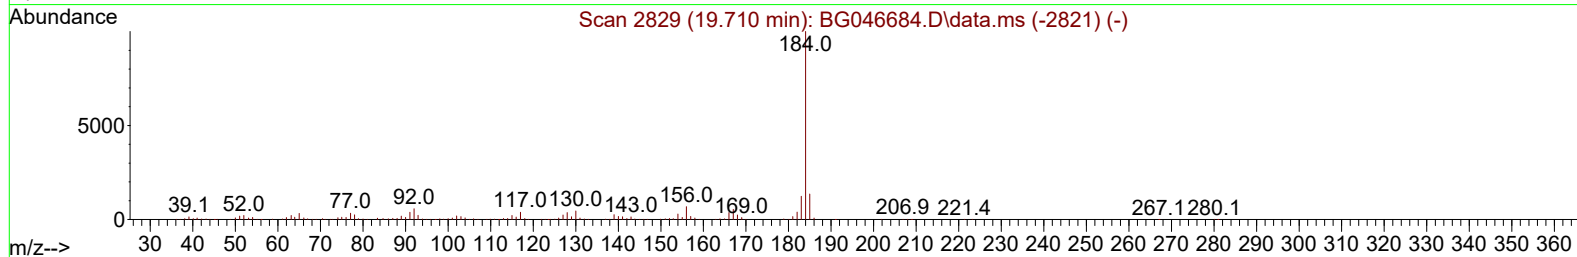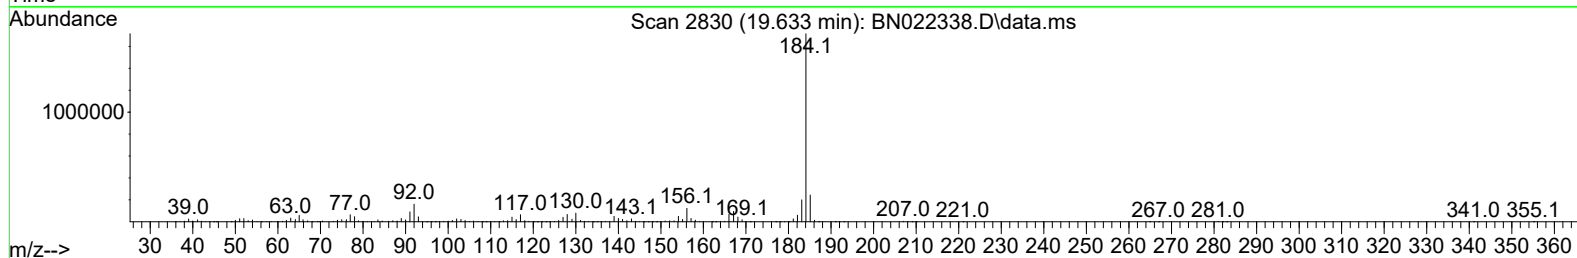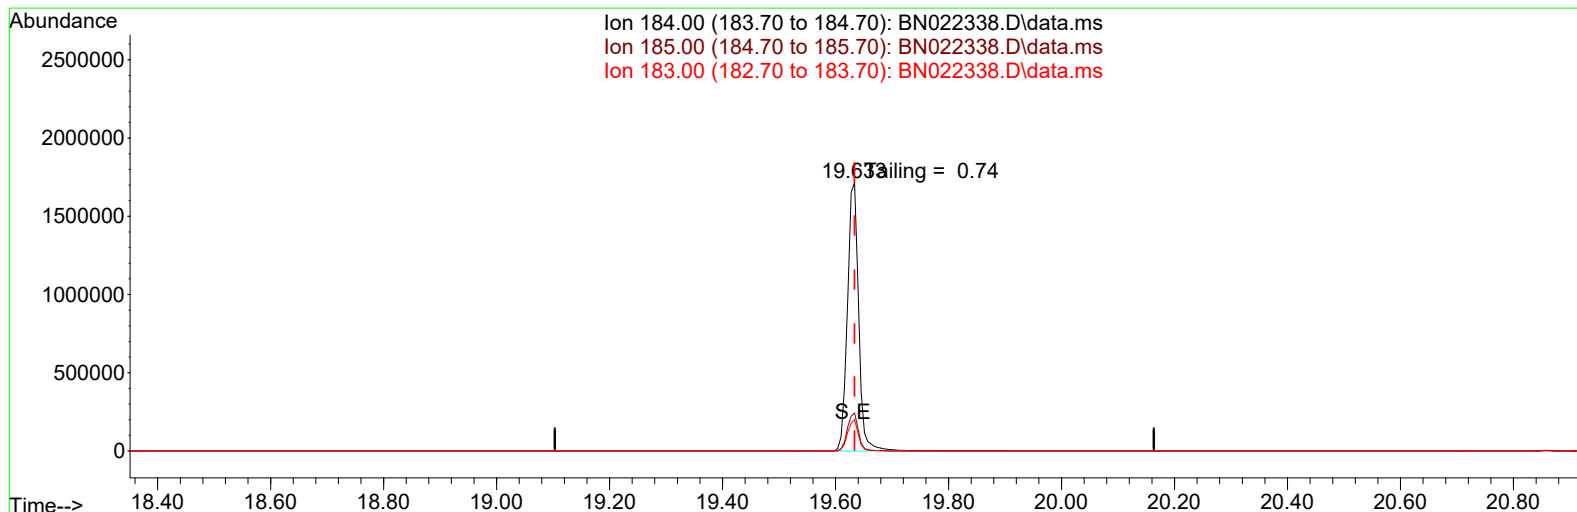

TIC: BN022338.D\data.ms

(77) Benzidine

19.633min (0.000) 0.00 ng

response 2380061

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.21
183.00	13.20	11.69
0.00	0.00	0.00