
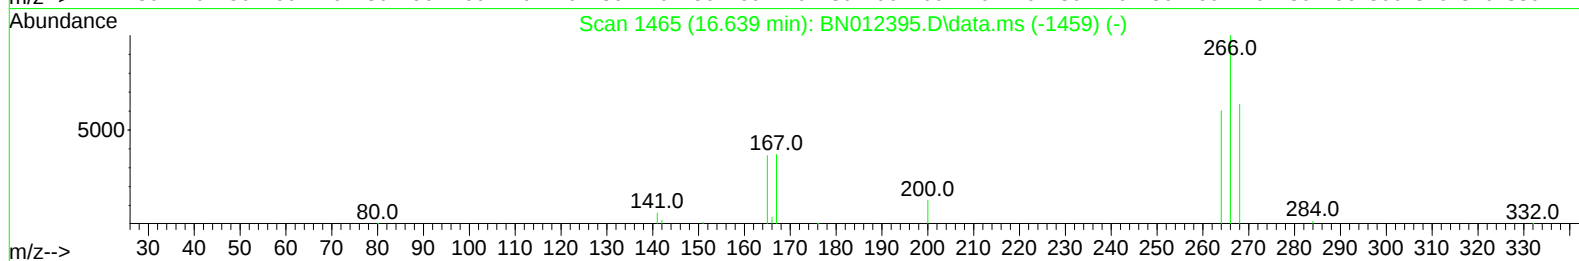
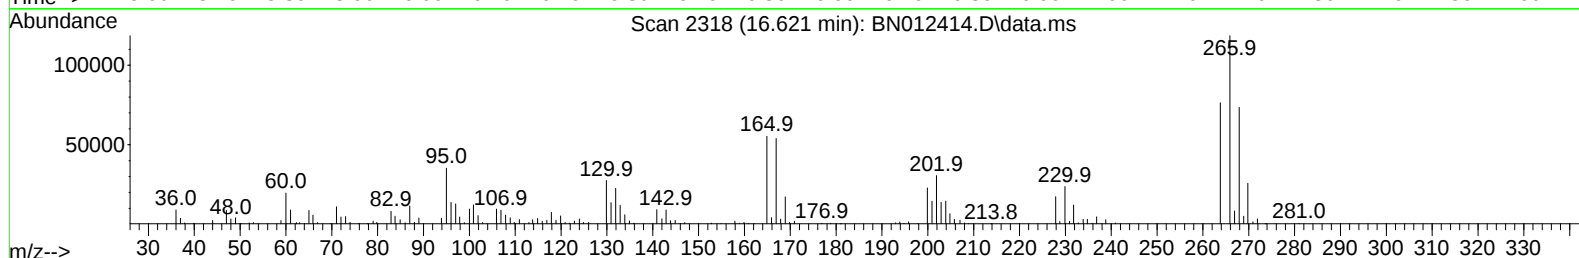


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102820\
Data File : BN012414.D
Acq On : 28 Oct 2020 09:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 29 01:52:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN102620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 28 10:32:42 2020
Response via : Initial Calibration

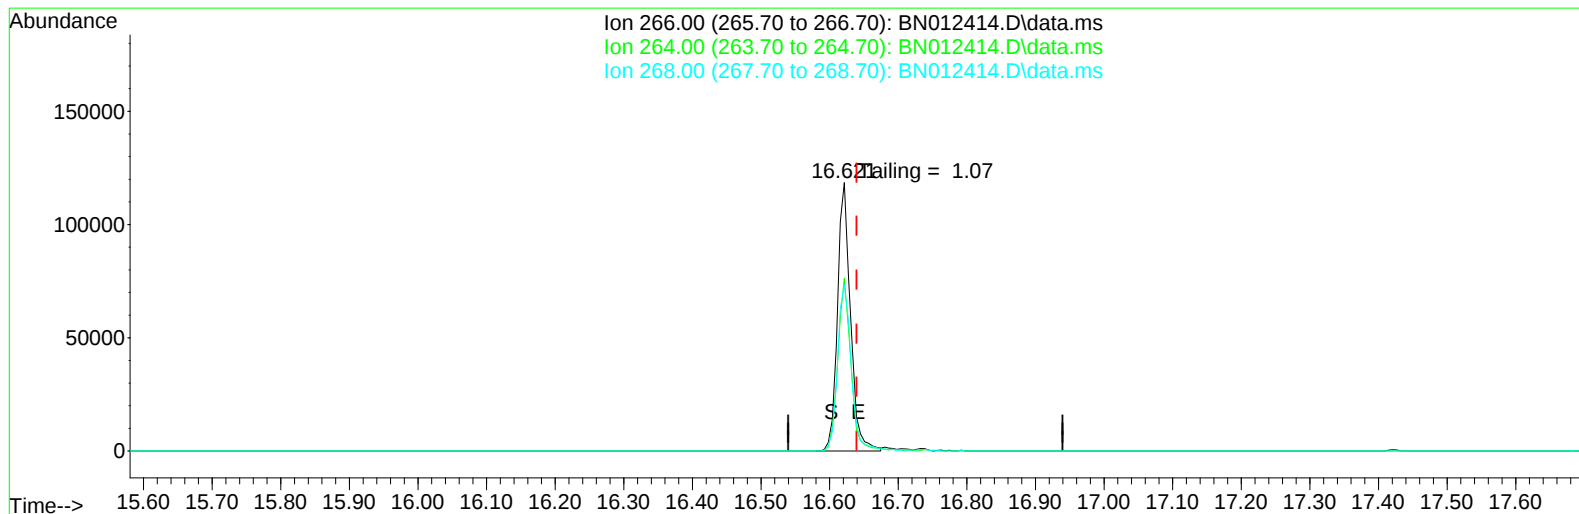

TIC: BN012414.D\data.ms

(24) Pentachlorophenol

16.621min (-0.018) 0.00 ng

response 155730

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	63.60	64.74
268.00	64.40	65.94
0.00	0.00	0.00