

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102820\
 Data File : BN012427.D
 Acq On : 28 Oct 2020 18:22
 Operator : CG/JU
 Sample : L4470-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BP-TT-MW179D-GW-20201015

Quant Time: Oct 29 01:24:43 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN102620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 28 10:32:42 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.578	152	798	0.40	ng	0.00
7) Naphthalene-d8	10.352	136	3121	0.40	ng	0.00
13) Acenaphthene-d10	14.217	164	1802	0.40	ng	0.00
19) Phenanthrene-d10	16.968	188	3746	0.40	ng	# 0.00
29) Chrysene-d12	21.184	240	3978	0.40	ng	# 0.01
36) Perylene-d12	23.354	264	4672	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.194	112	299	0.11	ng	0.00
5) Phenol-d6	6.757	99	217	0.07	ng	0.00
8) Nitrobenzene-d5	8.729	82	1155	0.34	ng	0.00
11) 2-Methylnaphthalene-d10	11.949	152	1403	0.28	ng	0.00
14) 2,4,6-Tribromophenol	15.727	330	449	0.35	ng	0.00
15) 2-Fluorobiphenyl	12.834	172	2588	0.39	ng	-0.01
27) Fluoranthene-d10	19.013	212	3998	0.35	ng	0.00
31) Terphenyl-d14	19.618	244	5299	0.57	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.173	88	384	0.30	ng	# 69
34) Bis(2-ethylhexyl)phtha...	21.099	149	1969	0.25	ng	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102820\
Data File : BN012427.D
Acq On : 28 Oct 2020 18:22
Operator : CG/JU
Sample : L4470-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BP-TT-MW179D-GW-20201015

Quant Time: Oct 29 01:24:43 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN102620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 28 10:32:42 2020
Response via : Initial Calibration




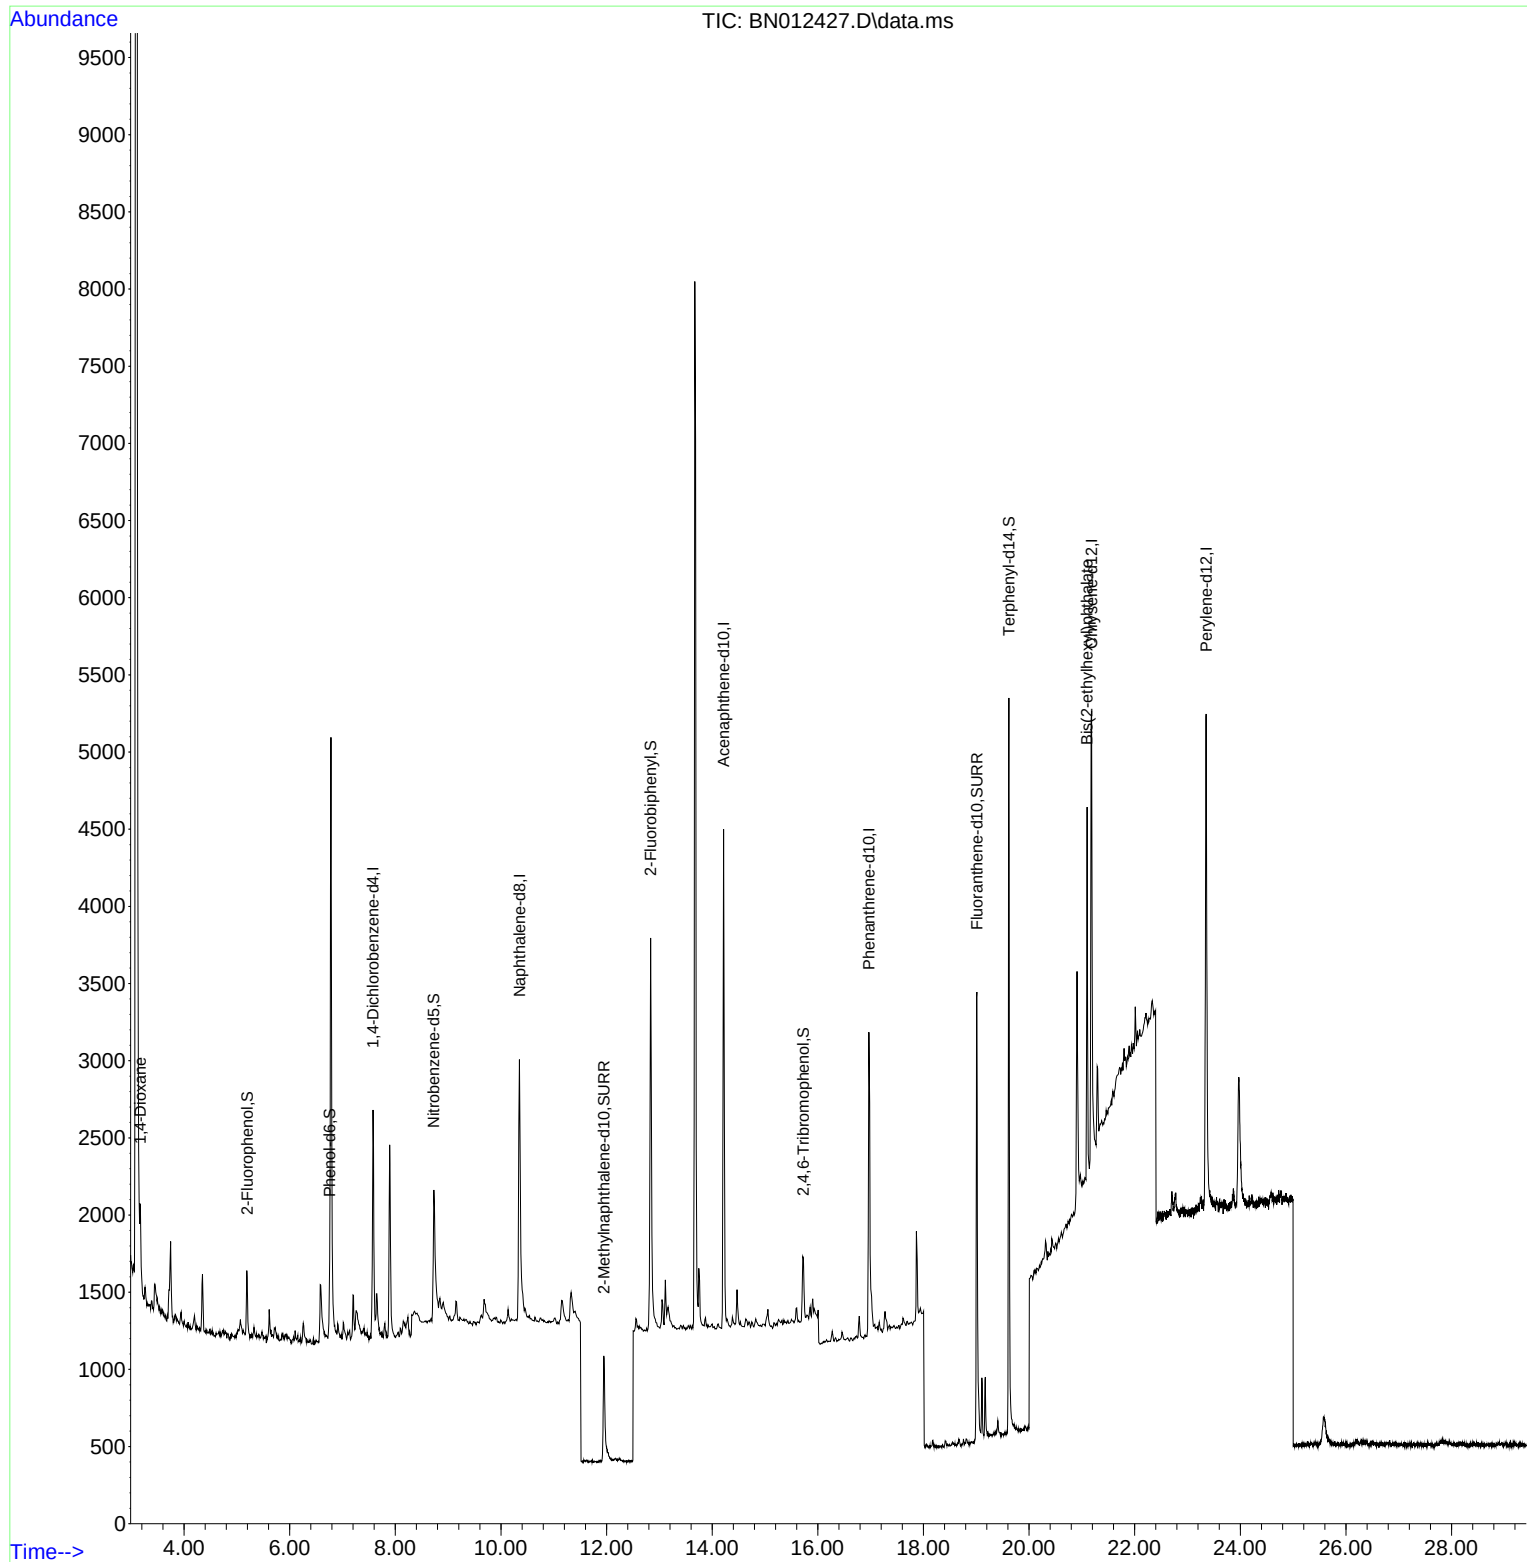




#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.578 min Scan# 571
Delta R.T. 0.000 min
Lab File: BN012427.D
Acq: 28 Oct 2020 18:22




Instrument :
BNA_N
ClientSampleId :
BP-TT-MW179D-GW-20201015


Tgt Ion:152 Resp: 798
Ion Ratio Lower Upper
152 100
150 150.2 116.6 174.8
115 76.4 52.9 79.3

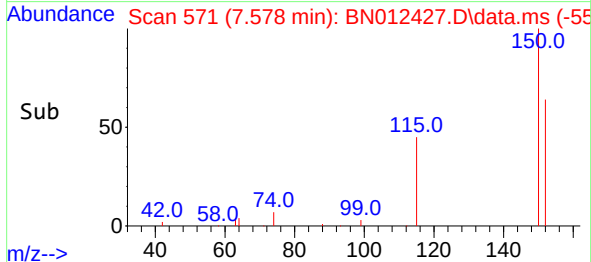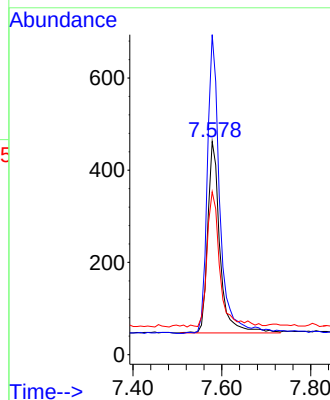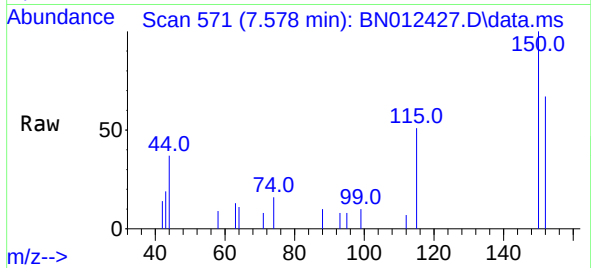

#2
1,4-Dioxane
Concen: 0.30 ng
RT: 3.173 min Scan# 24
Delta R.T. 0.000 min
Lab File: BN012427.D
Acq: 28 Oct 2020 18:22

Tgt Ion: 88 Resp: 384
Ion Ratio Lower Upper
88 100
58 50.3 59.4 89.2#
43 62.8 32.3 48.5#


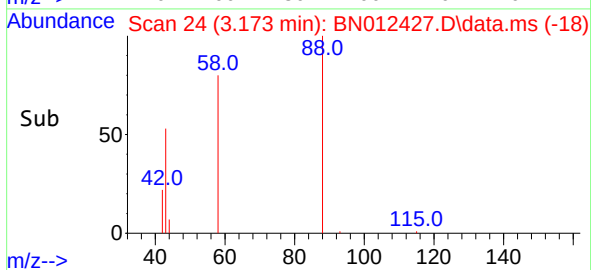
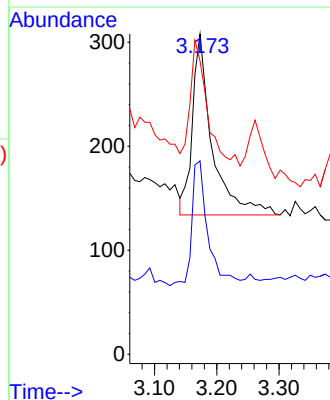





#4
2-Fluorophenol
Concen: 0.11 ng
RT: 5.194 min Scan# 275
Delta R.T. 0.000 min
Lab File: BN012427.D
Acq: 28 Oct 2020 18:22




Instrument :
BNA_N
ClientSampleId :
BP-TT-MW179D-GW-20201015


Tgt Ion:	112	Resp:	299
Ion	Ratio	Lower	Upper
112	100		
64	70.9	49.5	74.3
63	55.9	32.0	48.0

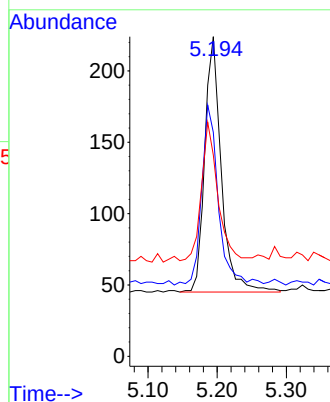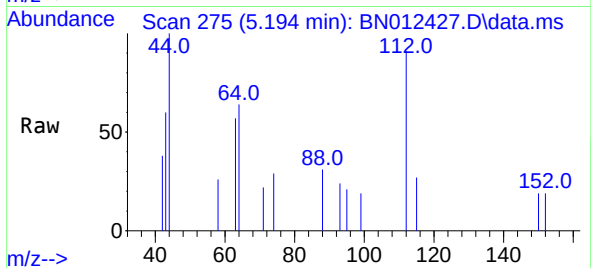

#5
Phenol-d6
Concen: 0.07 ng
RT: 6.757 min Scan# 469
Delta R.T. -0.008 min
Lab File: BN012427.D
Acq: 28 Oct 2020 18:22

Tgt Ion:	99	Resp:	217
Ion	Ratio	Lower	Upper
99	100		
42	0.0	22.4	33.6
71	78.8	37.8	56.6


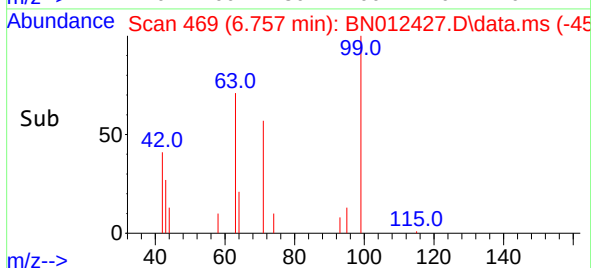
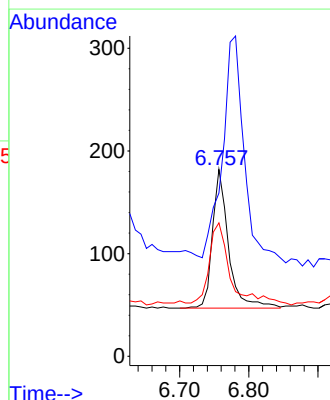





#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.352 min Scan# 823
Delta R.T. 0.000 min
Lab File: BN012427.D
Acq: 28 Oct 2020 18:22




Instrument :
BNA_N
ClientSampleId :
BP-TT-MW179D-GW-20201015


Tgt Ion:	136	Resp:	3121
Ion	Ratio	Lower	Upper
136	100		
137	14.2	10.6	15.8
54	12.1	8.6	12.8
68	7.0	5.7	8.5

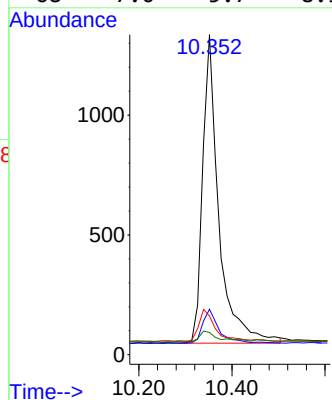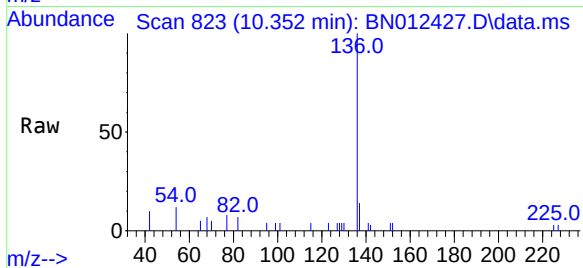

#8
Nitrobenzene-d5
Concen: 0.34 ng
RT: 8.729 min Scan# 695
Delta R.T. 0.000 min
Lab File: BN012427.D
Acq: 28 Oct 2020 18:22

Tgt Ion:	82	Resp:	1155
Ion	Ratio	Lower	Upper
82	100		
128	37.8	30.6	46.0
54	76.6	48.3	72.5


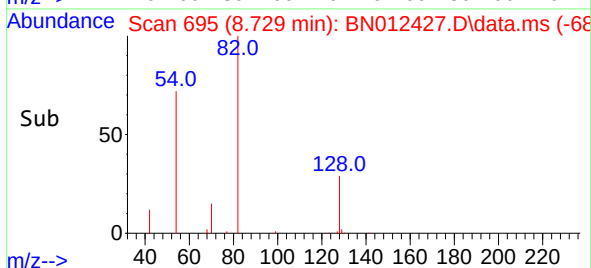
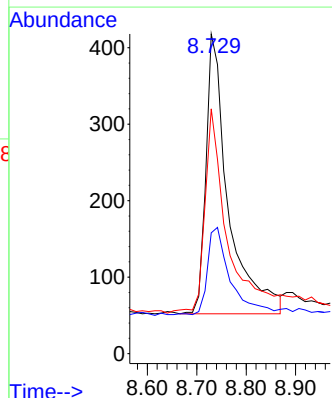
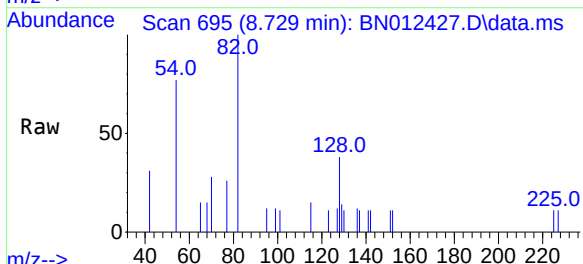




#11
2-Methylnaphthalene-d10
Concen: 0.28 ng
RT: 11.949 min Scan# 1012
Delta R.T. -0.004 min
Lab File: BN012427.D
Acq: 28 Oct 2020 18:22




Instrument :
BNA_N
ClientSampleId :
BP-TT-MW179D-GW-20201015


Tgt Ion:152 Resp: 1403
Ion Ratio Lower Upper
152 100
151 20.4 16.7 25.1

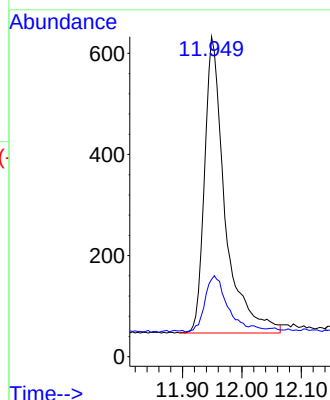

#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.217 min Scan# 1272
Delta R.T. 0.000 min
Lab File: BN012427.D
Acq: 28 Oct 2020 18:22

Tgt Ion:164 Resp: 1802
Ion Ratio Lower Upper
164 100
162 103.6 80.6 120.8
160 49.6 39.5 59.3


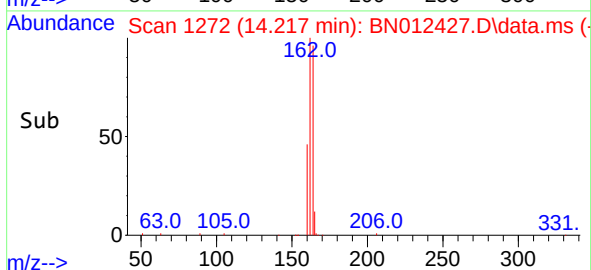
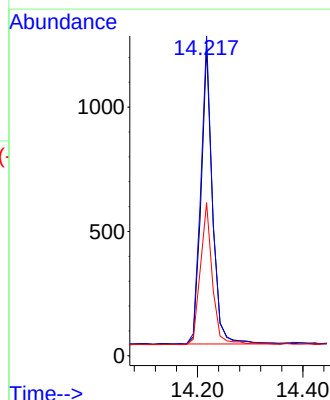





#14
2,4,6-Tribromophenol
Concen: 0.35 ng
RT: 15.727 min Scan# 1391
Delta R.T. 0.000 min
Lab File: BN012427.D
Acq: 28 Oct 2020 18:22




Instrument :
BNA_N
ClientSampleId :
BP-TT-MW179D-GW-20201015


Tgt Ion:330 Resp: 449
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 43.4 34.4 51.6

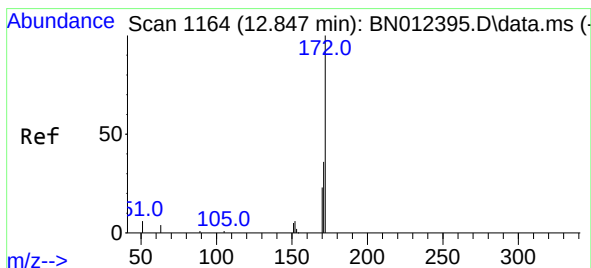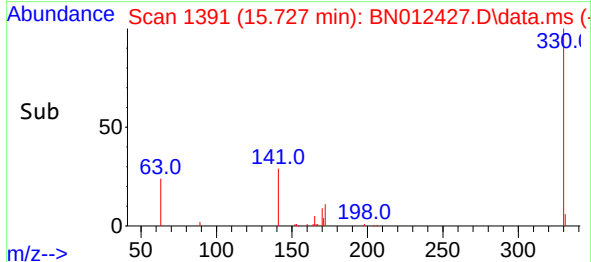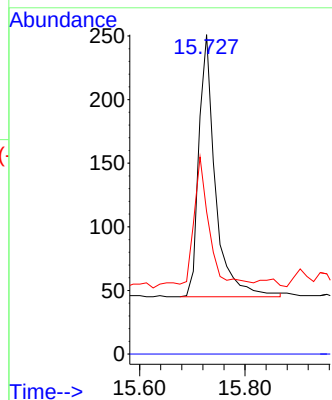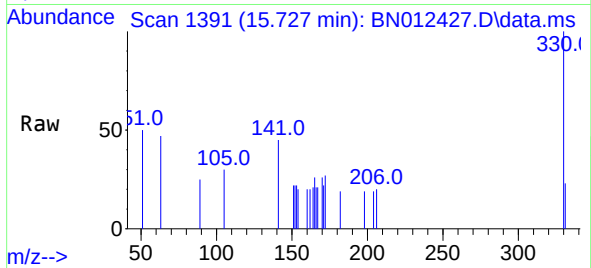

#15
2-Fluorobiphenyl
Concen: 0.39 ng
RT: 12.834 min Scan# 1163
Delta R.T. -0.013 min
Lab File: BN012427.D
Acq: 28 Oct 2020 18:22

Tgt Ion:172 Resp: 2588
Ion Ratio Lower Upper
172 100
171 37.6 28.2 42.4
170 27.9 20.0 30.0


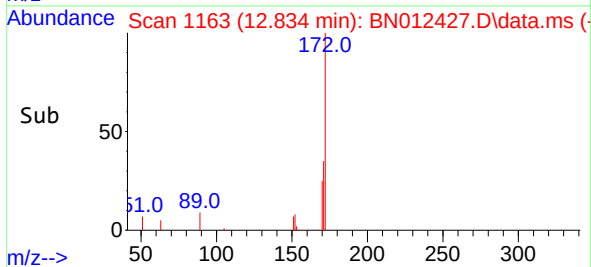
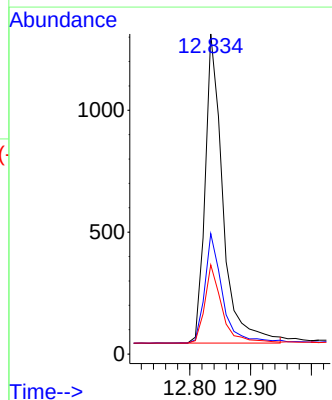
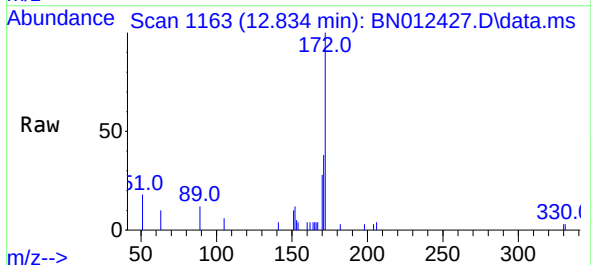




#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 16.968 min Scan# 1492
Delta R.T. 0.000 min
Lab File: BN012427.D
Acq: 28 Oct 2020 18:22




Instrument :
BNA_N
ClientSampleId :
BP-TT-MW179D-GW-20201015


Tgt Ion:188	Resp:	3746
Ion Ratio	Lower	Upper
188	100	
94	0.0	0.0
80	10.4	5.0

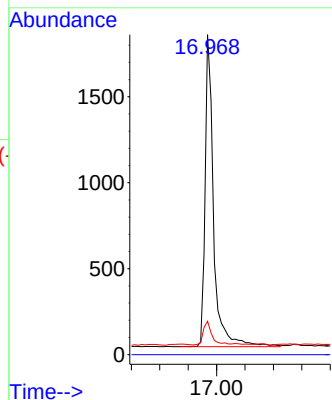

#27
Fluoranthene-d10
Concen: 0.35 ng
RT: 19.013 min Scan# 1779
Delta R.T. 0.000 min
Lab File: BN012427.D
Acq: 28 Oct 2020 18:22

Tgt Ion:212	Resp:	3998
Ion Ratio	Lower	Upper
212	100	
106	8.2	6.8
104	5.2	4.1


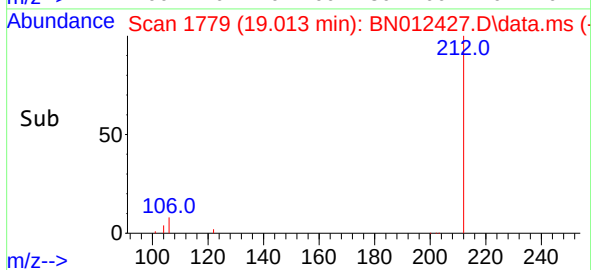
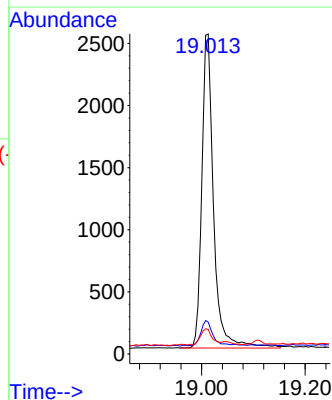





#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.184 min Scan# 2090
Delta R.T. 0.011 min
Lab File: BN012427.D
Acq: 28 Oct 2020 18:22




Instrument :
BNA_N
ClientSampleId :
BP-TT-MW179D-GW-20201015


Tgt Ion:240 Resp: 3978
Ion Ratio Lower Upper
240 100
120 10.5 5.3 7.9#
236 28.5 21.8 32.8

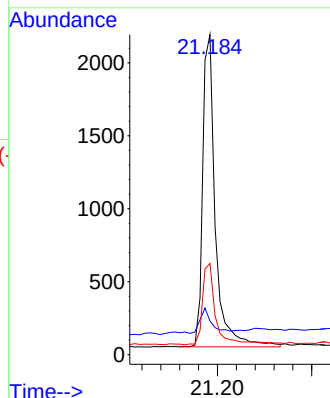

#31
Terphenyl-d14
Concen: 0.57 ng
RT: 19.618 min Scan# 1901
Delta R.T. -0.005 min
Lab File: BN012427.D
Acq: 28 Oct 2020 18:22

Tgt Ion:244 Resp: 5299
Ion Ratio Lower Upper
244 100
212 10.0 7.3 10.9
122 10.4 7.3 10.9

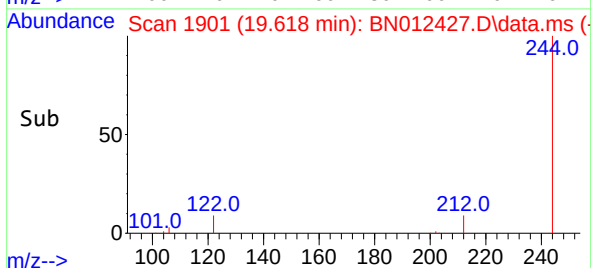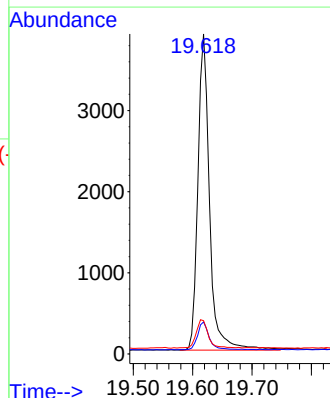




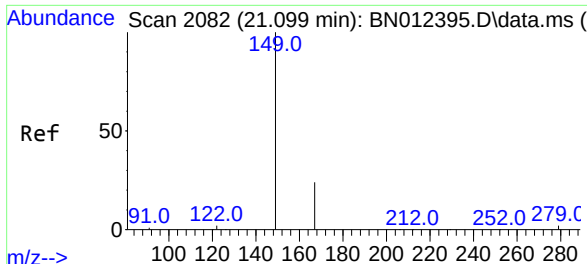


#34
Bis(2-ethylhexyl)phthalate
Concen: 0.25 ng
RT: 21.099 min Scan# 2082
Delta R.T. 0.000 min
Lab File: BN012427.D
Acq: 28 Oct 2020 18:22

Instrument :
BNA_N
ClientSampleId :
BP-TT-MW179D-GW-20201015

Tgt Ion:149 Resp: 1969

Ion	Ratio	Lower	Upper
149	100		
167	23.9	23.2	34.8
279	4.6	3.9	5.9

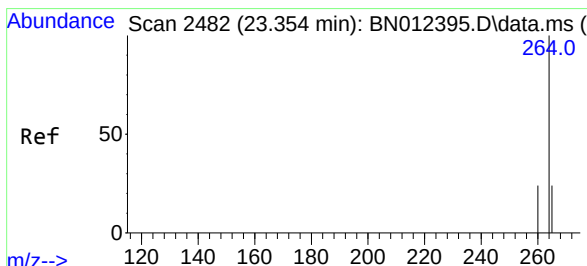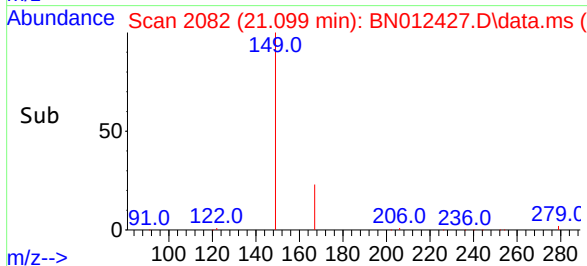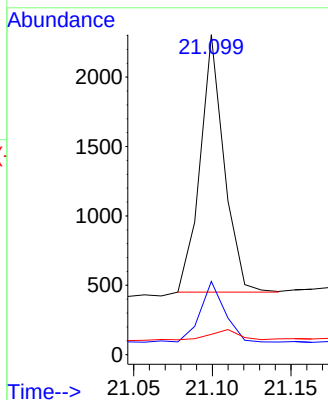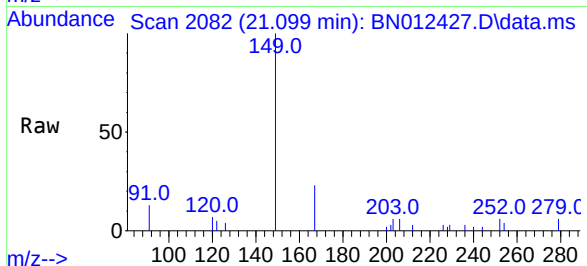

#36
Perylene-d12
Concen: 0.40 ng
RT: 23.354 min Scan# 2482
Delta R.T. 0.000 min
Lab File: BN012427.D
Acq: 28 Oct 2020 18:22

Tgt Ion:264 Resp: 4672

Ion	Ratio	Lower	Upper
264	100		
260	25.2	19.8	29.6
265	69.2	51.4	77.0

