


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN102820\  
 Data File : BN012414.D  
 Acq On : 28 Oct 2020 09:09  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\8270-SIM-BN102620.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Oct 28 10:32:42 2020

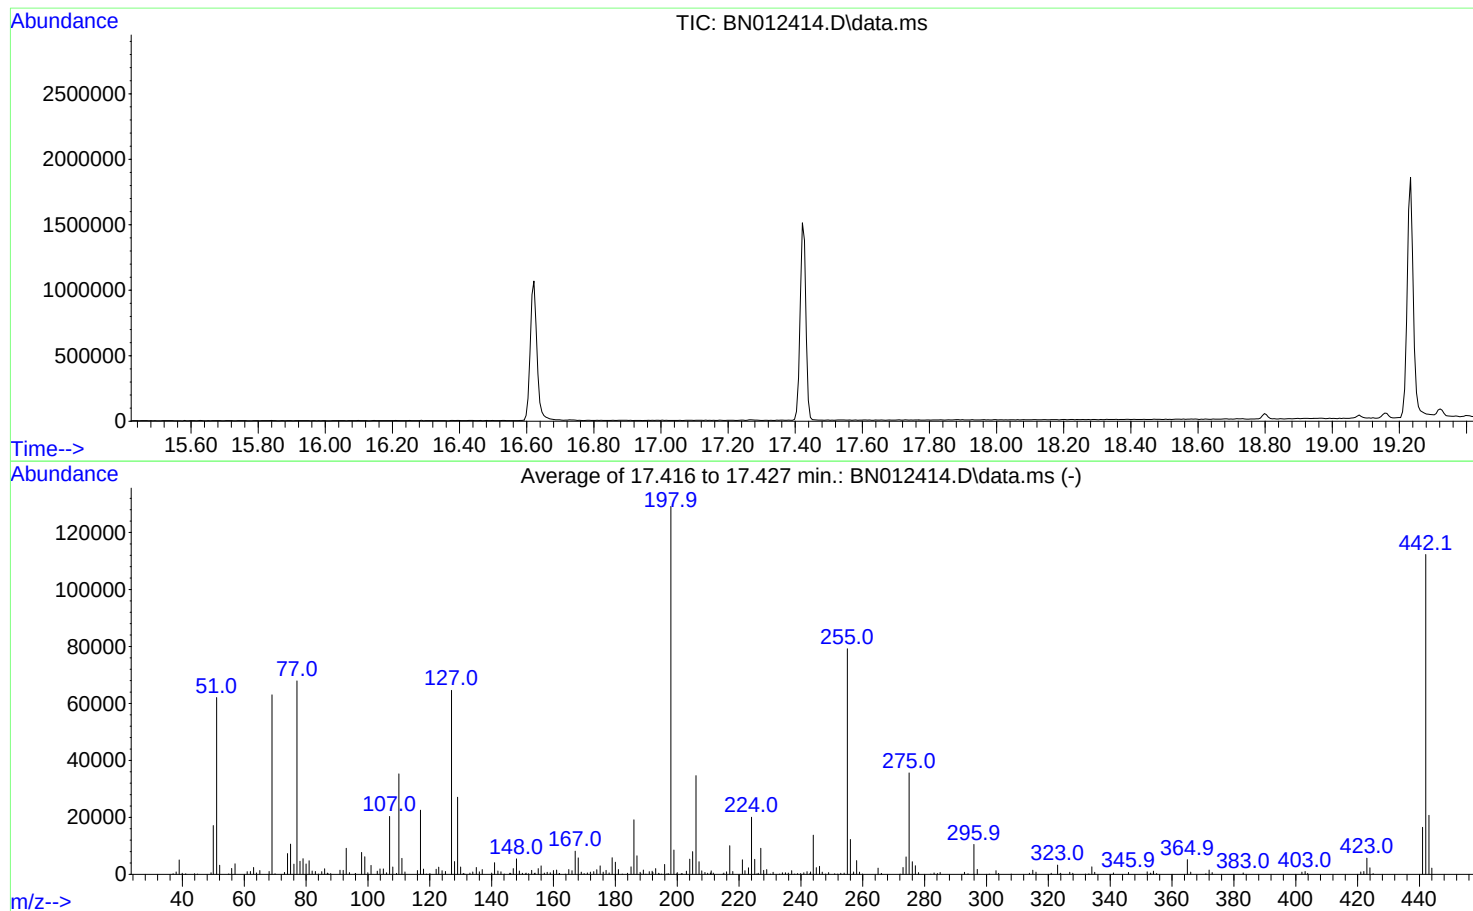

AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2447

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 48.1         | 62051      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.6          | 1032       | PASS                |
| 69             | 198             | 0.00            | 100             | 48.8         | 63045      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.4          | 228        | PASS                |
| 127            | 198             | 10              | 80              | 50.0         | 64619      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.2          | 249        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 129133     | PASS                |
| 199            | 198             | 5               | 9               | 6.6          | 8567       | PASS                |
| 275            | 198             | 10              | 60              | 27.6         | 35592      | PASS                |
| 365            | 198             | 1               | 100             | 4.0          | 5161       | PASS                |
| 441            | 198             | 0.01            | 100             | 12.8         | 16506      | PASS                |
| 442            | 198             | 50              | 100             | 86.9         | 112272     | PASS                |
| 443            | 442             | 15              | 24              | 18.5         | 20728      | PASS                |