

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102920\
 Data File : BN012446.D
 Acq On : 29 Oct 2020 19:58
 Operator : CG/JU
 Sample : L4561-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 STOCKPILE-LOC3-SO-0003

Manual Integrations
 APPROVED

mohammad
 10/30/2020 12:09:54 PM

Quant Time: Oct 30 00:55:38 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN102620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 28 10:32:42 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.578	152	1189	0.40	ng	0.00
7) Naphthalene-d8	10.339	136	4893	0.40	ng	#-0.01
13) Acenaphthene-d10	14.217	164	2663	0.40	ng	0.00
19) Phenanthrene-d10	16.968	188	5363	0.40	ng	# 0.00
29) Chrysene-d12	21.174	240	6491	0.40	ng	# 0.00
36) Perylene-d12	23.343	264	7254	0.40	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.186	112	1148	0.28	ng	0.00
5) Phenol-d6	6.757	99	1537	0.31	ng	0.00
8) Nitrobenzene-d5	8.729	82	1963	0.36	ng	0.00
11) 2-Methylnaphthalene-d10	11.940	152	2310	0.29	ng	-0.01
14) 2,4,6-Tribromophenol	15.714	330	534	0.28	ng	-0.01
15) 2-Fluorobiphenyl	12.834	172	3660	0.37	ng	-0.01
27) Fluoranthene-d10	19.008	212	5194	0.31	ng	0.00
31) Terphenyl-d14	19.613	244	5848	0.38	ng	0.00
Target Compounds						Qvalue
9) Naphthalene	10.390	128	1486	0.11	ng	# 91
12) 2-Methylnaphthalene	12.015	142	284	0.03	ng	# 77
16) Acenaphthylene	13.938	152	991	0.08	ng	# 93
17) Acenaphthene	14.281	154	1938	0.23	ng	91
18) Fluorene	15.270	166	1498	0.14	ng	100
25) Phenanthrene	17.005	178	69932	4.47	ng	99
26) Anthracene	17.102	178	5872	0.41	ng	# 90
28) Fluoranthene	19.037	202	321363	17.27	ng	99
30) Pyrene	19.400	202	281284	12.81	ng	# 95
32) Benzo(a)anthracene	21.152	228	129180	6.54	ng	99
33) Chrysene	21.206	228	178011	8.04	ng	98
34) Bis(2-ethylhexyl)phtha...	21.099	149	5271	0.41	ng	90
35) Indeno(1,2,3-cd)pyrene	25.500	276	175734	5.52	ng	98
37) Benzo(b)fluoranthene	22.700	252	300242	13.12	ng	97
38) Benzo(k)fluoranthene	22.738	252	98214m	3.94	ng	
39) Benzo(a)pyrene	23.251	252	187438	8.44	ng	94
40) Dibenzo(a,h)anthracene	25.507	278	36574	1.46	ng	# 96
41) Benzo(g,h,i)perylene	26.164	276	182374	6.92	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102920\
Data File : BN012446.D
Acq On : 29 Oct 2020 19:58
Operator : CG/JU
Sample : L4561-03
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
STOCKPILE-LOC3-SO-0003

Manual Integrations
APPROVED


mohammad
10/30/2020 12:09:54 PM

Quant Time: Oct 30 00:55:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN102620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 28 10:32:42 2020
Response via : Initial Calibration



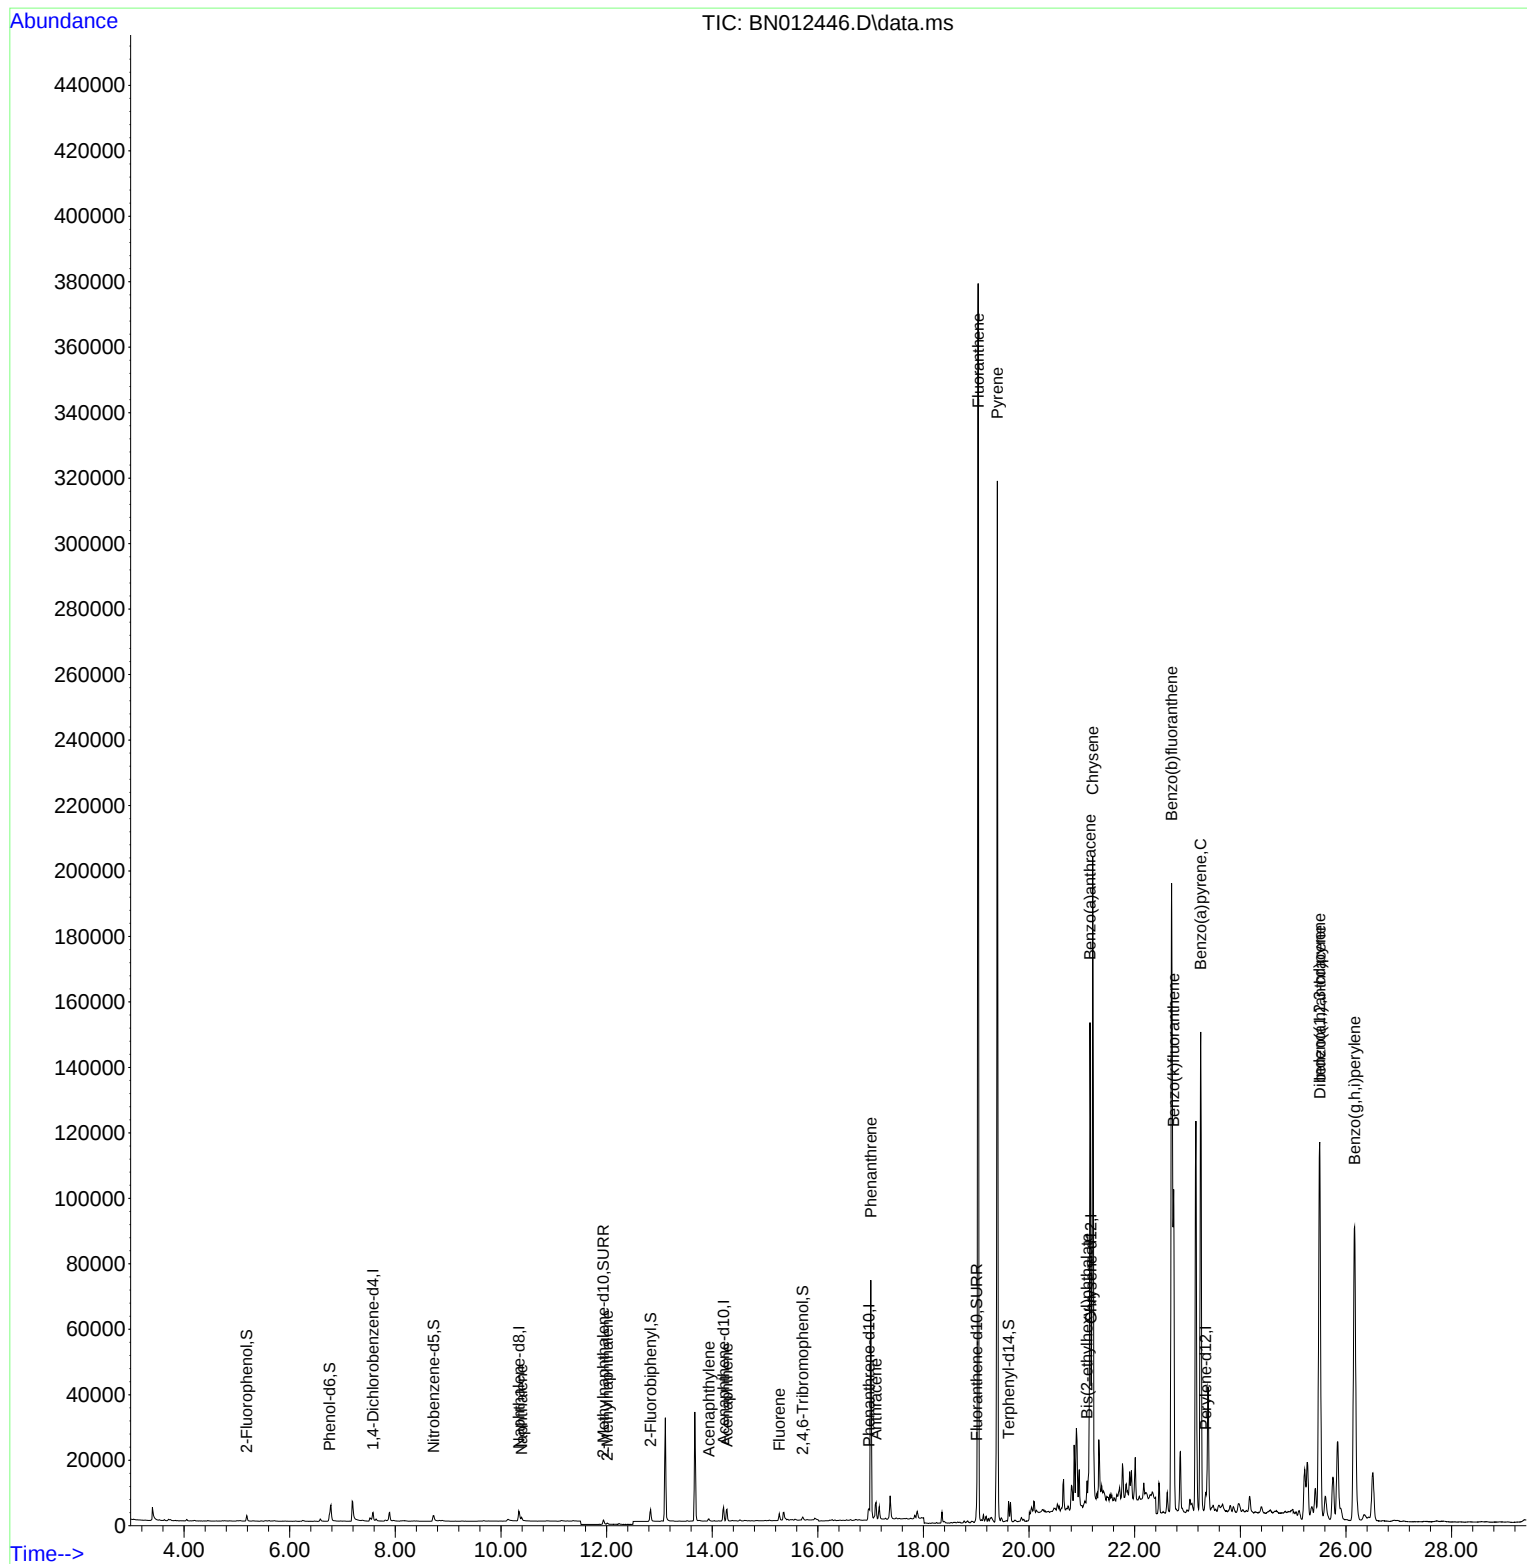


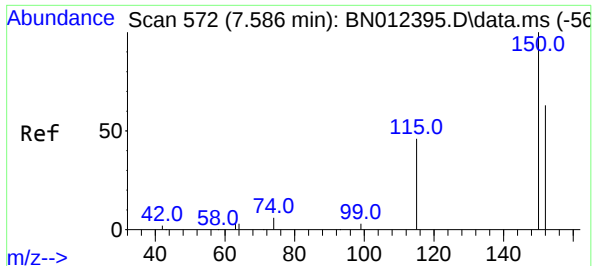


#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.578 min Scan# 571
Delta R.T. 0.000 min
Lab File: BN012446.D
Acq: 29 Oct 2020 19:58

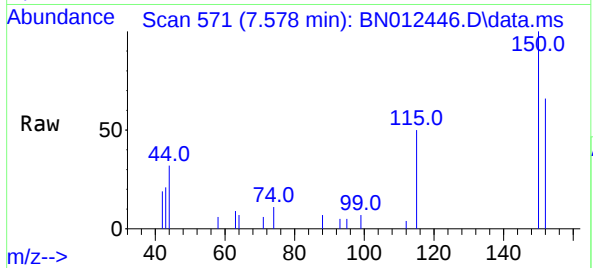



Tgt Ion:152 Resp: 1189
Ion Ratio Lower Upper
152 100
150 150.7 116.6 174.8
115 74.9 52.9 79.3

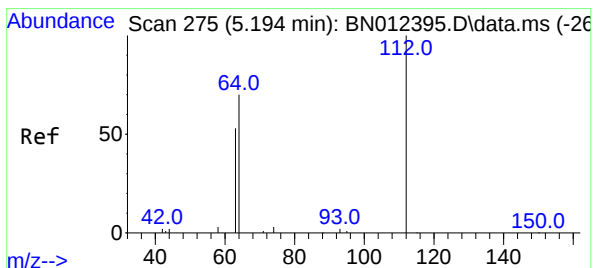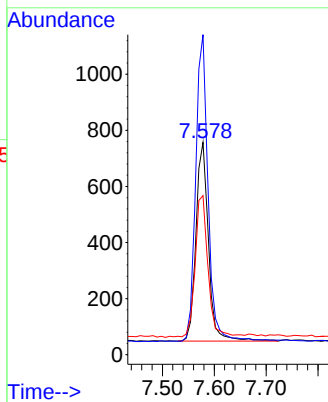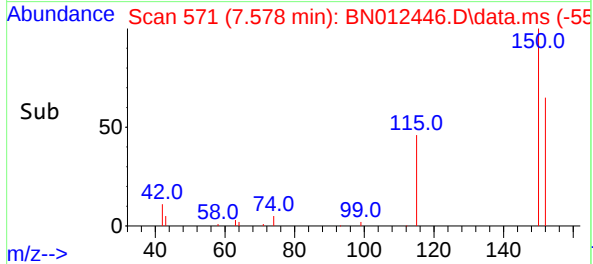

#4
2-Fluorophenol
Concen: 0.28 ng
RT: 5.186 min Scan# 274
Delta R.T. -0.008 min
Lab File: BN012446.D
Acq: 29 Oct 2020 19:58

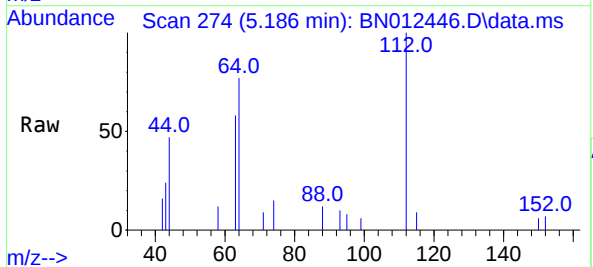


Tgt Ion:112 Resp: 1148
Ion Ratio Lower Upper
112 100
64 71.0 49.5 74.3
63 49.7 32.0 48.0#

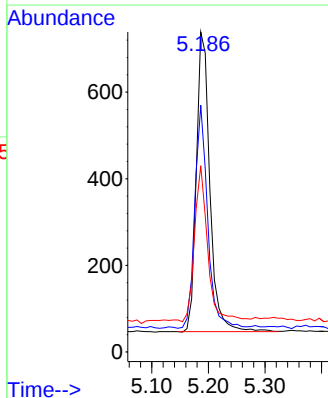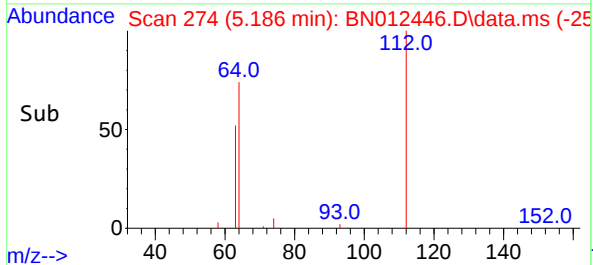


Instrument :
BNA_N
ClientSampleId :
STOCKPILE-LOC3-SO-0003

Manual Integrations
APPROVED

mohammad
10/30/2020 12:09:54 PM






#5
Phenol-d6
Concen: 0.31 ng
RT: 6.757 min Scan# 469
Delta R.T. -0.008 min
Lab File: BN012446.D
Acq: 29 Oct 2020 19:58




Tgt Ion: 99 Resp: 1537

Ion	Ratio	Lower	Upper
99	100		
42	66.6	22.4	33.6#
71	57.2	37.8	56.6#

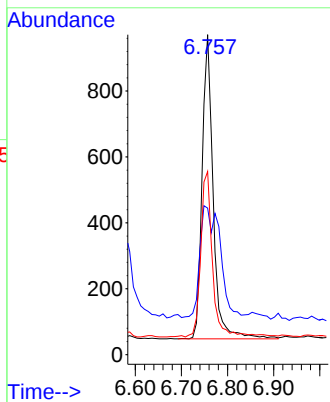



#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.339 min Scan# 822
Delta R.T. -0.013 min
Lab File: BN012446.D
Acq: 29 Oct 2020 19:58

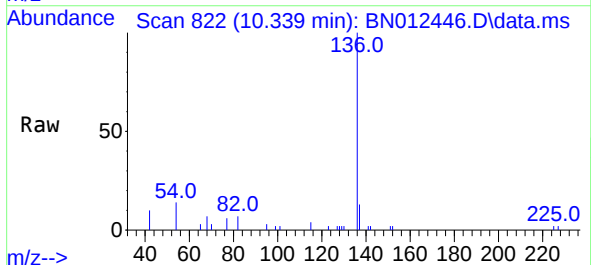

Tgt Ion: 136 Resp: 4893


Ion	Ratio	Lower	Upper
136	100		
137	13.0	10.6	15.8
54	13.5	8.6	12.8#
68	7.1	5.7	8.5

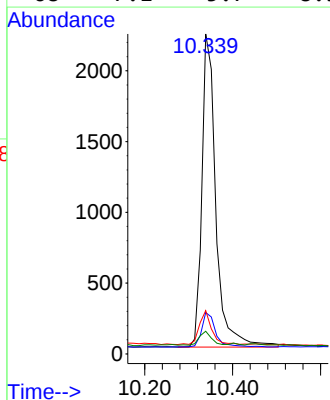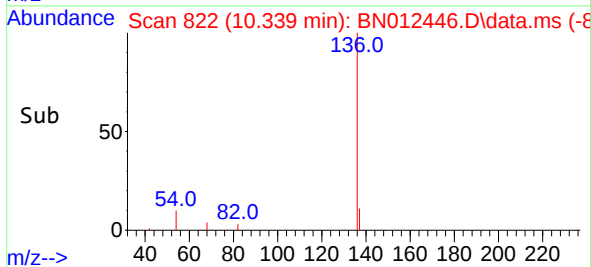


Instrument :
BNA_N
ClientSampleId :
STOCKPILE-LOC3-SO-0003

Manual Integrations
APPROVED

mohammad
10/30/2020 12:09:54 PM






#8
Nitrobenzene-d5
Concen: 0.36 ng
RT: 8.729 min Scan# 695
Delta R.T. 0.000 min
Lab File: BN012446.D
Acq: 29 Oct 2020 19:58




Tgt Ion: 82 Resp: 1963

Ion	Ratio	Lower	Upper
82	100		
128	42.2	30.6	46.0
54	62.5	48.3	72.5

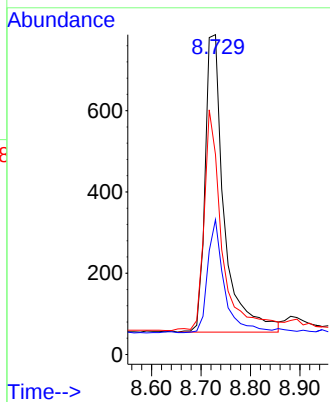



#9
Naphthalene
Concen: 0.11 ng
RT: 10.390 min Scan# 826
Delta R.T. -0.013 min
Lab File: BN012446.D
Acq: 29 Oct 2020 19:58

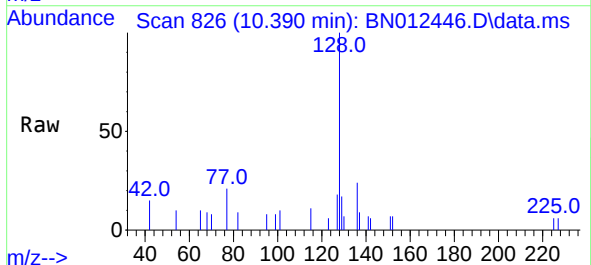

Tgt Ion: 128 Resp: 1486


Ion	Ratio	Lower	Upper
128	100		
129	16.8	9.8	14.8#
127	18.1	12.2	18.4

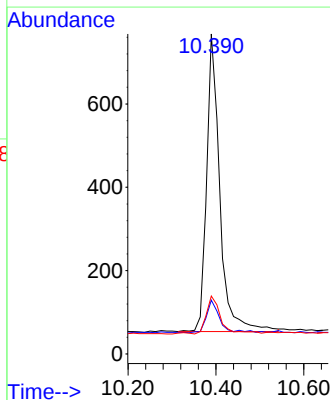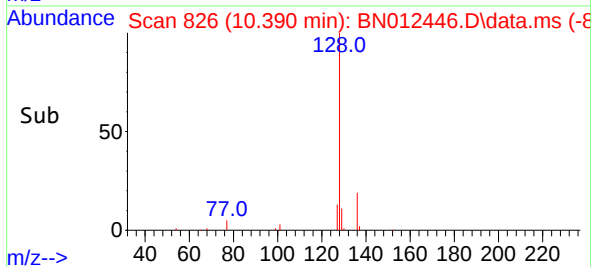

Instrument :
BNA_N
ClientSampleId :
STOCKPILE-LOC3-SO-0003

Manual Integrations
APPROVED

mohammad
10/30/2020 12:09:54 PM







#11
2-Methylnaphthalene-d10
Concen: 0.29 ng
RT: 11.940 min Scan# 1010
Delta R.T. -0.013 min
Lab File: BN012446.D
Acq: 29 Oct 2020 19:58

Tgt Ion:152 Resp: 2310
Ion Ratio Lower Upper
152 100
151 22.6 16.7 25.1

Instrument :
BNA_N
ClientSampleId :
STOCKPILE-LOC3-SO-0003




Manual Integrations
APPROVED


mohammad
10/30/2020 12:09:54 PM

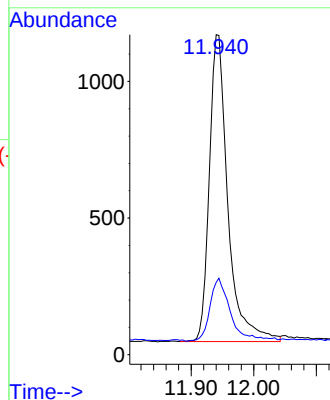


#12
2-Methylnaphthalene
Concen: 0.03 ng
RT: 12.015 min Scan# 1027
Delta R.T. -0.013 min
Lab File: BN012446.D
Acq: 29 Oct 2020 19:58

Tgt Ion:142 Resp: 284
Ion Ratio Lower Upper
142 100
141 95.8 69.4 104.2
115 75.9 35.7 53.5#

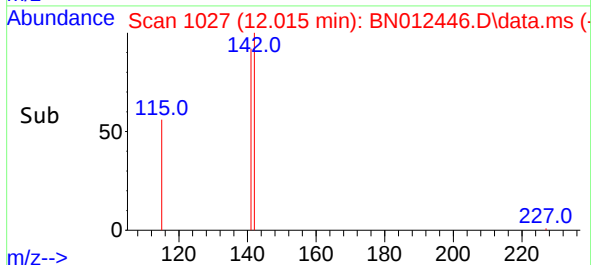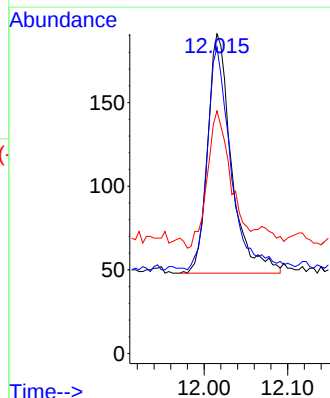
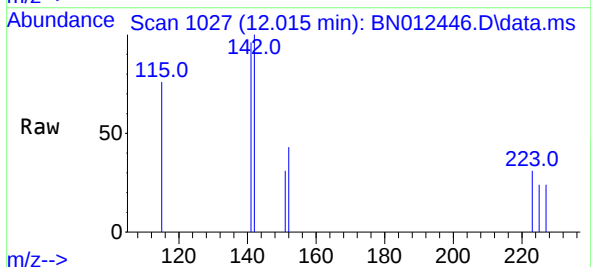




#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.217 min Scan# 1272
Delta R.T. 0.000 min
Lab File: BN012446.D
Acq: 29 Oct 2020 19:58




Tgt Ion:164 Resp: 2663
Ion Ratio Lower Upper
164 100
162 102.4 80.6 120.8
160 48.0 39.5 59.3

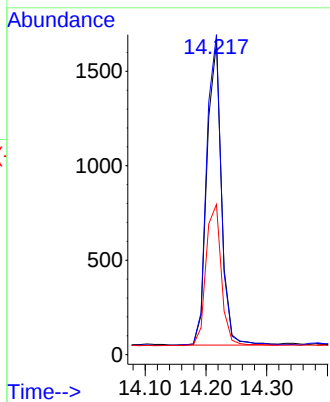


Instrument :
BNA_N
ClientSampleId :
STOCKPILE-LOC3-SO-0003

Manual Integrations
APPROVED



mohammad
10/30/2020 12:09:54 PM




#14
2,4,6-Tribromophenol
Concen: 0.28 ng
RT: 15.714 min Scan# 1390
Delta R.T. -0.013 min
Lab File: BN012446.D
Acq: 29 Oct 2020 19:58

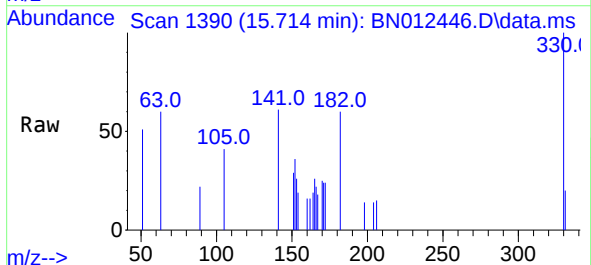

Tgt Ion:330 Resp: 534
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 47.2 34.4 51.6

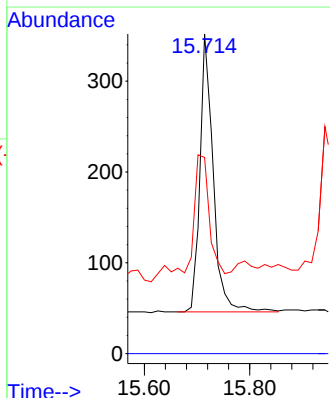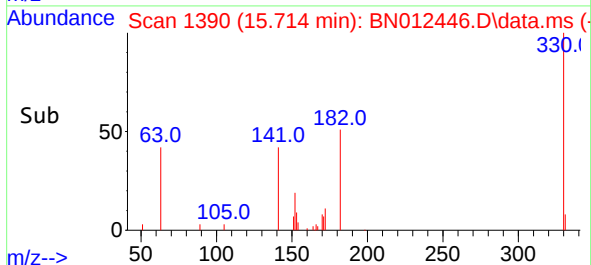







#15
2-Fluorobiphenyl
Concen: 0.37 ng
RT: 12.834 min Scan# 1163
Delta R.T. -0.013 min
Lab File: BN012446.D
Acq: 29 Oct 2020 19:58

Tgt Ion:	172	Resp:	3660
Ion	Ratio	Lower	Upper
172	100		
171	36.4	28.2	42.4
170	25.5	20.0	30.0

Instrument :
BNA_N
ClientSampleId :
STOCKPILE-LOC3-SO-0003




Manual Integrations
APPROVED


mohammad
10/30/2020 12:09:54 PM

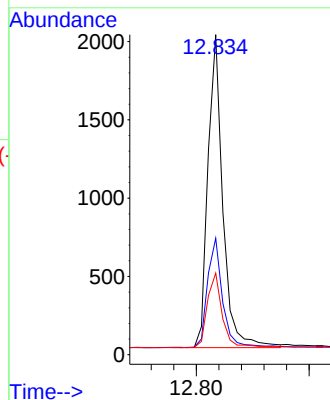

#16
Acenaphthylene
Concen: 0.08 ng
RT: 13.938 min Scan# 1250
Delta R.T. 0.000 min
Lab File: BN012446.D
Acq: 29 Oct 2020 19:58


Tgt Ion:	152	Resp:	991
Ion	Ratio	Lower	Upper
152	100		
151	24.9	15.8	23.8#
153	12.9	10.6	16.0

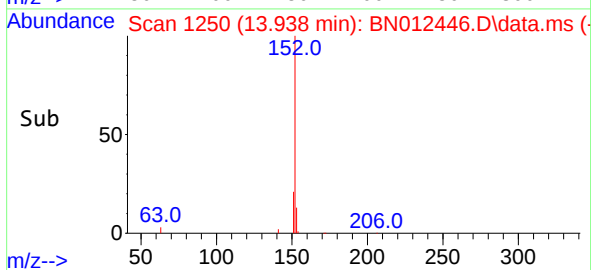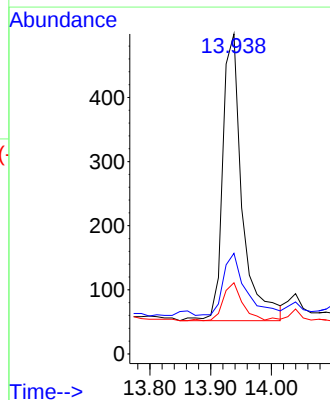



#17
Acenaphthene
Concen: 0.23 ng
RT: 14.281 min Scan# 1277
Delta R.T. 0.000 min
Lab File: BN012446.D
Acq: 29 Oct 2020 19:58




Instrument :
BNA_N
ClientSampleId :
STOCKPILE-LOC3-SO-0003



Tgt Ion:154 Resp: 1938
Ion Ratio Lower Upper
154 100
153 115.5 83.6 125.4
152 58.4 43.9 65.9




Manual Integrations
APPROVED


mohammad
10/30/2020 12:09:54 PM

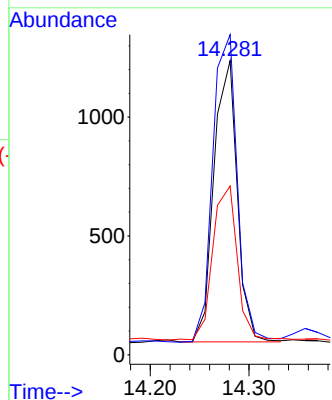

#18
Fluorene
Concen: 0.14 ng
RT: 15.270 min Scan# 1355
Delta R.T. -0.013 min
Lab File: BN012446.D
Acq: 29 Oct 2020 19:58


Tgt Ion:166 Resp: 1498
Ion Ratio Lower Upper
166 100
165 98.2 78.6 118.0
167 14.4 10.7 16.1

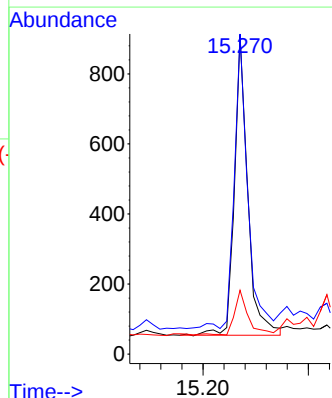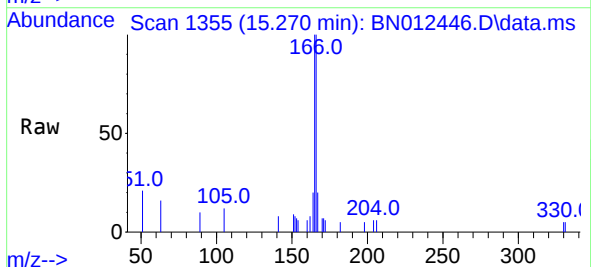

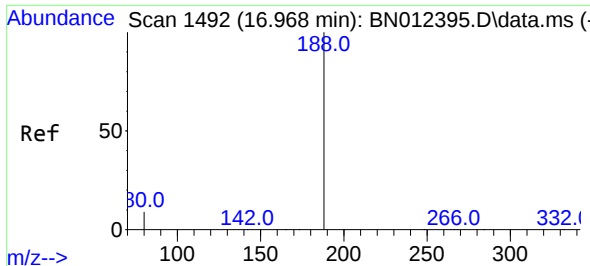

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 16.968 min Scan# 1492
Delta R.T. 0.000 min
Lab File: BN012446.D
Acq: 29 Oct 2020 19:58




Instrument :
BNA_N
ClientSampleId :
STOCKPILE-LOC3-SO-0003

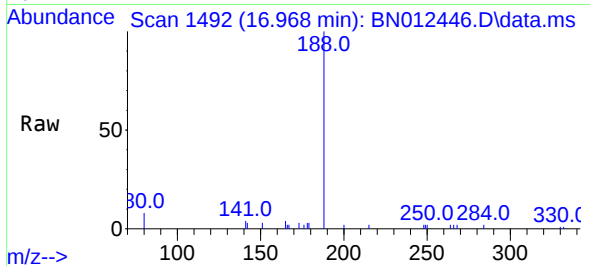


Tgt Ion:188 Resp: 5363
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 8.3 5.0 7.4#

Manual Integrations
APPROVED



mohammad
10/30/2020 12:09:54 PM

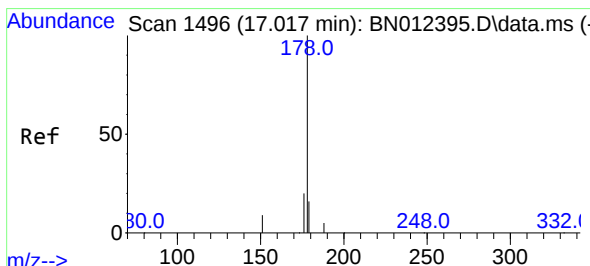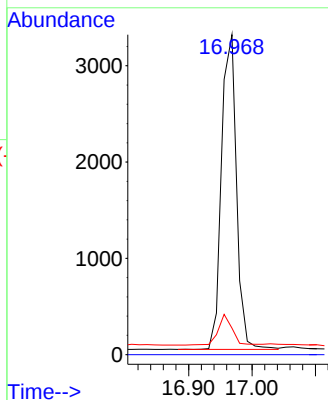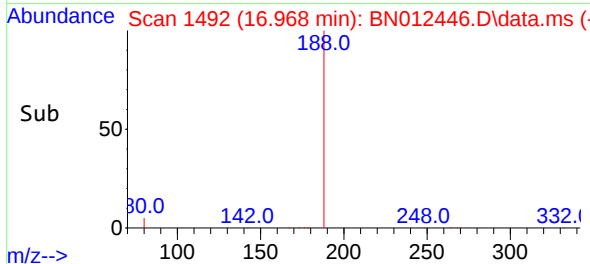


#25
Phenanthrene
Concen: 4.47 ng
RT: 17.005 min Scan# 1495
Delta R.T. -0.012 min
Lab File: BN012446.D
Acq: 29 Oct 2020 19:58

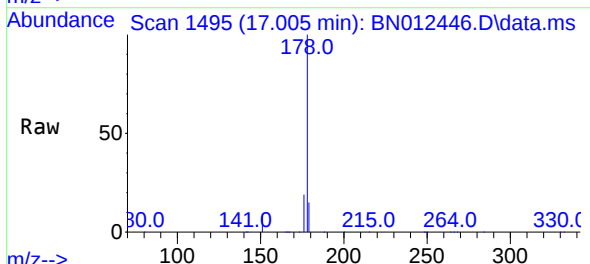

Tgt Ion:178 Resp: 69932
Ion Ratio Lower Upper
178 100
176 19.5 14.8 22.2
179 15.3 12.4 18.6

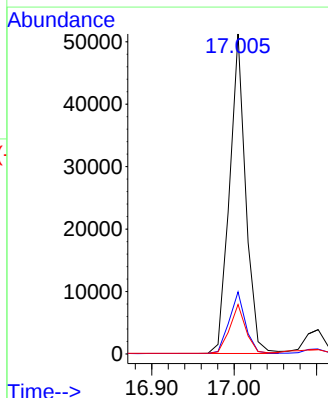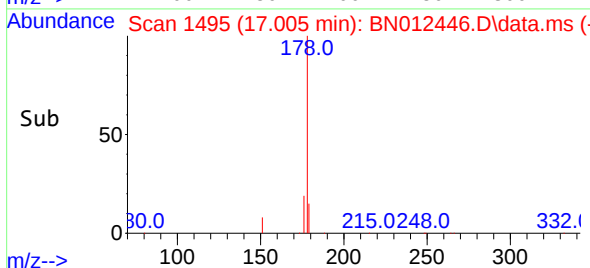







#26
 Anthracene
 Concen: 0.41 ng
 RT: 17.102 min Scan# 1503
 Delta R.T. 0.000 min
 Lab File: BN012446.D
 Acq: 29 Oct 2020 19:58

Tgt Ion:178 Resp: 5872
 Ion Ratio Lower Upper
 178 100
 176 19.3 14.8 22.2
 179 23.6 12.5 18.7#

Instrument :
 BNA_N
 ClientSampleId :
 STOCKPILE-LOC3-SO-0003




Manual Integrations
 APPROVED


mohammad
 10/30/2020 12:09:54 PM

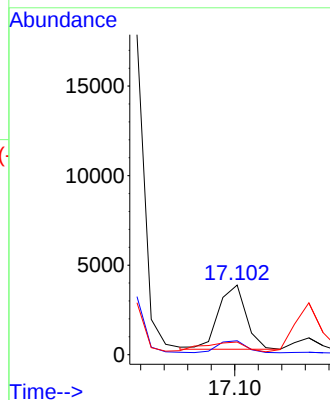

#27
 Fluoranthene-d10
 Concen: 0.31 ng
 RT: 19.008 min Scan# 1778
 Delta R.T. -0.005 min
 Lab File: BN012446.D
 Acq: 29 Oct 2020 19:58

Tgt Ion:212 Resp: 5194
 Ion Ratio Lower Upper
 212 100
 106 9.8 6.8 10.2
 104 6.4 4.1 6.1#

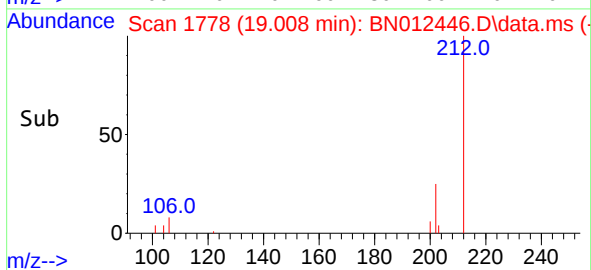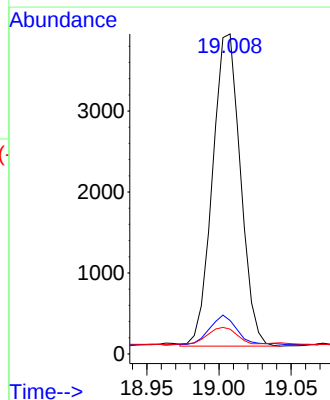







#28
Fluoranthene
Concen: 17.27 ng
RT: 19.037 min Scan# 1784
Delta R.T. -0.005 min
Lab File: BN012446.D
Acq: 29 Oct 2020 19:58

Tgt Ion:202 Resp: 321363
Ion Ratio Lower Upper
202 100
101 8.1 5.8 8.6
203 17.3 13.7 20.5

Instrument :
BNA_N
ClientSampleId :
STOCKPILE-LOC3-SO-0003




Manual Integrations
APPROVED


mohammad
10/30/2020 12:09:54 PM

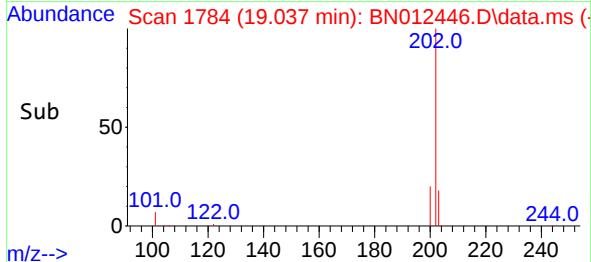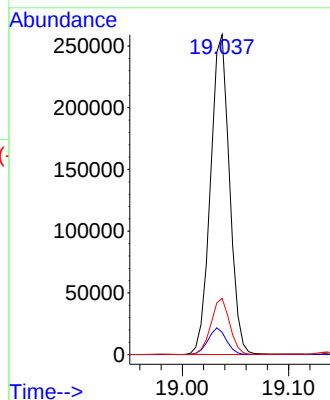


#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.174 min Scan# 2089
Delta R.T. 0.000 min
Lab File: BN012446.D
Acq: 29 Oct 2020 19:58

Tgt Ion:240 Resp: 6491
Ion Ratio Lower Upper
240 100
120 10.8 5.3 7.9#
236 28.4 21.8 32.8


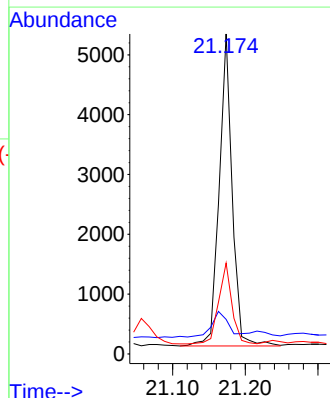






#30
Pyrene
Concen: 12.81 ng
RT: 19.400 min Scan# 1857
Delta R.T. -0.010 min
Lab File: BN012446.D
Acq: 29 Oct 2020 19:58





Tgt Ion:202 Resp: 281284
Ion Ratio Lower Upper
202 100
200 21.3 16.6 24.8
203 21.2 13.8 20.8#

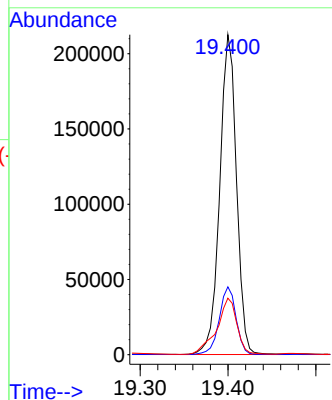

#31
Terphenyl-d14
Concen: 0.38 ng
RT: 19.613 min Scan# 1900
Delta R.T. -0.010 min
Lab File: BN012446.D
Acq: 29 Oct 2020 19:58




Tgt Ion:244 Resp: 5848
Ion Ratio Lower Upper
244 100
212 10.9 7.3 10.9
122 12.6 7.3 10.9#

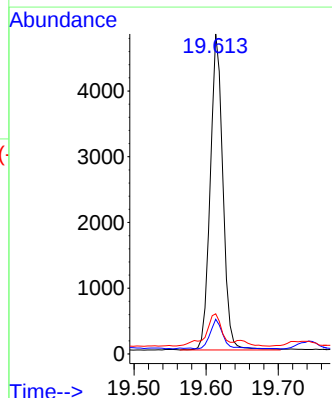

Instrument :
BNA_N
ClientSampleId :
STOCKPILE-LOC3-SO-0003

Manual Integrations
APPROVED

mohammad
10/30/2020 12:09:54 PM

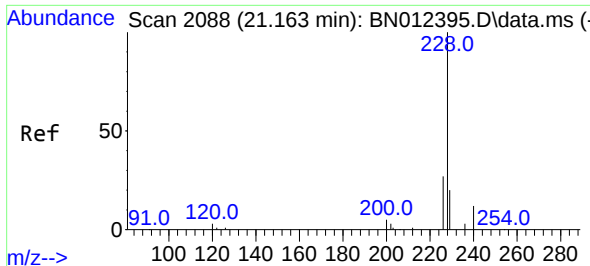





#32
Benzo(a)anthracene
Concen: 6.54 ng
RT: 21.152 min Scan# 2087
Delta R.T. -0.011 min
Lab File: BN012446.D
Acq: 29 Oct 2020 19:58

Tgt Ion:228 Resp: 129180
Ion Ratio Lower Upper
228 100
226 28.7 22.3 33.5
229 20.1 15.7 23.5

Instrument :
BNA_N
ClientSampleId :
STOCKPILE-LOC3-SO-0003




Manual Integrations
APPROVED


mohammad
10/30/2020 12:09:54 PM

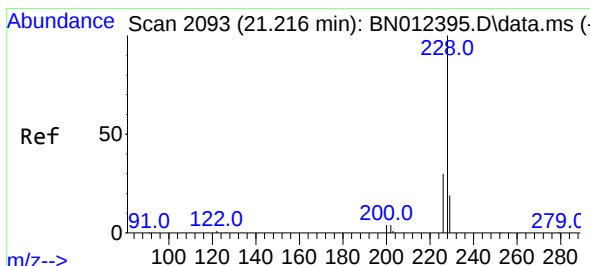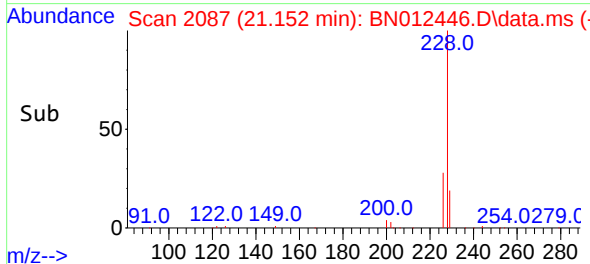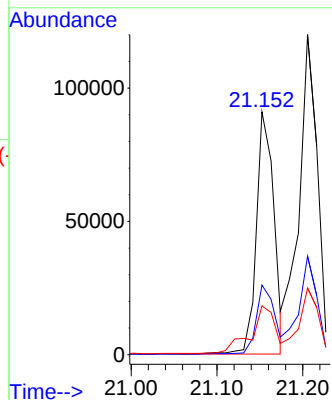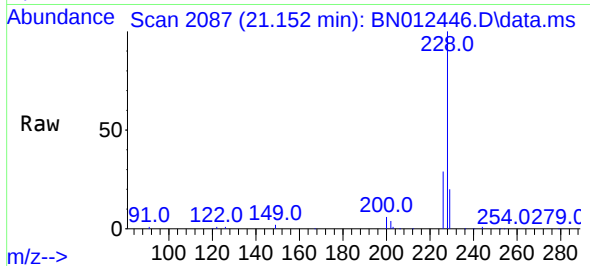

#33
Chrysene
Concen: 8.04 ng
RT: 21.206 min Scan# 2092
Delta R.T. -0.011 min
Lab File: BN012446.D
Acq: 29 Oct 2020 19:58


Tgt Ion:228 Resp: 178011
Ion Ratio Lower Upper
228 100
226 30.8 24.2 36.2
229 20.8 15.7 23.5

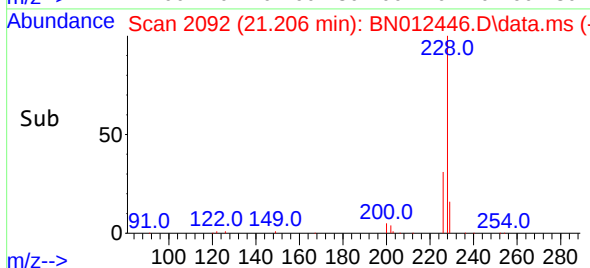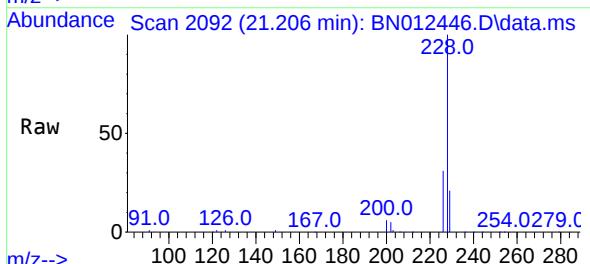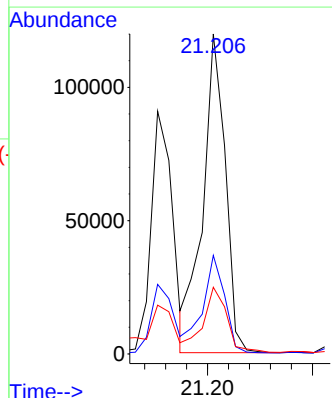

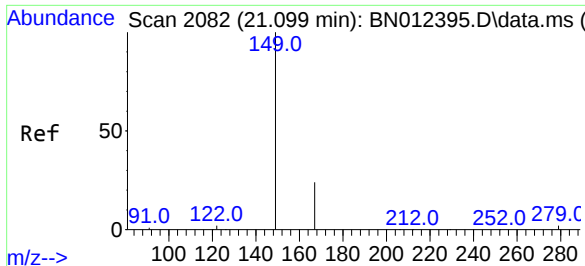

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.41 ng
RT: 21.099 min Scan# 2082
Delta R.T. 0.000 min
Lab File: BN012446.D
Acq: 29 Oct 2020 19:58




Instrument :
BNA_N
ClientSampleId :
STOCKPILE-LOC3-SO-0003

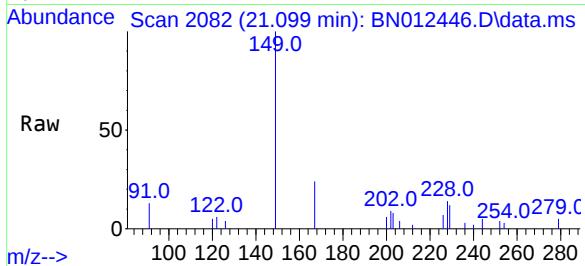

Tgt Ion:149 Resp: 5271
Ion Ratio Lower Upper
149 100
167 23.2 23.2 34.8
279 3.9 3.9 5.9




Manual Integrations
APPROVED


mohammad
10/30/2020 12:09:54 PM

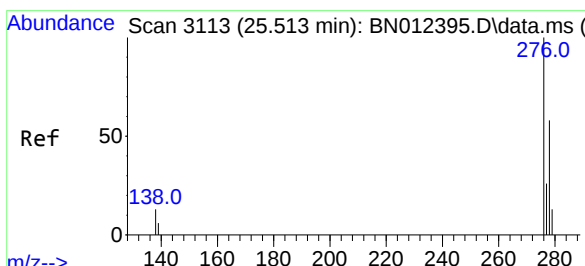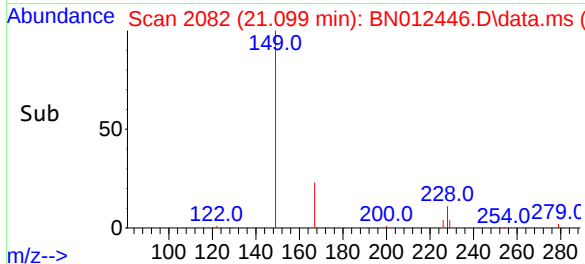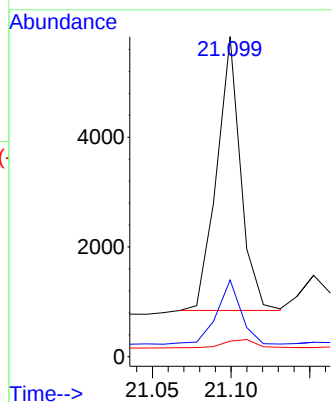

#35
Indeno(1,2,3-cd)pyrene
Concen: 5.52 ng
RT: 25.500 min Scan# 3109
Delta R.T. -0.010 min
Lab File: BN012446.D
Acq: 29 Oct 2020 19:58


Tgt Ion:276 Resp: 175734
Ion Ratio Lower Upper
276 100
138 15.9 13.3 19.9
277 24.4 20.2 30.4

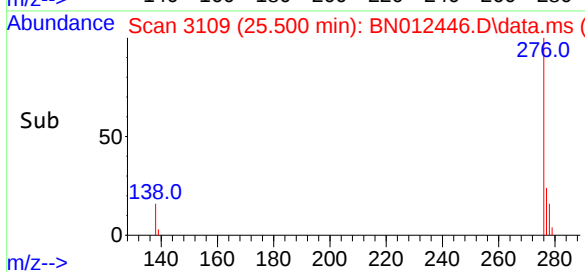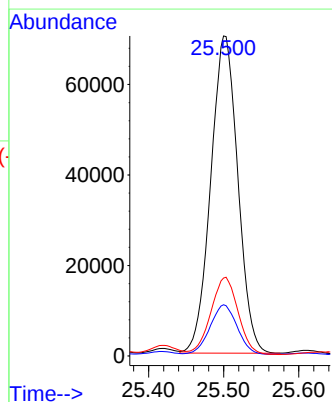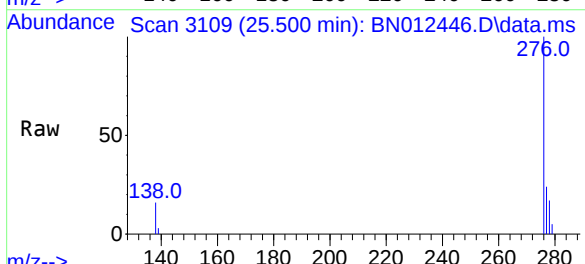

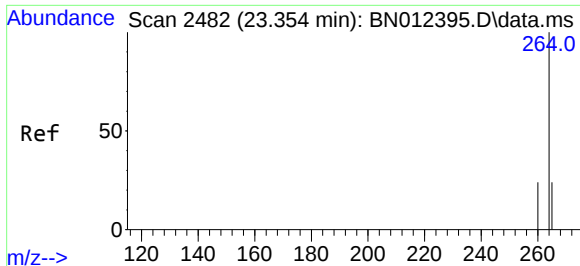

#36
Perylene-d12
Concen: 0.40 ng
RT: 23.343 min Scan# 2479
Delta R.T. -0.010 min
Lab File: BN012446.D
Acq: 29 Oct 2020 19:58




Instrument :
BNA_N
ClientSampleId :
STOCKPILE-LOC3-SO-0003

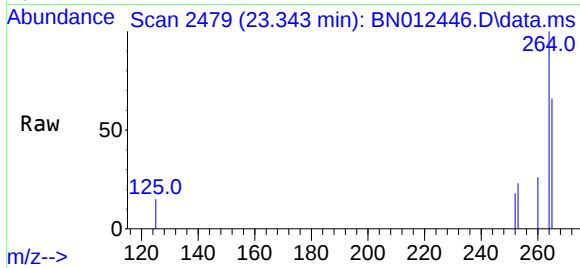

Tgt Ion:264 Resp: 7254
Ion Ratio Lower Upper
264 100
260 26.5 19.8 29.6
265 66.3 51.4 77.0




Manual Integrations
APPROVED


mohammad
10/30/2020 12:09:54 PM

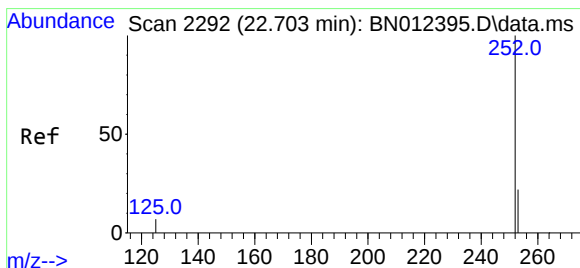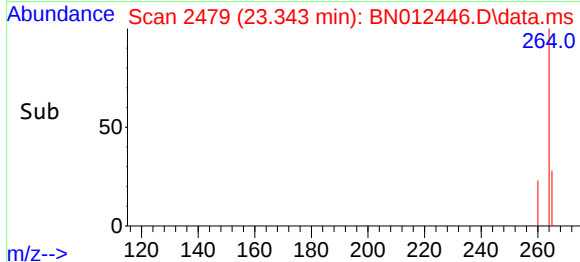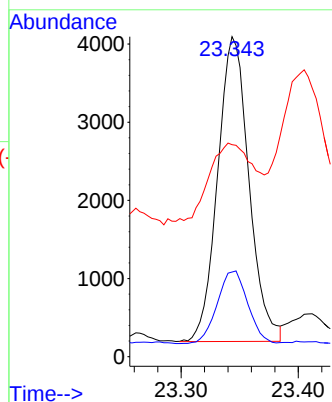

#37
Benzo(b)fluoranthene
Concen: 13.12 ng
RT: 22.700 min Scan# 2291
Delta R.T. -0.003 min
Lab File: BN012446.D
Acq: 29 Oct 2020 19:58

Tgt Ion:252 Resp: 300242
Ion Ratio Lower Upper
252 100
253 22.8 20.1 30.1
125 8.9 7.2 10.8

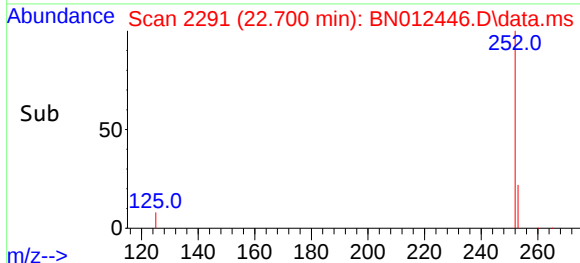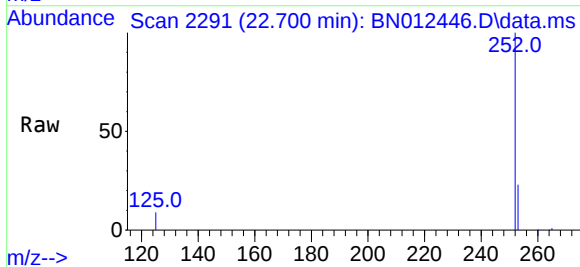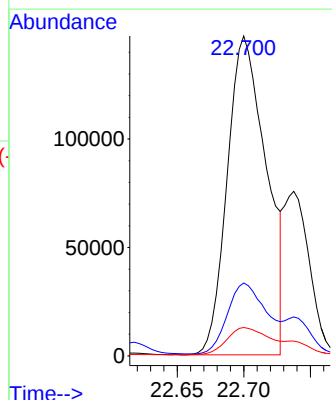







#38
Benzo(k)fluoranthene
Concen: 3.94 ng m
RT: 22.738 min Scan# 2302
Delta R.T. -0.010 min
Lab File: BN012446.D
Acq: 29 Oct 2020 19:58

Tgt Ion:252	Resp:	98214
Ion Ratio	Lower	Upper
252	100	
253	23.7	19.8 29.8
125	9.0	7.1 10.7

Instrument :
BNA_N
ClientSampleId :
STOCKPILE-LOC3-SO-0003




Manual Integrations
APPROVED


mohammad
10/30/2020 12:09:54 PM

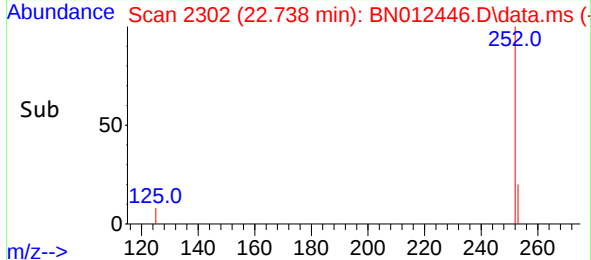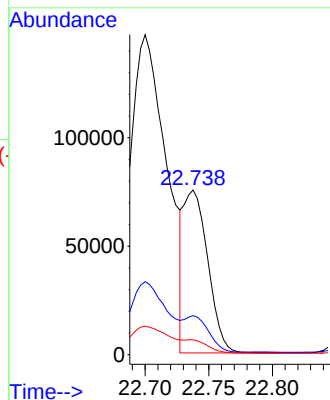

#39
Benzo(a)pyrene
Concen: 8.44 ng
RT: 23.251 min Scan# 2452
Delta R.T. -0.010 min
Lab File: BN012446.D
Acq: 29 Oct 2020 19:58

Tgt Ion:252	Resp:	187438
Ion Ratio	Lower	Upper
252	100	
253	23.2	21.3 31.9
125	9.4	8.3 12.5

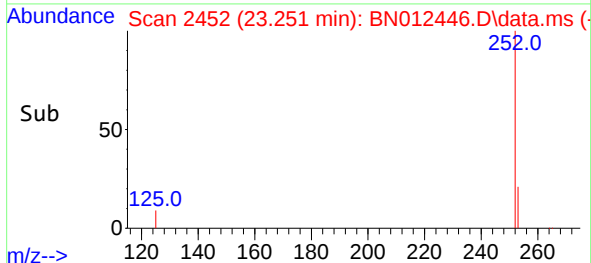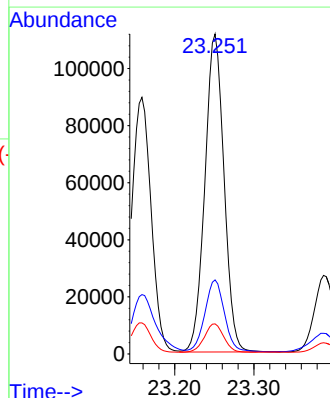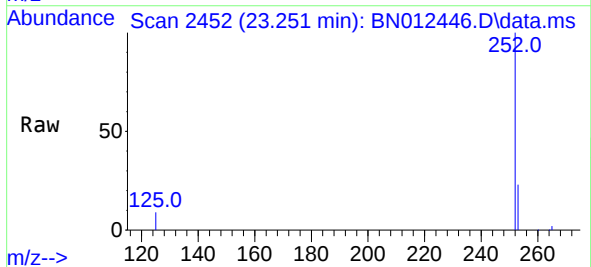







#40
Dibenzo(a,h)anthracene
Concen: 1.46 ng
RT: 25.507 min Scan# 3111
Delta R.T. -0.020 min
Lab File: BN012446.D
Acq: 29 Oct 2020 19:58

Tgt Ion:278 Resp: 36574
Ion Ratio Lower Upper
278 100
139 16.6 9.3 13.9#
279 27.1 21.6 32.4

Instrument :
BNA_N
ClientSampleId :
STOCKPILE-LOC3-SO-0003

Manual Integrations
APPROVED

mohammad
10/30/2020 12:09:54 PM

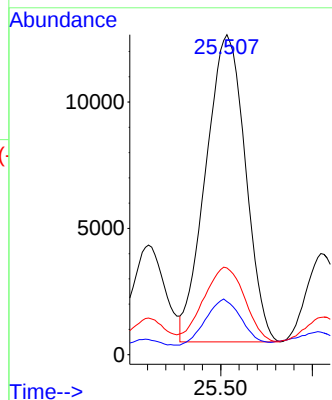

#41
Benzo(g,h,i)perylene
Concen: 6.92 ng
RT: 26.164 min Scan# 3303
Delta R.T. -0.007 min
Lab File: BN012446.D
Acq: 29 Oct 2020 19:58

Tgt Ion:276 Resp: 182374
Ion Ratio Lower Upper
276 100
277 24.1 19.8 29.8
138 16.3 11.7 17.5

