


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102920\
 Data File : BN012430.D
 Acq On : 29 Oct 2020 08:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN102620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 28 10:32:42 2020

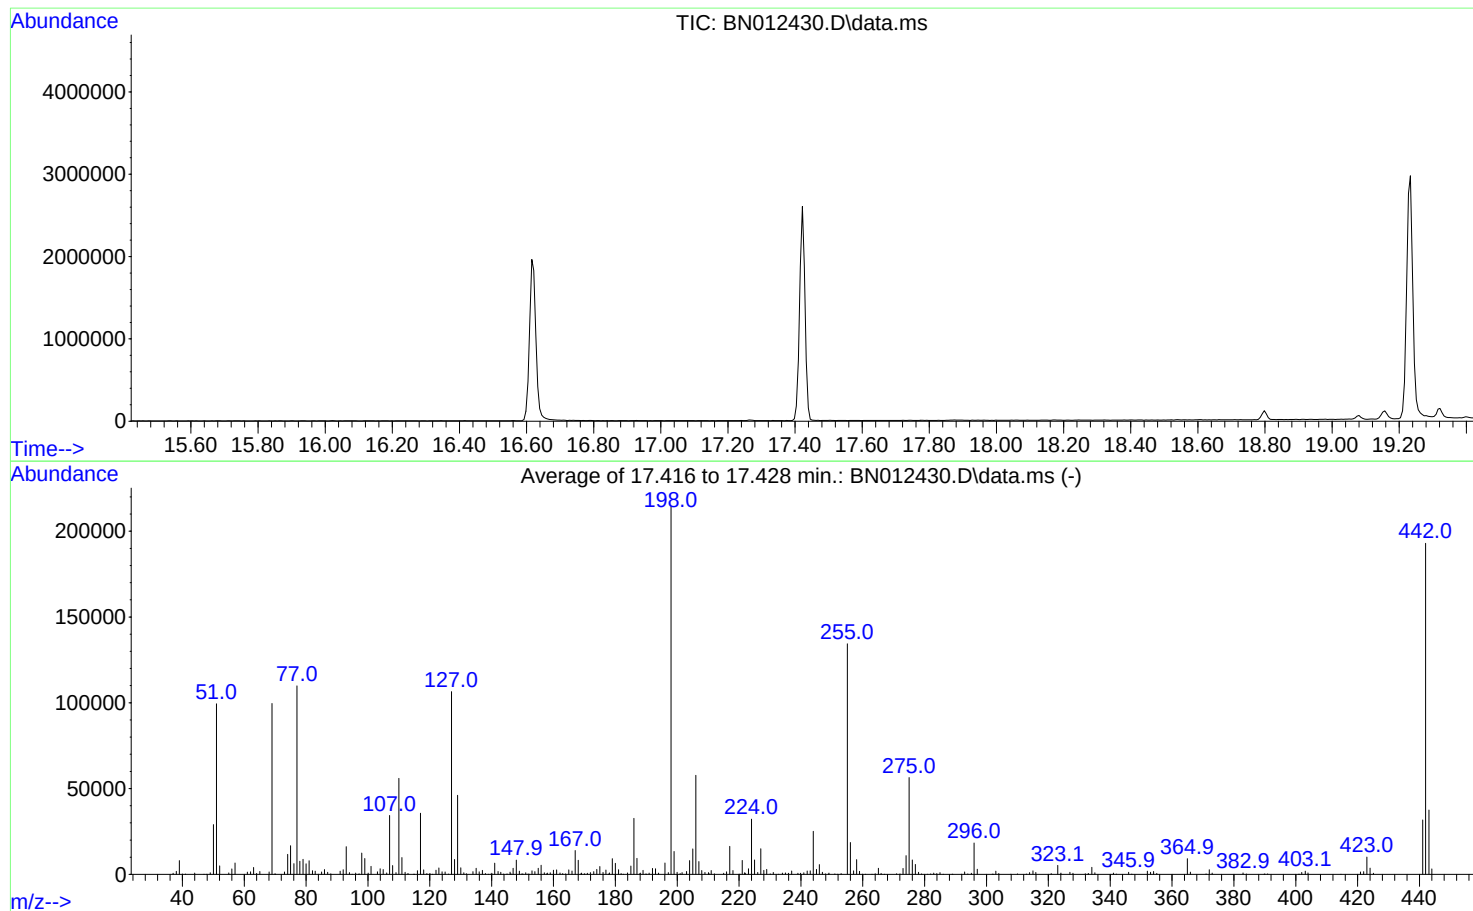

AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.4	99443	PASS
68	69	0.00	2	1.5	1451	PASS
69	198	0.00	100	46.5	99597	PASS
70	69	0.00	2	0.3	260	PASS
127	198	10	80	49.7	106472	PASS
197	198	0.00	2	0.5	991	PASS
198	198	100	100	100.0	214400	PASS
199	198	5	9	6.2	13369	PASS
275	198	10	60	26.3	56429	PASS
365	198	1	100	4.3	9191	PASS
441	198	0.01	100	14.8	31685	PASS
442	198	50	100	90.0	192963	PASS
443	442	15	24	19.4	37456	PASS