


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102920\
 Data File : BN012448.D
 Acq On : 29 Oct 2020 21:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN102620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 28 10:32:42 2020

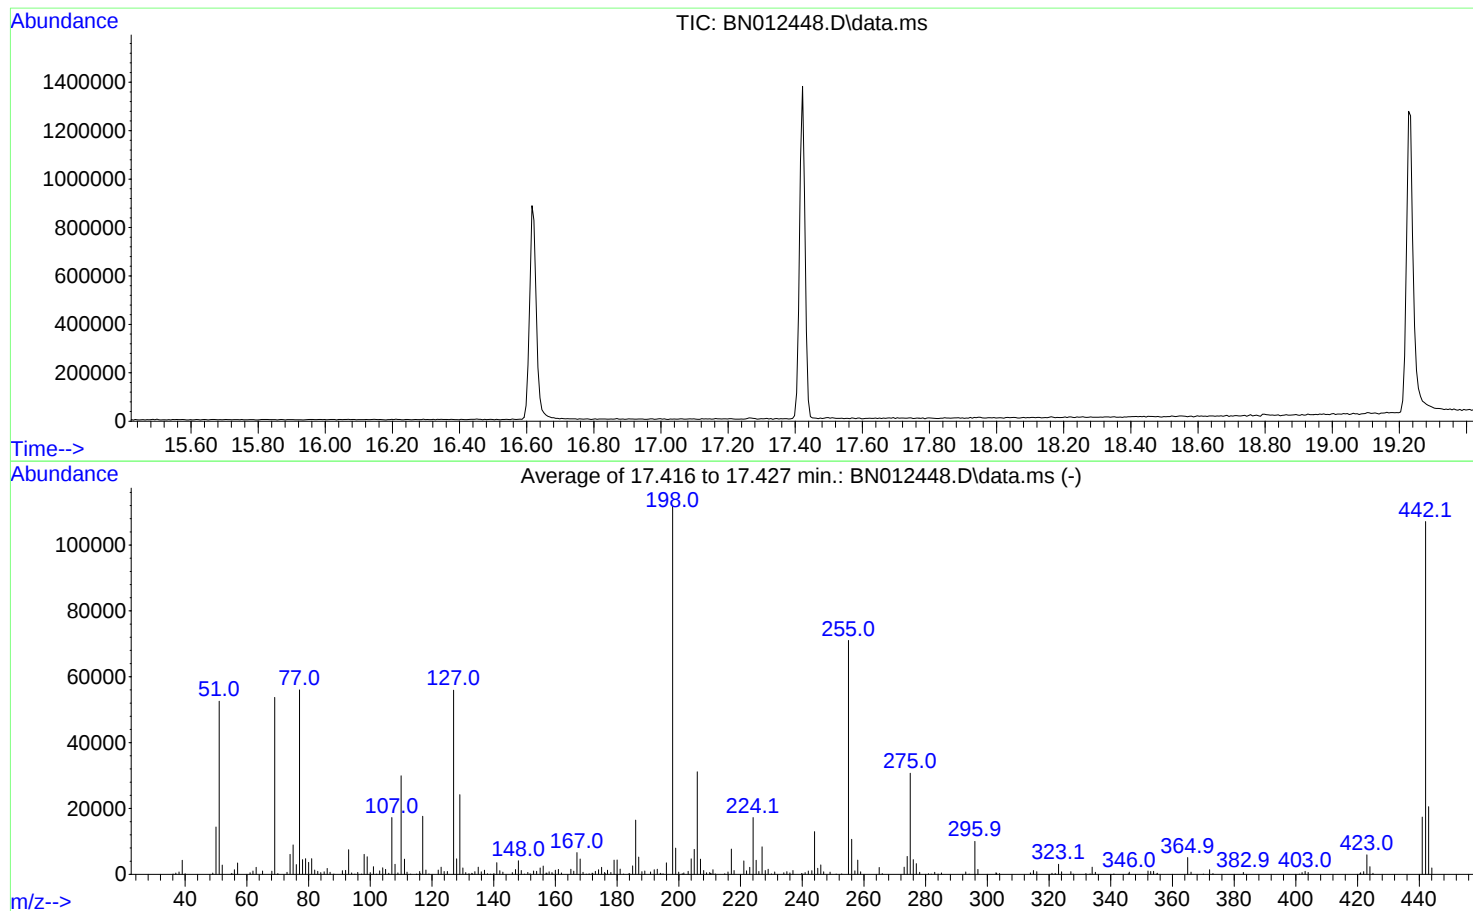

AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.1	52581	PASS
68	69	0.00	2	1.8	961	PASS
69	198	0.00	100	48.1	53752	PASS
70	69	0.00	2	0.3	162	PASS
127	198	10	80	50.1	55949	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	111704	PASS
199	198	5	9	7.2	7993	PASS
275	198	10	60	27.5	30696	PASS
365	198	1	100	4.6	5107	PASS
441	198	0.01	100	15.6	17379	PASS
442	198	50	100	95.9	107144	PASS
443	442	15	24	19.2	20553	PASS