

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
 Data File : BN022369.D
 Acq On : 27 Oct 2022 19:56
 Operator : CG/JU
 Sample : N5232-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHAC6

Quant Time: Oct 28 00:37:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 28 00:29:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	162155	20.000	ng/ul	0.00
20) Naphthalene-d8	10.763	136	693914	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.610	164	395632	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.363	188	682628	20.000	ng/ul	0.00
79) Chrysene-d12	21.569	240	467808	20.000	ng/ul	0.00
88) Perylene-d12	24.021	264	461719	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.246	96	19168	4.480	ng/uL	0.00
4) Pyridine-d5	3.705	84	20344	1.529	ng/ul	0.02
7) Phenol-d5	7.093	99	100419	6.335	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.263	67	330315	33.252	ng/ul	0.00
11) 2-Chlorophenol-d4	7.457	132	289950	26.380	ng/ul	0.00
15) 4-Methylphenol-d8	8.657	113	185334	14.713	ng/ul	0.00
21) Nitrobenzene-d5	9.116	128	203318	39.959	ng/ul	0.00
24) 2-Nitrophenol-d4	9.840	143	200172	38.382	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.381	165	310526	31.721	ng/ul	0.00
31) 4-Chloroaniline-d4	10.916	131	20602	1.287	ng/ul	0.00
46) Dimethylphthalate-d6	14.022	166	1053221	38.189	ng/ul	0.00
49) Acenaphthylene-d8	14.304	160	1221090	39.649	ng/ul	0.00
54) 4-Nitrophenol-d4	14.816	143	28055	4.766	ng/ul	0.00
60) Fluorene-d10	15.604	176	886243	38.099	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.734	200	131786	33.841	ng/ul	0.00
73) Anthracene-d10	17.463	188	1271760	42.871	ng/ul	0.00
81) Pyrene-d10	19.769	212	1122323	48.187	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.868	264	965080	42.621	ng/ul	0.00
Target Compounds						
48) 2,6-Dinitrotoluene	14.028	165	5789	1.043	ng/ul#	33


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
Data File : BN022369.D
Acq On : 27 Oct 2022 19:56
Operator : CG/JU
Sample : N5232-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHAC6


Quant Time: Oct 28 00:37:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 28 00:29:18 2022
Response via : Initial Calibration

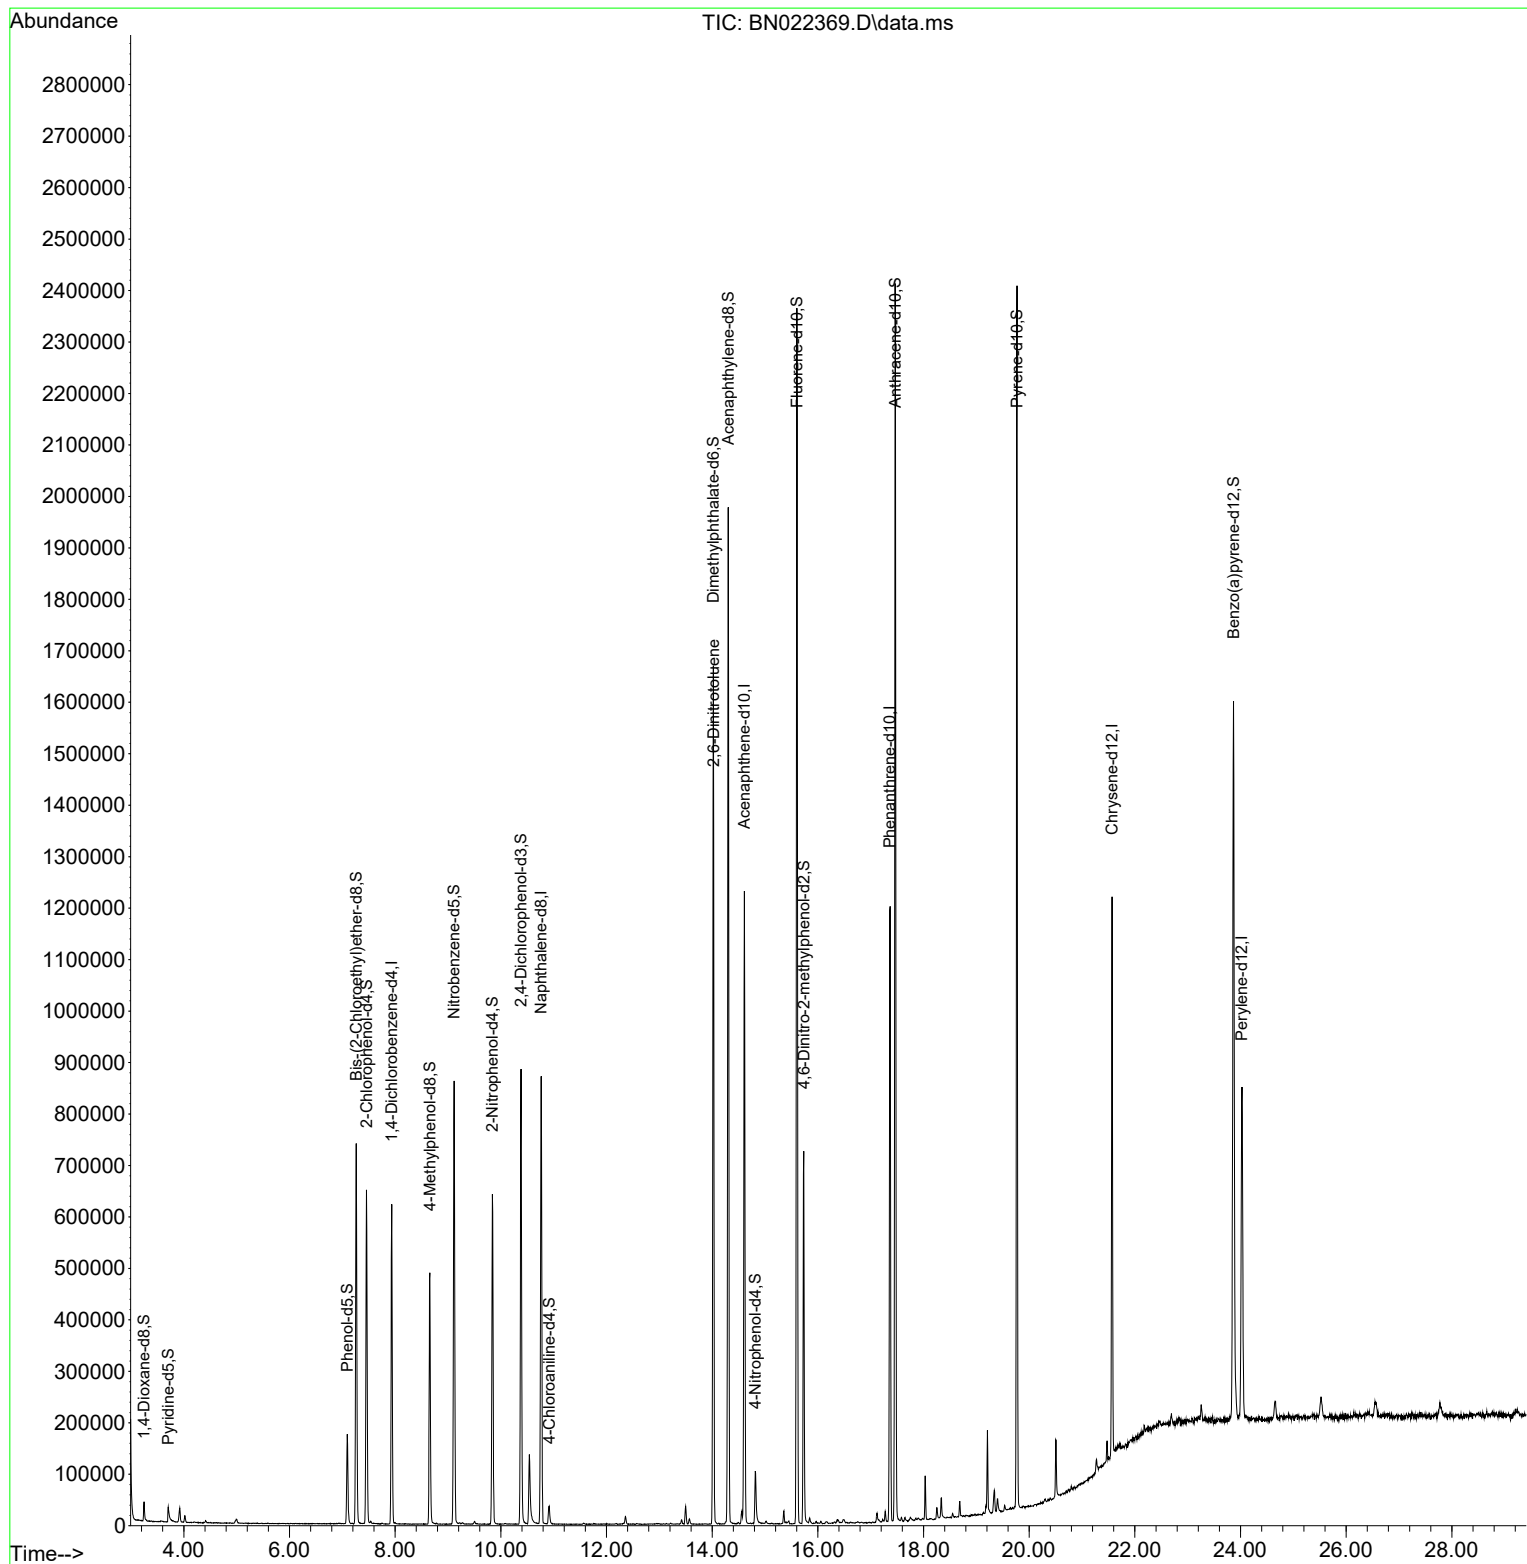

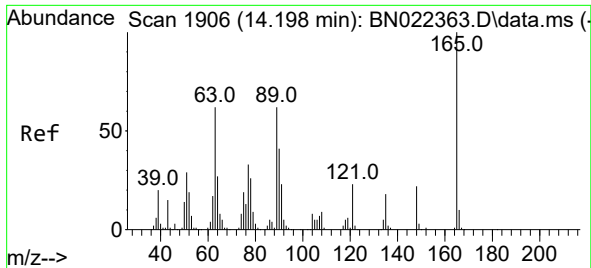

#48
 2,6-Dinitrotoluene
 Concen: 1.043 ng/ul
 RT: 14.028 min Scan# 11
 Delta R.T. -0.170 min
 Lab File: BN022369.D
 Acq: 27 Oct 2022 19:56

Instrument :
 BNA_N
 ClientSampleId :
 BHAC6

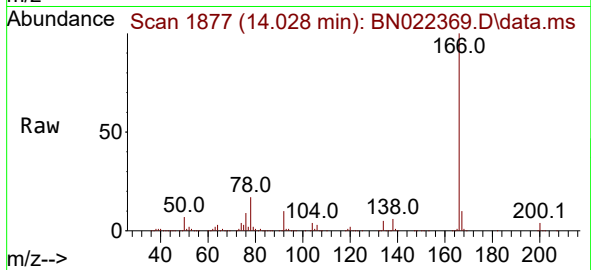

Tgt Ion	Ratio	Lower	Upper
165	100		
89	0.0	52.1	78.1#
121	36.6	19.0	28.4#

