

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
 Data File : BN022385.D
 Acq On : 28 Oct 2022 15:18
 Operator : CG/JU
 Sample : N5233-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHA52

Quant Time: Oct 29 01:10:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 29 00:50:42 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.922	152	141677	20.000	ng/ul	0.00
20) Naphthalene-d8	10.751	136	659364	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.598	164	415130	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.357	188	824878	20.000	ng/ul	0.00
79) Chrysene-d12	21.556	240	577928	20.000	ng/ul	0.00
88) Perylene-d12	24.009	264	472372	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	15986	4.277	ng/uL	0.00
4) Pyridine-d5	3.693	84	22769	1.958	ng/ul	0.02
7) Phenol-d5	7.081	99	90352	6.523	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.251	67	278697	32.111	ng/ul	0.00
11) 2-Chlorophenol-d4	7.451	132	250799	26.116	ng/ul	0.00
15) 4-Methylphenol-d8	8.645	113	172432	15.668	ng/ul	0.00
21) Nitrobenzene-d5	9.104	128	178144	36.846	ng/ul	0.00
24) 2-Nitrophenol-d4	9.834	143	183002	36.929	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	285464	30.689	ng/ul	0.00
31) 4-Chloroaniline-d4	10.898	131	139630	9.181	ng/ul	0.00
46) Dimethylphthalate-d6	14.016	166	1129684	39.038	ng/ul	0.00
49) Acenaphthylene-d8	14.298	160	1198756	37.096	ng/ul	0.00
54) 4-Nitrophenol-d4	14.810	143	37164	6.017	ng/ul	0.00
60) Fluorene-d10	15.598	176	945120	38.722	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.721	200	157271	33.420	ng/ul	0.00
73) Anthracene-d10	17.457	188	1518557	42.363	ng/ul	0.00
81) Pyrene-d10	19.757	212	1493709	51.912	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.850	264	1019729	44.018	ng/ul	0.00
Target Compounds						
48) 2,6-Dinitrotoluene	14.022	165	6058	1.040	ng/ul#	37


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
Data File : BN022385.D
Acq On : 28 Oct 2022 15:18
Operator : CG/JU
Sample : N5233-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHA52


Quant Time: Oct 29 01:10:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 29 00:50:42 2022
Response via : Initial Calibration

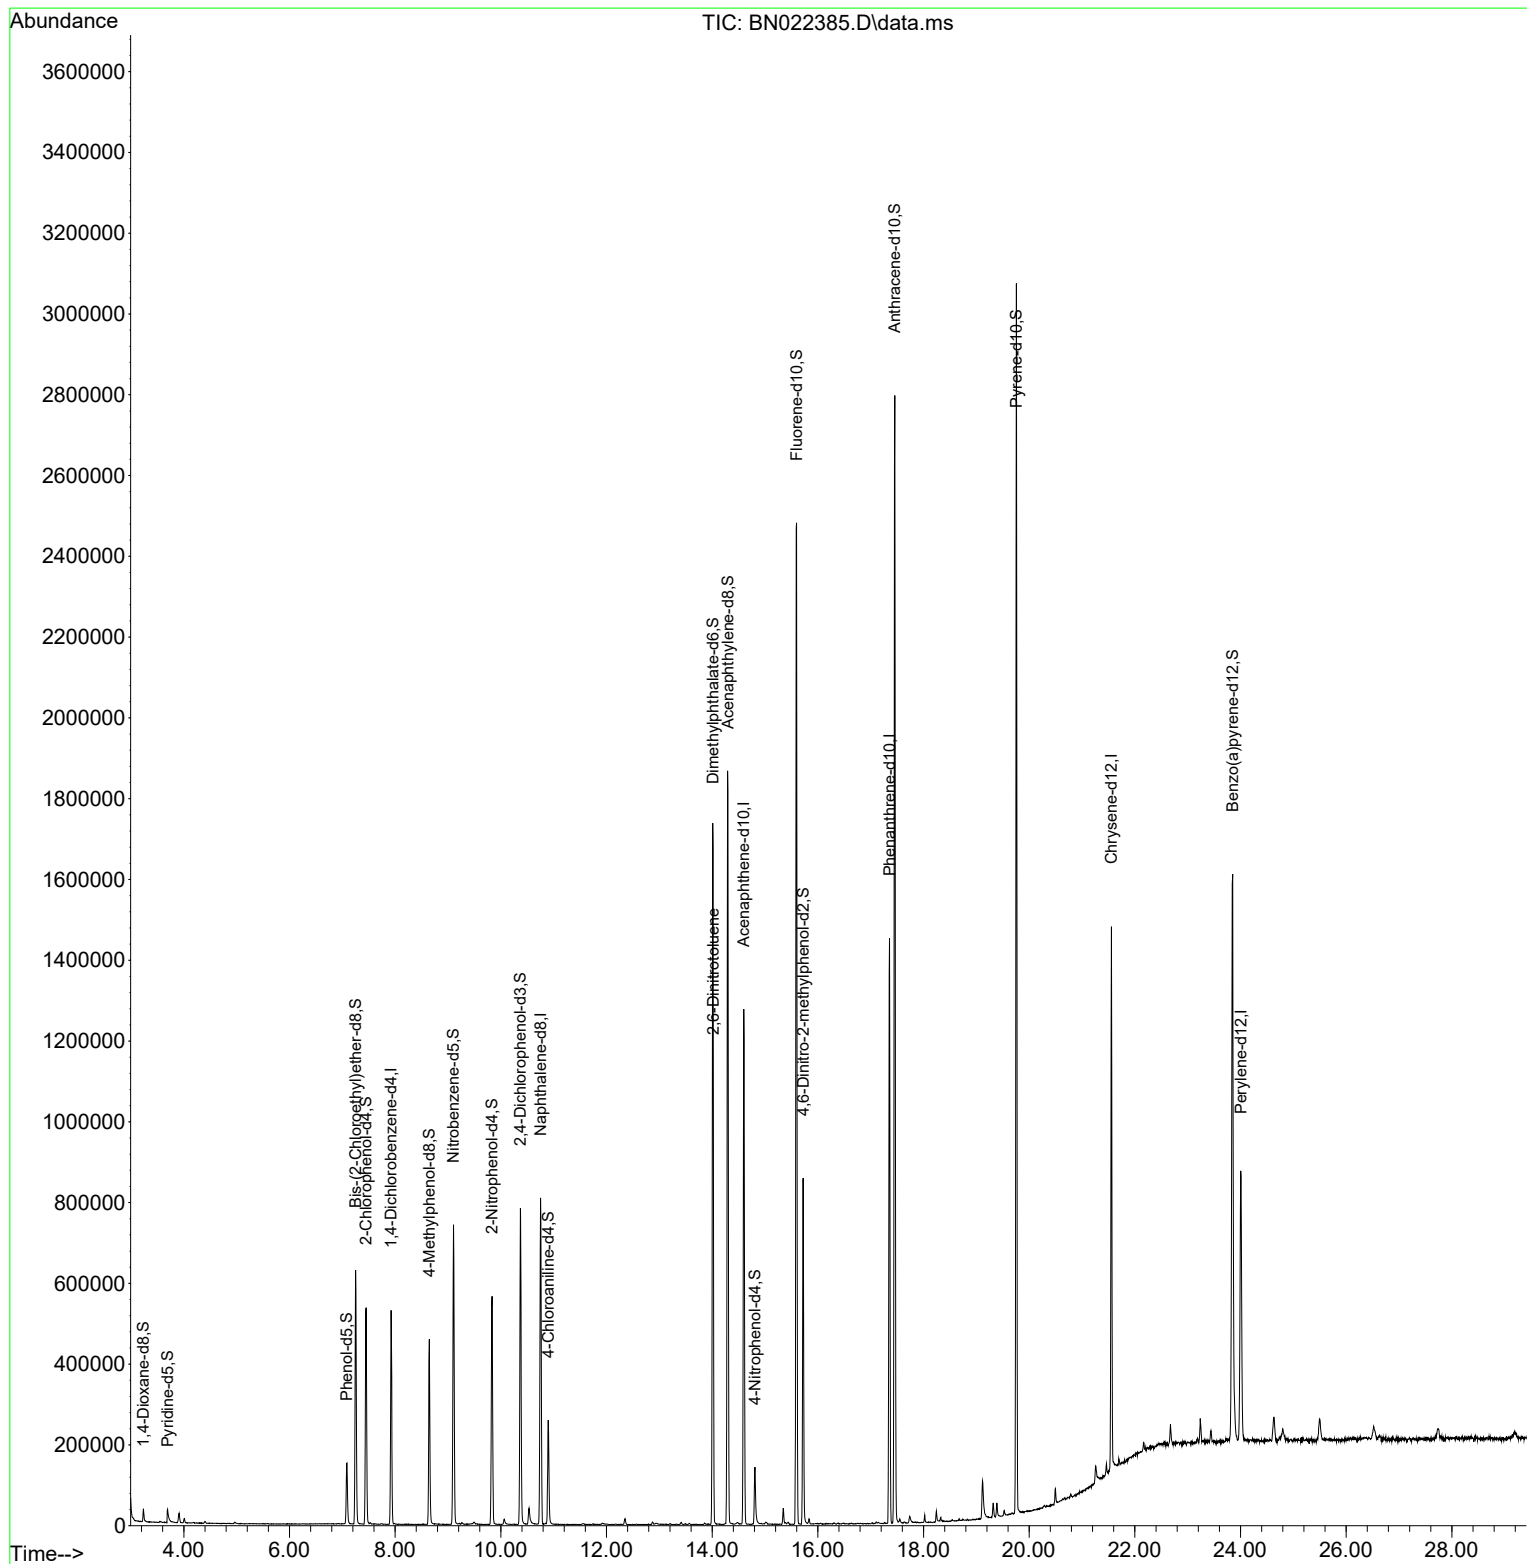

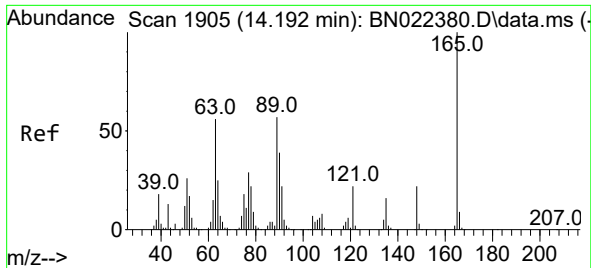

#48
 2,6-Dinitrotoluene
 Concen: 1.040 ng/ul
 RT: 14.022 min Scan# 11
 Delta R.T. -0.171 min
 Lab File: BN022385.D
 Acq: 28 Oct 2022 15:18

Instrument :
 BNA_N
 ClientSampleId :
 BHA52

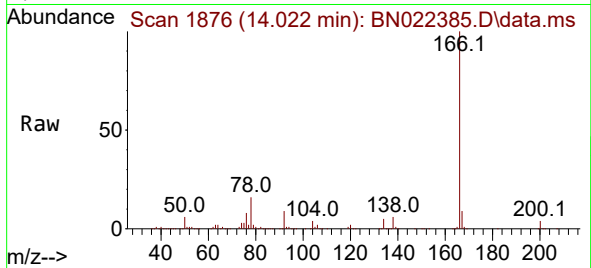

Tgt Ion	Ratio	Lower	Upper
165	100		
89	0.0	52.1	78.1#
121	29.1	19.0	28.4#

