

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
 Data File : BN022376.D
 Acq On : 28 Oct 2022 00:15
 Operator : CG/JU
 Sample : N5119-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BC4

Quant Time: Oct 28 01:28:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 28 00:29:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	155665	20.000	ng/u1	0.00
20) Naphthalene-d8	10.763	136	599661	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.610	164	327202	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.363	188	613273	20.000	ng/u1	0.00
79) Chrysene-d12	21.563	240	539228	20.000	ng/u1	-0.01
88) Perylene-d12	24.021	264	580123	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.246	96	16915	4.118	ng/uL	0.00
4) Pyridine-d5	3.699	84	33081	2.589	ng/u1	0.02
7) Phenol-d5	7.093	99	264639	17.390	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.258	67	181689	19.053	ng/u1	0.00
11) 2-Chlorophenol-d4	7.458	132	212124	20.104	ng/u1	0.00
15) 4-Methylphenol-d8	8.652	113	82702	6.839	ng/u1	0.00
21) Nitrobenzene-d5	9.110	128	102791	23.377	ng/u1	0.00
24) 2-Nitrophenol-d4	9.840	143	107240	23.795	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.381	165	165819	19.601	ng/u1	0.00
31) 4-Chloroaniline-d4	10.904	131	203578	14.719	ng/u1	0.00
46) Dimethylphthalate-d6	14.022	166	482119	21.138	ng/u1	0.00
49) Acenaphthylene-d8	14.304	160	561674	22.052	ng/u1	0.00
54) 4-Nitrophenol-d4	14.816	143	64467	13.242	ng/u1	0.00
60) Fluorene-d10	15.604	176	417276	21.690	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.728	200	40761	11.650	ng/u1	-0.01
73) Anthracene-d10	17.463	188	563017	21.126	ng/u1	0.00
81) Pyrene-d10	19.763	212	656358	24.448	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.857	264	627936	22.071	ng/u1	-0.02
Target Compounds						
					Qvalue	
80) Fluoranthene	19.428	202	36682	1.088	ng/u1	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
Data File : BN022376.D
Acq On : 28 Oct 2022 00:15
Operator : CG/JU
Sample : N5119-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BC4

Quant Time: Oct 28 01:28:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 28 00:29:18 2022
Response via : Initial Calibration

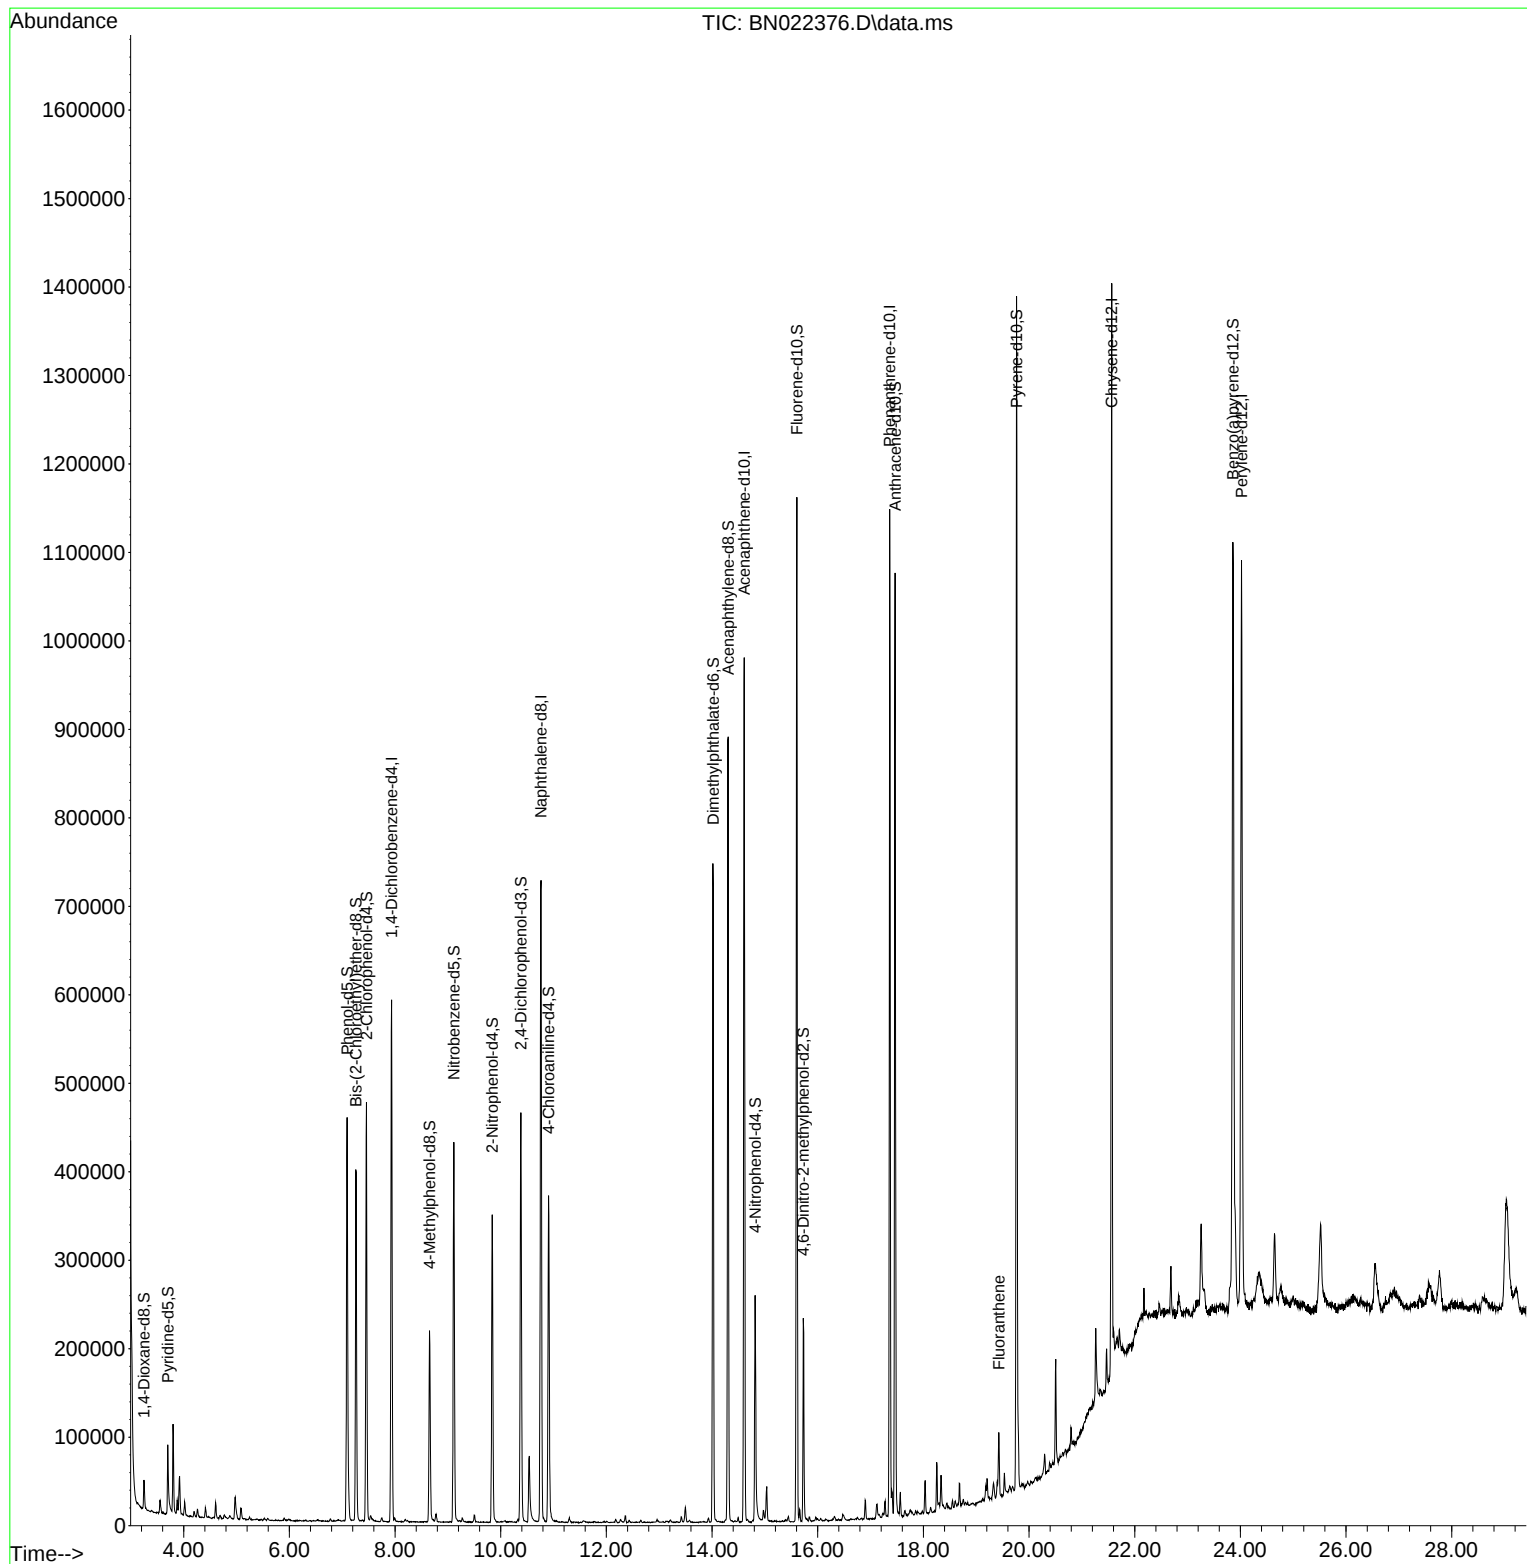

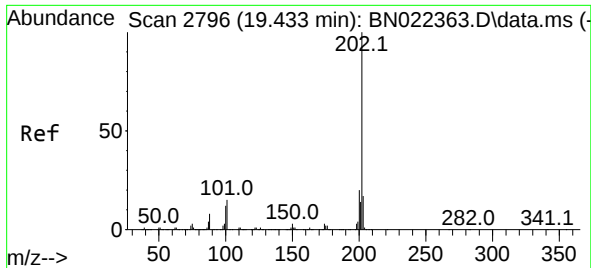

#80

Fluoranthene

Concen: 1.088 ng/ul

RT: 19.428 min Scan# 21

Delta R.T. -0.006 min

Lab File: BN022376.D


Acq: 28 Oct 2022 00:15

Instrument :

BNA_N

ClientSampleId :

C0BC4

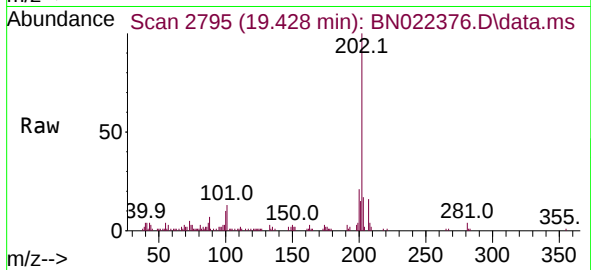

Tgt Ion:202 Resp: 36682

Ion Ratio Lower Upper

202 100

101 12.9 10.3 15.5

100 10.0 7.8 11.8

