

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
 Data File : BN022365.D
 Acq On : 27 Oct 2022 17:24
 Operator : CG/JU
 Sample : PB148426BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK426

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022365.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	40	44	56	rVB	59540	83757	2.82%	0.218%
2	3.681	115	118	139	rBV	651734	1006422	33.86%	2.623%
3	4.022	171	176	184	rVB	16022	24632	0.83%	0.064%
4	7.093	691	698	712	rBV	816376	1316425	44.29%	3.431%
5	7.263	720	727	747	rVB	680770	1069894	36.00%	2.789%
6	7.457	753	760	775	rBV	801414	1313758	44.20%	3.424%
7	7.934	834	841	854	rBV	703023	1154221	38.83%	3.008%
8	8.657	957	964	978	rBV	947149	1534434	51.62%	3.999%
9	9.116	1034	1042	1055	rBV	743304	1214737	40.87%	3.166%
10	9.846	1159	1166	1177	rBV	587303	981301	33.01%	2.558%
11	10.381	1250	1257	1277	rBV	858382	1457178	49.02%	3.798%
12	10.763	1311	1322	1333	rBV	913747	1566132	52.69%	4.082%
13	10.910	1339	1347	1365	rBV	811985	1401827	47.16%	3.654%
14	12.363	1588	1594	1601	rBV2	12708	21324	0.72%	0.056%
15	13.575	1796	1800	1805	rBV3	2223	3575	0.12%	0.009%
16	14.022	1869	1876	1887	rBV	1298039	1768343	59.49%	4.609%
17	14.304	1917	1924	1936	rBV	1500127	2269201	76.34%	5.915%
18	14.610	1968	1976	1988	rBV	1238865	1799044	60.53%	4.689%
19	14.816	2005	2011	2032	rBV	568230	894967	30.11%	2.333%
20	15.034	2046	2048	2053	rVB3	3588	3941	0.13%	0.010%
21	15.604	2136	2145	2155	rBV	1824648	2643194	88.93%	6.889%
22	15.733	2160	2167	2179	rVV	537246	743302	25.01%	1.937%
23	15.845	2182	2186	2190	rVB4	7958	11132	0.37%	0.029%
24	15.969	2203	2207	2209	rBV3	4085	4960	0.17%	0.013%
25	16.480	2290	2294	2300	rBV7	4969	8447	0.28%	0.022%
26	17.122	2397	2403	2408	rBV3	18910	34708	1.17%	0.090%
27	17.233	2418	2422	2425	rBV5	6153	8242	0.28%	0.021%
28	17.275	2425	2429	2434	rVV2	20686	27821	0.94%	0.073%
29	17.369	2438	2445	2452	rVB	1215958	1773917	59.68%	4.624%
30	17.469	2455	2462	2473	rBV	1873796	2649814	89.15%	6.907%
31	17.651	2488	2493	2498	rBV2	7052	11713	0.39%	0.031%
32	17.751	2505	2510	2518	rBV8	5661	14568	0.49%	0.038%
33	17.851	2524	2527	2532	rBV5	4434	6306	0.21%	0.016%
34	17.986	2546	2550	2554	rBV5	2846	4131	0.14%	0.011%
35	18.033	2554	2558	2563	rVB	14440	17968	0.60%	0.047%
36	18.139	2573	2576	2580	rBV6	2346	3118	0.10%	0.008%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
 Data File : BN022365.D
 Acq On : 27 Oct 2022 17:24
 Operator : CG/JU
 Sample : PB148426BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK426

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Title : SVOA CALIBRATION

37	18.257	2592	2596	2601	rBV6	6102	10280	0.35%	0.027%
38	18.339	2605	2610	2620	rVB	44696	64606	2.17%	0.168%
39	18.551	2643	2646	2651	rBV3	8811	11523	0.39%	0.030%
40	18.686	2665	2669	2674	rVB2	28623	34499	1.16%	0.090%
41	19.186	2751	2754	2760	rBV2	8021	11061	0.37%	0.029%
42	19.327	2774	2778	2783	rBV2	23538	38045	1.28%	0.099%
43	19.404	2787	2791	2800	rVV	19914	34883	1.17%	0.091%
44	19.769	2847	2853	2859	rBV	2115235	2743731	92.31%	7.151%
45	20.510	2975	2979	2985	rBV	132610	160907	5.41%	0.419%
46	21.474	3140	3143	3148	rVB	34664	39035	1.31%	0.102%
47	21.568	3154	3159	3165	rBV2	1268093	1657692	55.77%	4.321%
48	23.868	3543	3550	3564	rVB2	1350005	2972338	100.00%	7.747%
49	24.027	3571	3577	3585	rVB2	874583	1739056	58.51%	4.533%




Sum of corrected areas: 38366110

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
Data File : BN022365.D
Acq On : 27 Oct 2022 17:24
Operator : CG/JU
Sample : PB148426BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK426

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

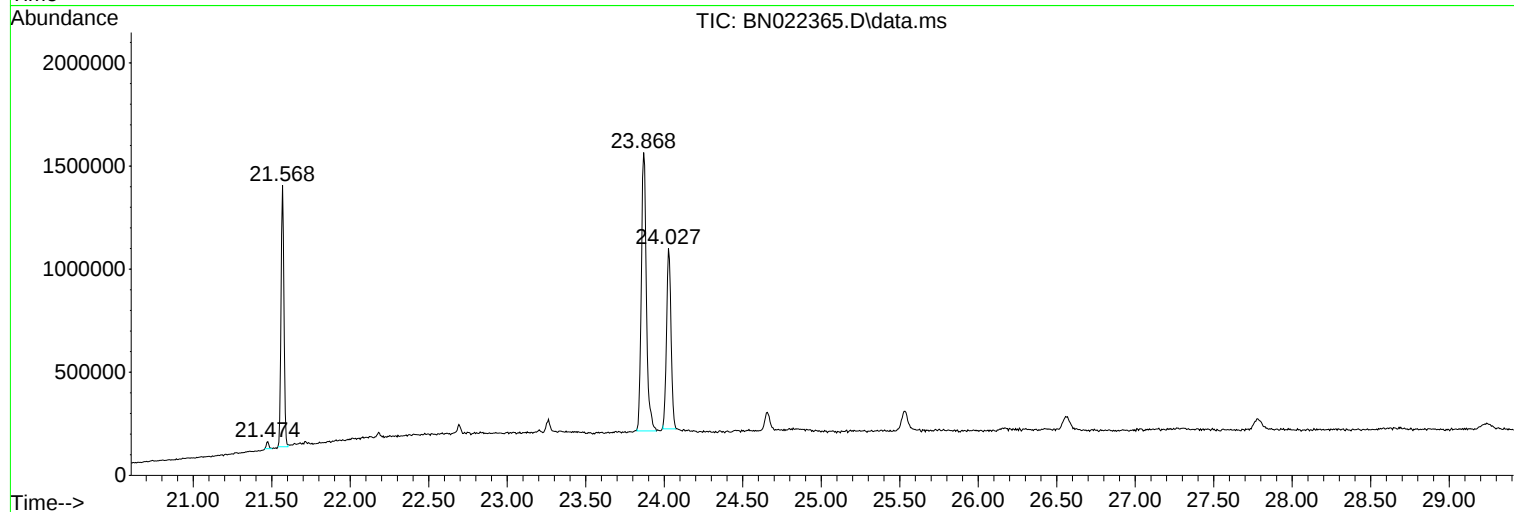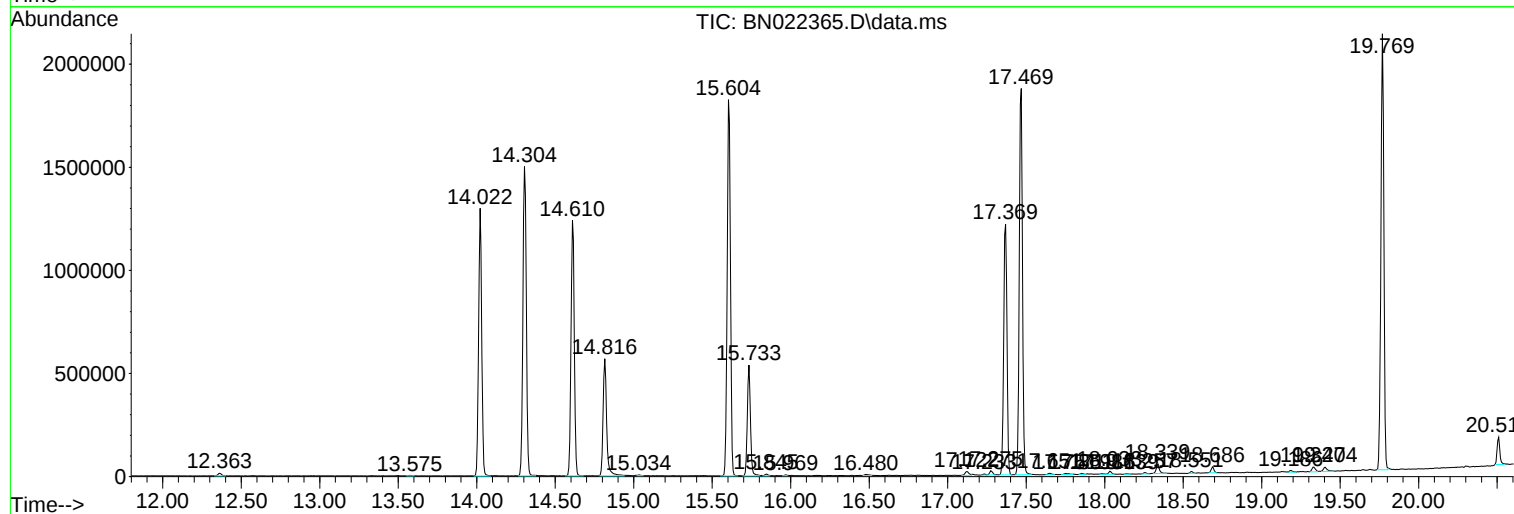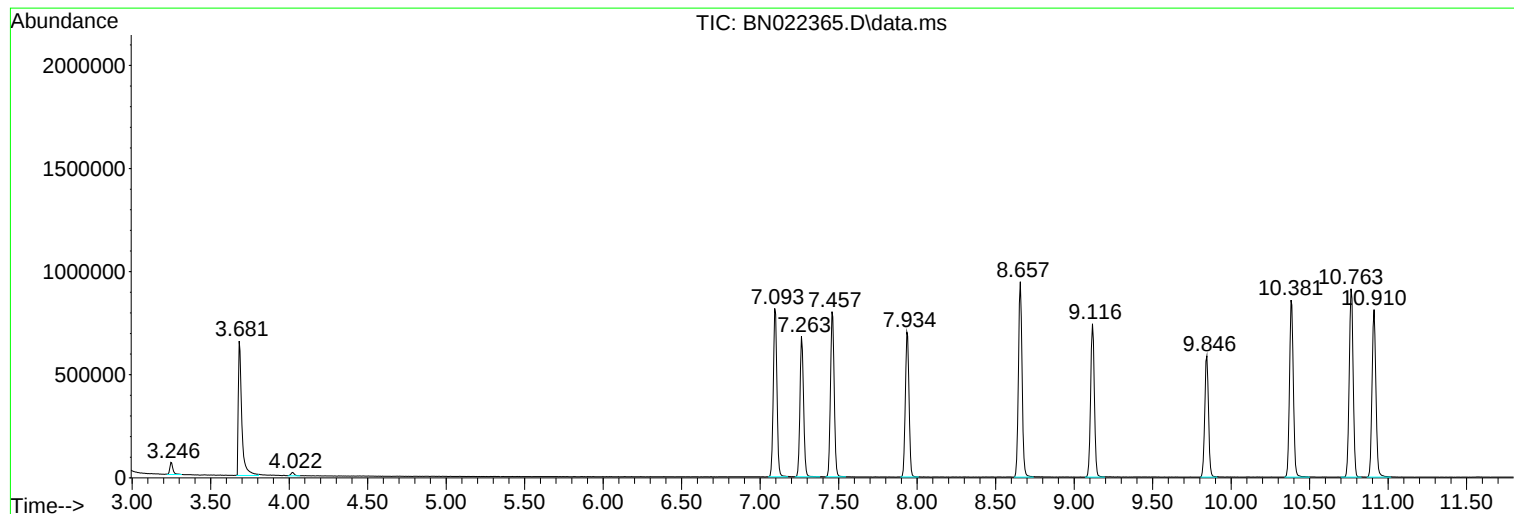

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
Data File : BN022365.D
Acq On : 27 Oct 2022 17:24
Operator : CG/JU
Sample : PB148426BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK426

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
Data File : BN022365.D
Acq On : 27 Oct 2022 17:24
Operator : CG/JU
Sample : PB148426BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK426

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc