

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
 Data File : BN022375.D
 Acq On : 27 Oct 2022 23:38
 Operator : CG/JU
 Sample : N5119-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022375.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	40	44	52	rVB	42298	58384	2.17%	0.183%
2	3.552	93	96	107	rVB	15804	25371	0.94%	0.080%
3	3.699	116	121	133	rBV	71169	110144	4.10%	0.346%
4	3.799	134	138	148	rVV	111428	148940	5.54%	0.468%
5	3.875	148	151	154	rVV	16051	20604	0.77%	0.065%
6	3.922	154	159	164	rVB	45267	71812	2.67%	0.226%
7	4.022	171	176	181	rVB	20468	29073	1.08%	0.091%
8	4.199	202	206	210	rBV4	7524	9863	0.37%	0.031%
9	4.410	238	242	249	rVB	10730	16512	0.61%	0.052%
10	4.604	270	275	283	rVB	29642	43842	1.63%	0.138%
11	4.769	297	303	306	rBV5	5601	9604	0.36%	0.030%
12	4.975	332	338	349	rVB2	25715	59999	2.23%	0.188%
13	5.081	352	356	368	rVB	16386	27321	1.02%	0.086%
14	5.522	427	431	438	rVB	7506	13384	0.50%	0.042%
15	5.898	487	495	501	rBV3	13888	30454	1.13%	0.096%
16	6.398	574	580	585	rBV5	3428	7299	0.27%	0.023%
17	7.093	690	698	712	rVV	565988	955218	35.56%	3.000%
18	7.263	719	727	738	rBV	496823	789310	29.38%	2.479%
19	7.457	753	760	770	rBV	591447	935095	34.81%	2.937%
20	7.540	770	774	777	rVV2	8608	13716	0.51%	0.043%
21	7.745	803	809	817	rBV3	5296	9827	0.37%	0.031%
22	7.934	831	841	849	rVV	580820	920159	34.25%	2.890%
23	7.998	849	852	856	rVV	4747	7308	0.27%	0.023%
24	8.192	879	885	892	rBV3	4136	9848	0.37%	0.031%
25	8.657	957	964	974	rBV	292453	498897	18.57%	1.567%
26	8.775	979	984	992	rVB3	11144	19370	0.72%	0.061%
27	9.116	1034	1042	1049	rBV	517497	884978	32.94%	2.779%
28	9.275	1064	1069	1075	rVB7	4658	9069	0.34%	0.028%
29	9.498	1102	1107	1113	rBV	9903	15048	0.56%	0.047%
30	9.839	1158	1165	1180	rBV	432992	722877	26.91%	2.270%
31	10.381	1250	1257	1266	rVV	593790	978743	36.43%	3.074%
32	10.539	1277	1284	1296	rBV	87290	177972	6.62%	0.559%
33	10.763	1311	1322	1328	rBV	720907	1247152	46.42%	3.917%
34	10.810	1328	1330	1338	rVB	14953	20958	0.78%	0.066%
35	10.904	1338	1346	1366	rBV	407990	756331	28.15%	2.375%
36	12.180	1558	1563	1567	rBV3	7156	10755	0.40%	0.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
 Data File : BN022375.D
 Acq On : 27 Oct 2022 23:38
 Operator : CG/JU
 Sample : N5119-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Title : SVOA CALIBRATION

37	12.357	1587	1593	1598	rVV2	10379	16280	0.61%	0.051%
38	12.428	1598	1605	1613	rVV	13862	22338	0.83%	0.070%
39	12.645	1637	1642	1649	rVV	10537	17355	0.65%	0.055%
40	13.416	1768	1773	1782	rVV2	12233	22804	0.85%	0.072%
41	13.498	1782	1787	1792	rVV3	11052	18018	0.67%	0.057%
42	13.927	1852	1860	1866	rVB6	9855	15934	0.59%	0.050%
43	14.022	1866	1876	1883	rBV	942287	1339345	49.85%	4.206%
44	14.075	1883	1885	1889	rVV3	5708	7112	0.26%	0.022%
45	14.304	1917	1924	1935	rVB	1155661	1703799	63.42%	5.351%
46	14.492	1952	1956	1961	rVB2	9302	12754	0.47%	0.040%
47	14.610	1968	1976	1983	rBV	976158	1459888	54.34%	4.585%
48	14.669	1983	1986	1992	rVB3	6399	10057	0.37%	0.032%
49	14.816	2005	2011	2024	rVV	348298	555468	20.68%	1.744%
50	14.974	2034	2038	2041	rBV2	12825	20523	0.76%	0.064%
51	15.033	2041	2048	2053	rVV2	40517	68508	2.55%	0.215%
52	15.398	2105	2110	2113	rVV	15663	21904	0.82%	0.069%
53	15.445	2113	2118	2123	rVB2	10566	17148	0.64%	0.054%
54	15.604	2138	2145	2151	rBV	1427004	2042278	76.02%	6.414%
55	15.657	2151	2154	2159	rVB	40772	54127	2.01%	0.170%
56	15.727	2161	2166	2180	rBV	296683	430731	16.03%	1.353%
57	15.845	2180	2186	2192	rBV3	8006	12494	0.47%	0.039%
58	15.957	2201	2205	2209	rBV3	6248	10536	0.39%	0.033%
59	16.063	2217	2223	2226	rBV4	5077	8969	0.33%	0.028%
60	16.310	2262	2265	2267	rBV3	11589	15728	0.59%	0.049%
61	16.898	2361	2365	2373	rVB	28396	40026	1.49%	0.126%
62	17.116	2394	2402	2406	rBV5	19746	40623	1.51%	0.128%
63	17.245	2417	2424	2425	rBV5	4937	9629	0.36%	0.030%
64	17.274	2425	2429	2434	rVV2	18664	25115	0.93%	0.079%
65	17.363	2437	2444	2449	rVV	1131628	1566665	58.31%	4.920%
66	17.404	2449	2451	2455	rVV	83726	105811	3.94%	0.332%
67	17.463	2455	2461	2471	rVV2	1319673	1951586	72.64%	6.129%
68	17.563	2474	2478	2483	rVB	34193	48819	1.82%	0.153%
69	17.645	2487	2492	2498	rBV2	8594	17037	0.63%	0.054%
70	17.751	2505	2510	2512	rBV5	8600	14695	0.55%	0.046%
71	17.774	2512	2514	2523	rVB2	11332	16880	0.63%	0.053%
72	17.851	2523	2527	2531	rBV2	11191	13851	0.52%	0.043%
73	17.898	2531	2535	2540	rVB7	6015	11053	0.41%	0.035%
74	18.033	2553	2558	2562	rBV	40337	48726	1.81%	0.153%
75	18.251	2590	2595	2599	rBV2	55910	77887	2.90%	0.245%
76	18.292	2599	2602	2606	rVV	16826	25767	0.96%	0.081%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
 Data File : BN022375.D
 Acq On : 27 Oct 2022 23:38
 Operator : CG/JU
 Sample : N5119-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Title : SVOA CALIBRATION

77	18.333	2606	2609	2614	rVB	37534	47050	1.75%	0.148%
78	18.439	2623	2627	2632	rBV3	17456	30046	1.12%	0.094%
79	18.551	2642	2646	2651	rBV2	18142	23369	0.87%	0.073%
80	18.604	2651	2655	2660	rBV3	14600	26390	0.98%	0.083%
81	18.686	2665	2669	2673	rVV	26702	37630	1.40%	0.118%
82	18.751	2677	2680	2684	rVV2	12685	18463	0.69%	0.058%
83	18.804	2684	2689	2692	rVV7	7891	12108	0.45%	0.038%
84	19.180	2748	2753	2756	rBV4	22510	39753	1.48%	0.125%
85	19.327	2774	2778	2785	rVB4	24946	41855	1.56%	0.131%
86	19.398	2786	2790	2791	rBV2	25411	29002	1.08%	0.091%
87	19.427	2791	2795	2802	rVB	226158	318482	11.85%	1.000%
88	19.533	2809	2813	2817	rBV7	20866	30724	1.14%	0.096%
89	19.768	2847	2853	2866	rVB	1712751	2686592	100.00%	8.437%
90	20.298	2939	2943	2947	rVB2	41806	58304	2.17%	0.183%
91	20.392	2956	2959	2962	rVB	20987	24733	0.92%	0.078%
92	20.504	2974	2978	2984	rBV	120341	152293	5.67%	0.478%
93	20.798	3025	3028	3031	rBV	30930	34296	1.28%	0.108%
94	21.262	3104	3107	3116	rVB5	101736	189231	7.04%	0.594%
95	21.468	3139	3142	3145	rVB2	54140	58970	2.19%	0.185%
96	21.562	3152	3158	3163	rBV	1335940	1897899	70.64%	5.960%
97	21.604	3163	3165	3168	rVB	94873	105690	3.93%	0.332%
98	23.262	3443	3447	3452	rBV2	139970	288494	10.74%	0.906%
99	23.862	3542	3549	3555	rBV2	1137634	2321162	86.40%	7.290%
100	24.021	3570	3576	3584	rVB	847123	1786195	66.49%	5.610%



Sum of corrected areas: 31842236

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
Data File : BN022375.D
Acq On : 27 Oct 2022 23:38
Operator : CG/JU
Sample : N5119-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

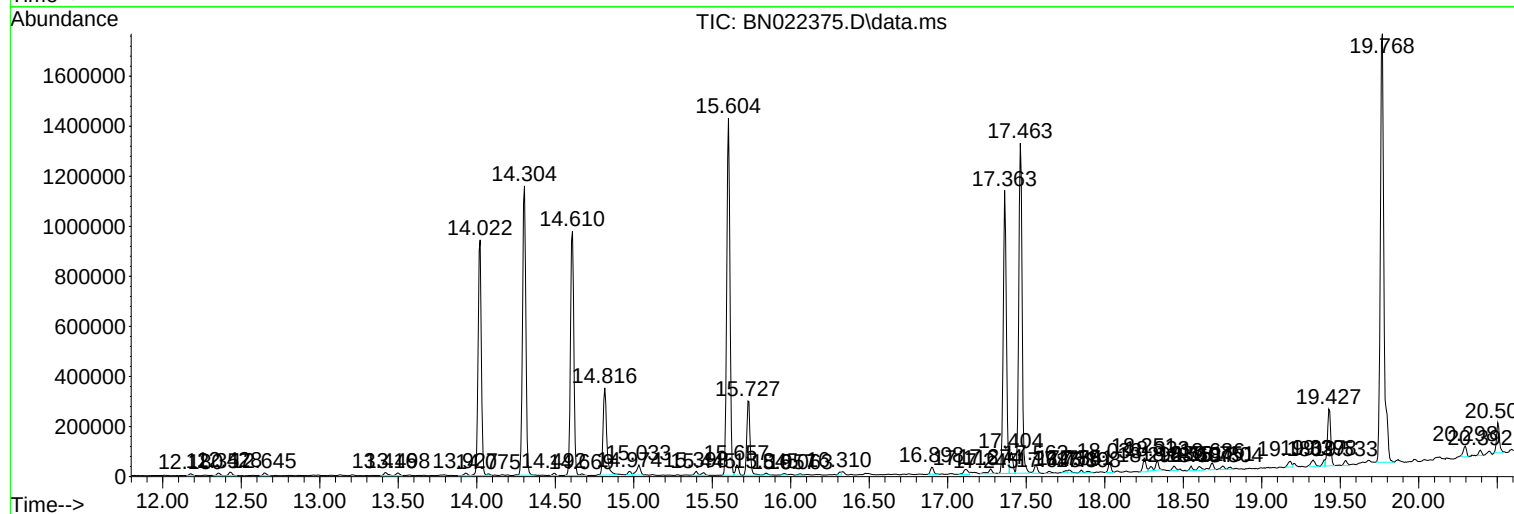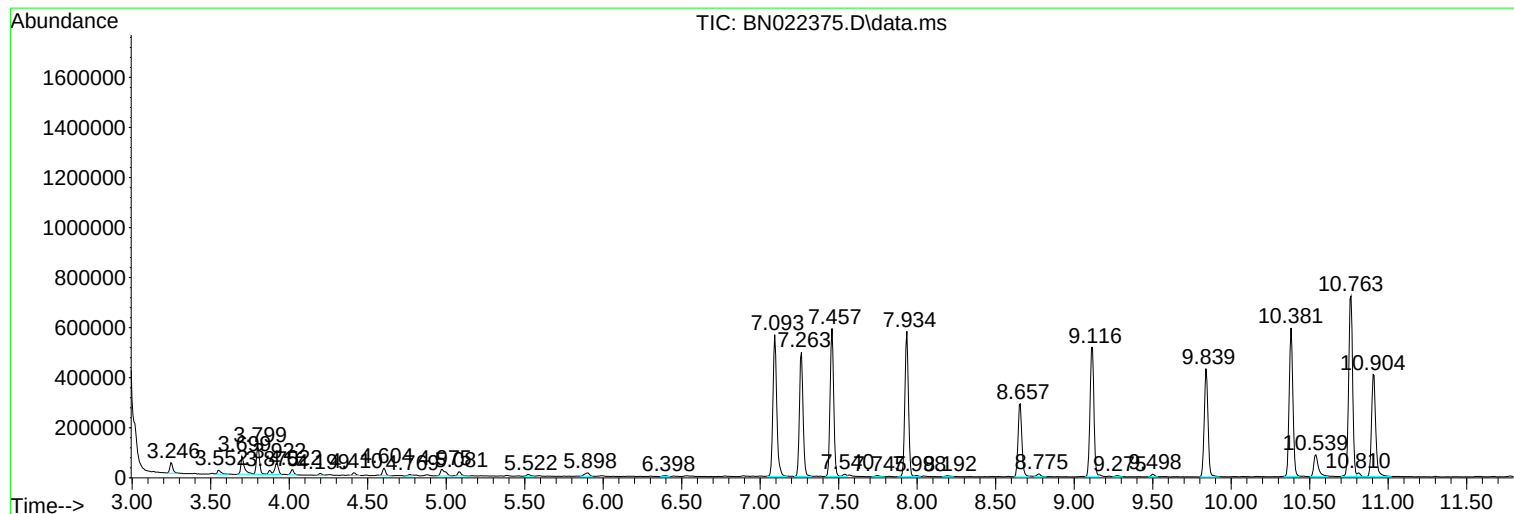

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
Data File : BN022375.D
Acq On : 27 Oct 2022 23:38
Operator : CG/JU
Sample : N5119-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BC3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.799	3.24 ng/ul	148940	1,4-Dichlorobenzene-d4	7.934

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pyrrolidinone			85	C4H7NO	000616-45-5	38
2	Methacrylamide			85	C4H7NO	000079-39-0	36
3	2-Pyrrolidinone			85	C4H7NO	000616-45-5	9
4	2-Pyrrolidinone			85	C4H7NO	000616-45-5	9
5	2-Pyrrolidinone			85	C4H7NO	000616-45-5	9

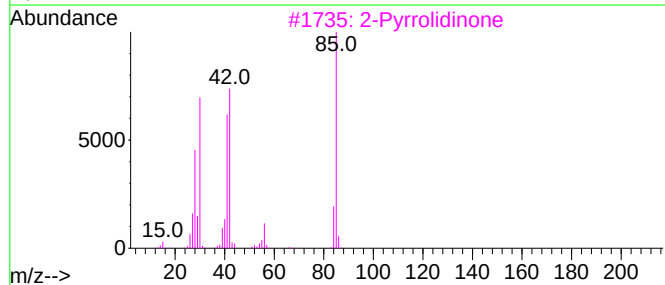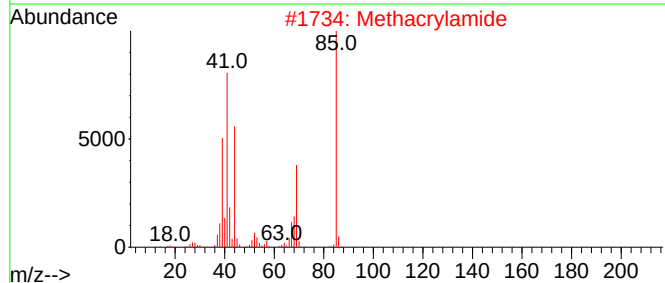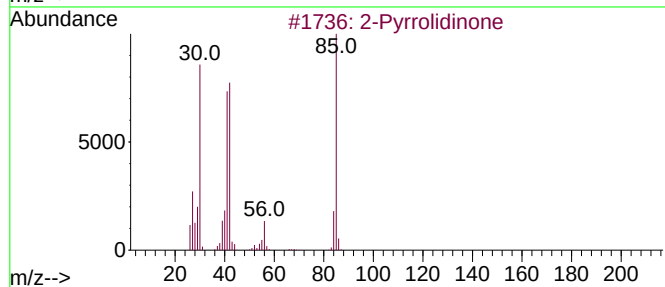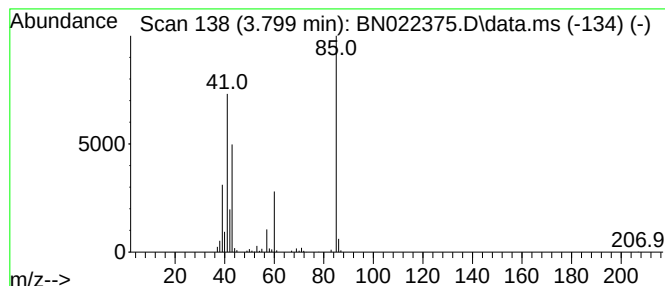

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
Data File : BN022375.D
Acq On : 27 Oct 2022 23:38
Operator : CG/JU
Sample : N5119-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BC3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.539	2.85 ng/ul	177972	Naphthalene-d8	10.763

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	83
3			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	83
4			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	83
5			Ethylene glycol monoisobutyl ether	118	C6H14O2	004439-24-1	64

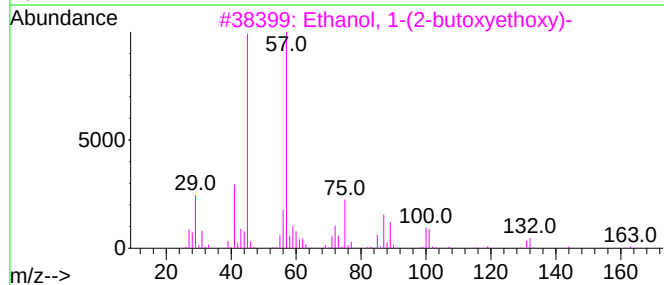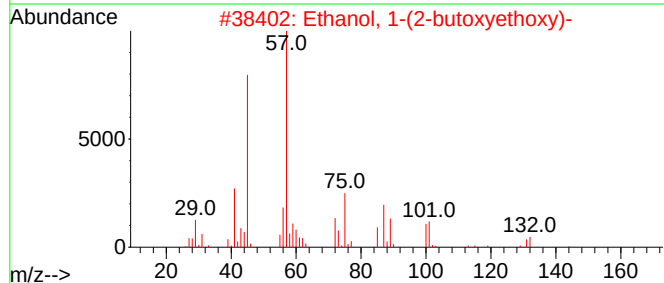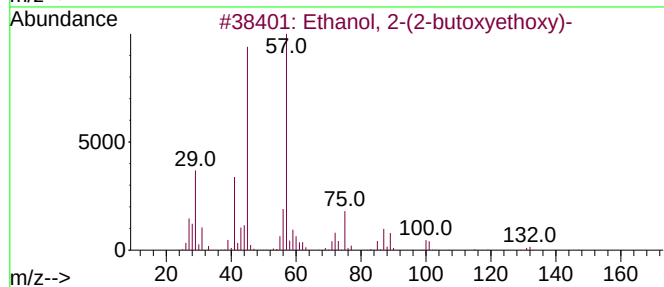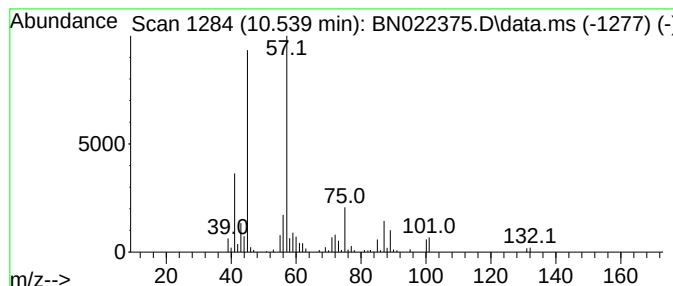

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
Data File : BN022375.D
Acq On : 27 Oct 2022 23:38
Operator : CG/JU
Sample : N5119-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	3.799	3.2	ng/ul	148940	1	7.934	920159	20.0
Ethanol, 2-(2-b...	10.539	2.9	ng/ul	177972	2	10.763	1247150	20.0