

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
 Data File : BN022376.D
 Acq On : 28 Oct 2022 00:15
 Operator : CG/JU
 Sample : N5119-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BC4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022376.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	40	44	56	rVB	34464	51804	2.65%	0.199%
2	3.552	93	96	106	rVB	14710	23257	1.19%	0.089%
3	3.699	117	121	134	rBV	77409	121491	6.21%	0.468%
4	3.799	134	138	147	rVV	101037	132178	6.76%	0.509%
5	3.875	147	151	154	rVV	15605	20205	1.03%	0.078%
6	3.922	154	159	164	rVB	42491	66081	3.38%	0.254%
7	4.017	171	175	180	rVB	15448	20924	1.07%	0.081%
8	4.199	202	206	210	rBV3	5863	8956	0.46%	0.034%
9	4.258	212	216	222	rVB4	8853	13226	0.68%	0.051%
10	4.411	238	242	248	rVB2	11059	14584	0.75%	0.056%
11	4.605	271	275	283	rVB	17933	25327	1.30%	0.097%
12	4.687	285	289	293	rBV2	4209	6960	0.36%	0.027%
13	4.769	300	303	308	rBV4	4009	6874	0.35%	0.026%
14	4.869	318	320	328	rVB5	3617	5993	0.31%	0.023%
15	4.975	333	338	349	rVB2	25378	49902	2.55%	0.192%
16	5.081	353	356	366	rVB	12729	20126	1.03%	0.077%
17	5.246	381	384	389	rVB7	3419	4666	0.24%	0.018%
18	5.587	438	442	449	rBV4	2534	4465	0.23%	0.017%
19	7.093	690	698	712	rBV	456180	761265	38.93%	2.929%
20	7.258	720	726	739	rVB	397213	640839	32.77%	2.466%
21	7.458	753	760	770	rBV	473363	756158	38.67%	2.910%
22	7.540	770	774	786	rVB8	5972	14689	0.75%	0.057%
23	7.752	804	810	814	rBV3	4295	7421	0.38%	0.029%
24	7.934	834	841	848	rBV	589608	933465	47.74%	3.592%
25	7.993	848	851	856	rVB3	4132	5807	0.30%	0.022%
26	8.199	879	886	889	rBV5	2922	5681	0.29%	0.022%
27	8.652	957	963	973	rBV	215594	359833	18.40%	1.385%
28	8.775	979	984	989	rVB	8778	14328	0.73%	0.055%
29	9.110	1034	1041	1054	rBV	429386	712148	36.42%	2.740%
30	9.269	1065	1068	1074	rBV5	4218	6254	0.32%	0.024%
31	9.499	1101	1107	1112	rBV2	8127	13553	0.69%	0.052%
32	9.840	1158	1165	1180	rBV	347864	576765	29.50%	2.219%
33	10.328	1243	1248	1250	rBV2	3559	4927	0.25%	0.019%
34	10.381	1250	1257	1267	rVV	462223	781481	39.97%	3.007%
35	10.540	1277	1284	1301	rBV	75023	160926	8.23%	0.619%
36	10.763	1311	1322	1329	rBV	725016	1249170	63.89%	4.807%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
 Data File : BN022376.D
 Acq On : 28 Oct 2022 00:15
 Operator : CG/JU
 Sample : N5119-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BC4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Title : SVOA CALIBRATION

37	10.904	1338	1346	1365	rBV	368892	655105	33.50%	2.521%
38	11.299	1407	1413	1421	rVB4	5685	10142	0.52%	0.039%
39	12.175	1559	1562	1569	rVB6	3753	6253	0.32%	0.024%
40	12.269	1574	1578	1584	rVV3	3708	7384	0.38%	0.028%

41	12.357	1587	1593	1598	rVB2	7947	13437	0.69%	0.052%
42	13.216	1733	1739	1741	rBV6	2628	4465	0.23%	0.017%
43	13.416	1768	1773	1779	rBV2	6530	10734	0.55%	0.041%
44	13.493	1779	1786	1792	rVV2	17127	30855	1.58%	0.119%
45	13.934	1856	1861	1866	rVB5	4705	6963	0.36%	0.027%

46	14.016	1866	1875	1889	rBV	744856	1059426	54.18%	4.077%
47	14.304	1917	1924	1933	rVB	886720	1320521	67.54%	5.082%
48	14.492	1952	1956	1962	rVB3	5591	7959	0.41%	0.031%
49	14.610	1969	1976	1983	rBV	976747	1453230	74.32%	5.592%
50	14.663	1983	1985	1993	rVB4	3467	6582	0.34%	0.025%

51	14.769	1998	2003	2005	rBV4	2882	4460	0.23%	0.017%
52	14.816	2005	2011	2025	rBV	254958	412975	21.12%	1.589%
53	14.969	2033	2037	2042	rBV2	10664	16228	0.83%	0.062%
54	15.034	2042	2048	2054	rVB3	38918	62094	3.18%	0.239%
55	15.445	2113	2118	2125	rVB3	6297	10161	0.52%	0.039%

56	15.604	2138	2145	2151	rBV	1157070	1618685	82.79%	6.229%
57	15.657	2151	2154	2158	rVB	13704	17180	0.88%	0.066%
58	15.728	2161	2166	2175	rBV	229797	322800	16.51%	1.242%
59	15.839	2182	2185	2190	rBV3	4853	7020	0.36%	0.027%
60	15.963	2201	2206	2209	rBV4	4049	5975	0.31%	0.023%

61	16.057	2218	2222	2227	rVB7	3008	4709	0.24%	0.018%
62	16.151	2234	2238	2246	rVB8	2582	5898	0.30%	0.023%
63	16.316	2261	2266	2271	rVB5	4417	8417	0.43%	0.032%
64	16.475	2289	2293	2308	rVB5	6967	17736	0.91%	0.068%
65	16.751	2337	2340	2346	rVB5	2921	4662	0.24%	0.018%

66	16.898	2361	2365	2371	rVB2	21727	29312	1.50%	0.113%
67	17.122	2397	2403	2407	rBV3	16184	29982	1.53%	0.115%
68	17.234	2418	2422	2424	rBV4	5007	7148	0.37%	0.028%
69	17.275	2425	2429	2434	rVV2	18735	26149	1.34%	0.101%
70	17.363	2438	2444	2449	rVV	1139613	1549022	79.22%	5.961%

71	17.404	2449	2451	2455	rVV	28908	38541	1.97%	0.148%
72	17.463	2455	2461	2471	rVV2	1066911	1526303	78.06%	5.873%
73	17.563	2474	2478	2484	rVB2	27984	38188	1.95%	0.147%
74	17.651	2489	2493	2497	rBV2	6315	10648	0.54%	0.041%
75	17.751	2506	2510	2513	rBV6	4544	7142	0.37%	0.027%

76	17.851	2524	2527	2531	rBV4	4152	5214	0.27%	0.020%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
 Data File : BN022376.D
 Acq On : 28 Oct 2022 00:15
 Operator : CG/JU
 Sample : N5119-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BC4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Title : SVOA CALIBRATION

77	18.033	2553	2558	2565	rVV	37394	48688	2.49%	0.187%
78	18.133	2572	2575	2582	rVB8	5861	8404	0.43%	0.032%
79	18.251	2591	2595	2599	rBV2	55853	73838	3.78%	0.284%
80	18.333	2605	2609	2615	rBV	35020	45783	2.34%	0.176%
81	18.445	2624	2628	2631	rBV5	5606	7893	0.40%	0.030%
82	18.551	2642	2646	2650	rBV4	9647	13441	0.69%	0.052%
83	18.604	2651	2655	2660	rVV4	7534	13240	0.68%	0.051%
84	18.680	2665	2668	2674	rVV	26186	35702	1.83%	0.137%
85	18.757	2678	2681	2685	rVB6	6501	8896	0.45%	0.034%
86	19.180	2750	2753	2755	rBV4	13202	15725	0.80%	0.061%
87	19.204	2755	2757	2763	rVB4	21785	25894	1.32%	0.100%
88	19.328	2774	2778	2784	rVB4	17162	30845	1.58%	0.119%
89	19.398	2786	2790	2791	rVV	17322	20775	1.06%	0.080%
90	19.428	2791	2795	2802	rVB	72080	102749	5.25%	0.395%
91	19.533	2810	2813	2821	rBV3	23882	32660	1.67%	0.126%
92	19.763	2846	2852	2864	rBV	1348816	1893091	96.82%	7.285%
93	20.292	2940	2942	2946	rVB2	22714	26084	1.33%	0.100%
94	20.504	2973	2978	2986	rBV	118830	158465	8.10%	0.610%
95	20.792	3025	3027	3031	rVB	19087	18633	0.95%	0.072%
96	21.263	3104	3107	3116	rVB4	74018	108945	5.57%	0.419%
97	21.469	3139	3142	3145	rBV2	38597	41228	2.11%	0.159%
98	21.563	3152	3158	3163	rBV	1235533	1654677	84.63%	6.367%
99	23.857	3542	3548	3564	rVB2	860609	1955275	100.00%	7.524%
100	24.021	3569	3576	3586	rVB2	830810	1663927	85.10%	6.403%


Sum of corrected areas: 25986292

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
Data File : BN022376.D
Acq On : 28 Oct 2022 00:15
Operator : CG/JU
Sample : N5119-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BC4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

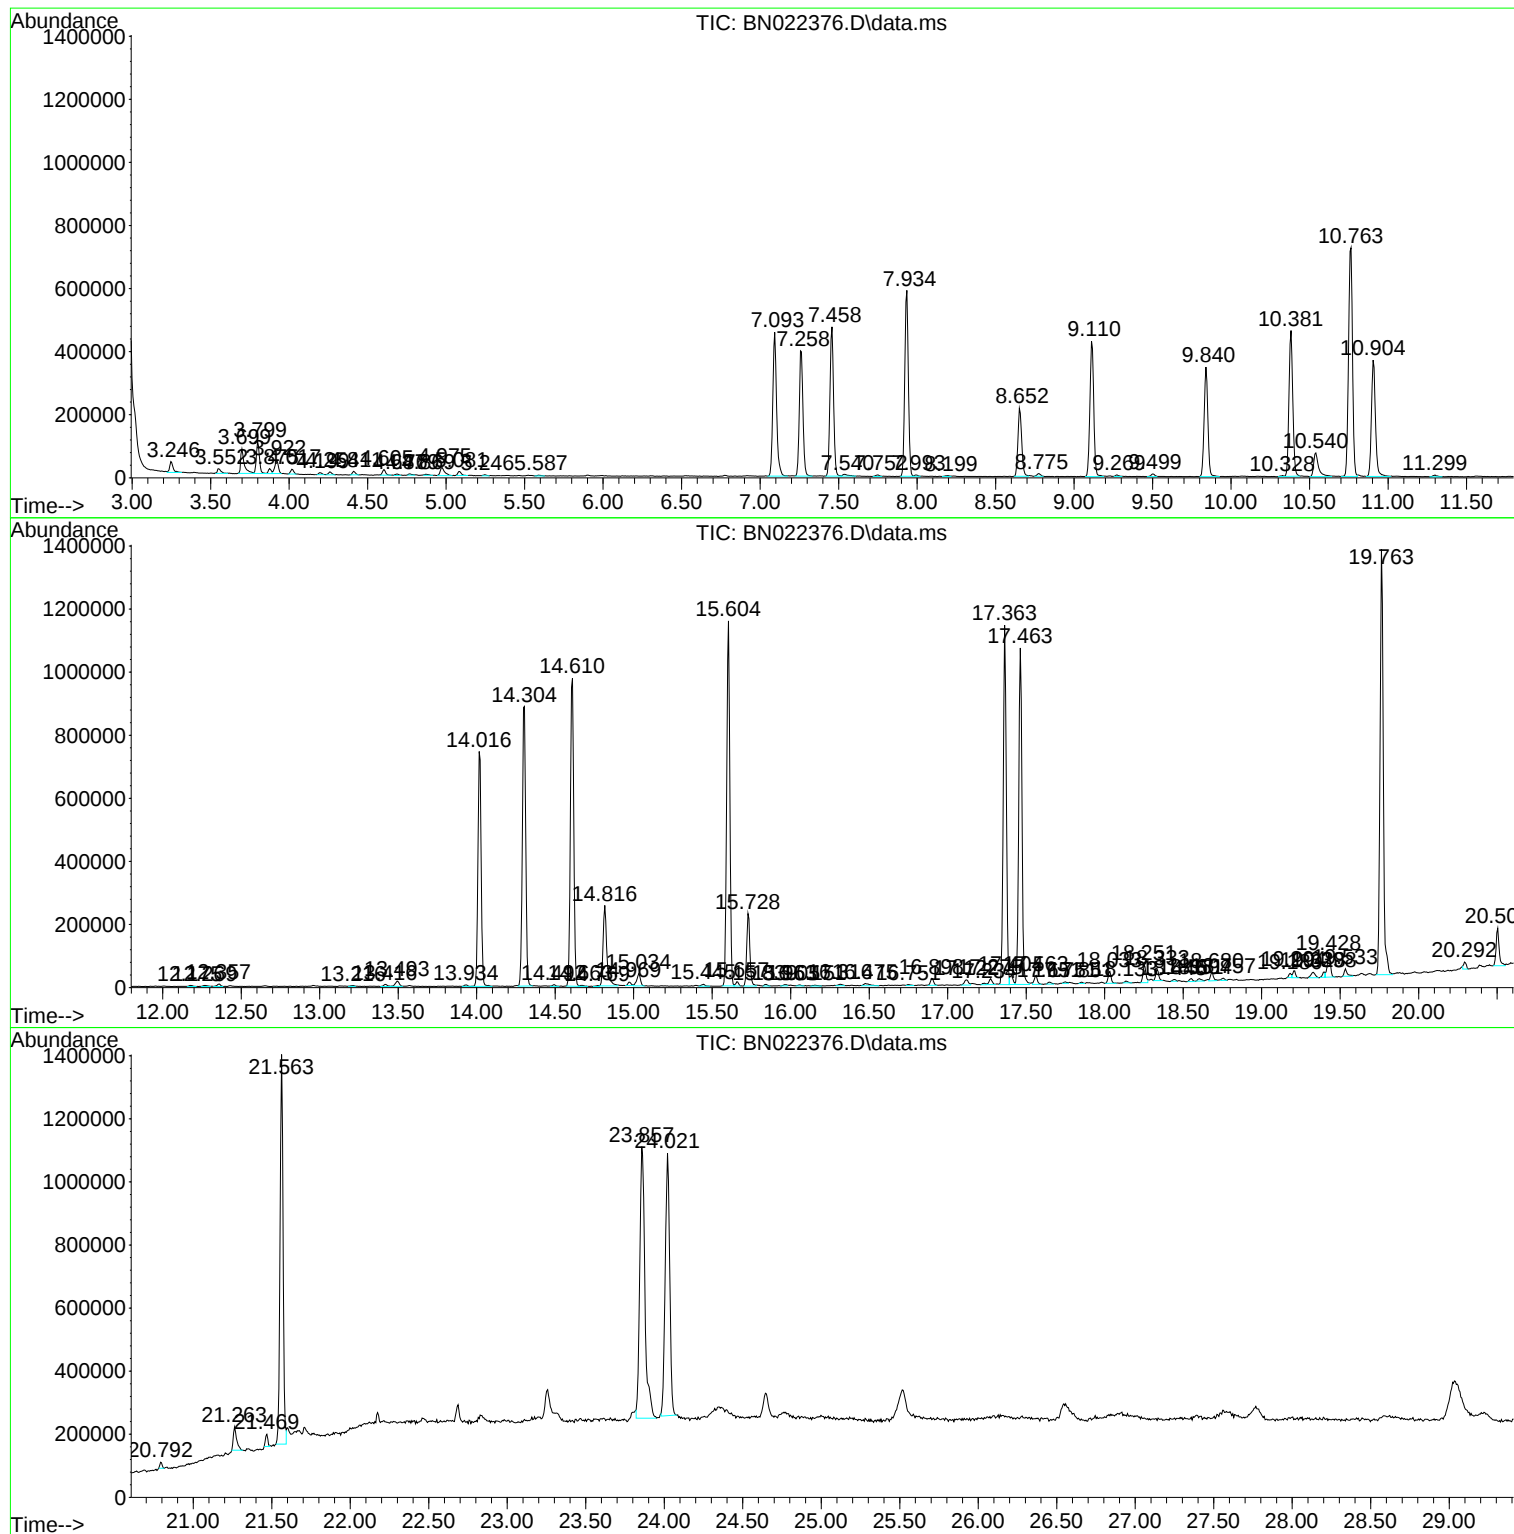

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
Data File : BN022376.D
Acq On : 28 Oct 2022 00:15
Operator : CG/JU
Sample : N5119-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BC4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.799	2.83 ng/ul	132178	1,4-Dichlorobenzene-d4	7.934

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Oxirane, (2-methylpropyl)-		100	C6H12O		023850-78-4	36
2	2-Pyrrolidinone		85	C4H7NO		000616-45-5	28
3	(S)-(-)-1-Amino-2-(methoxymethyl)-		130	C6H14N2O		059983-39-0	23
4	3-Aminopyrrolidine		86	C4H10N2		079286-79-6	9
5	Isobutylene epoxide		72	C4H8O		000558-30-5	9

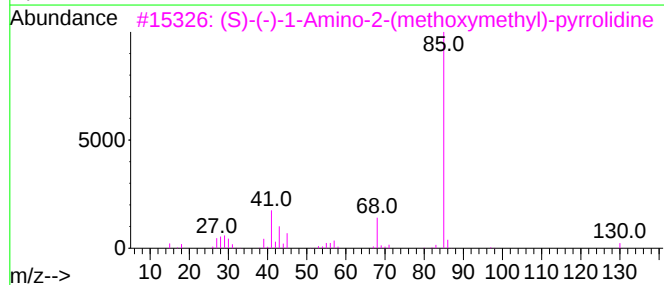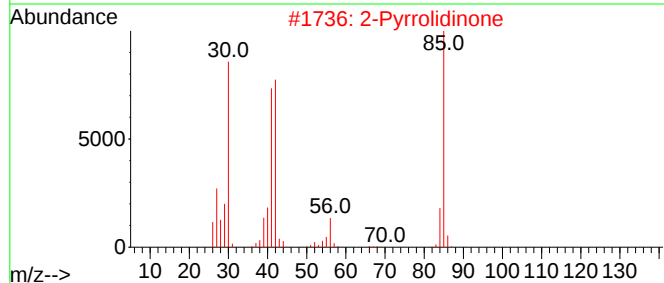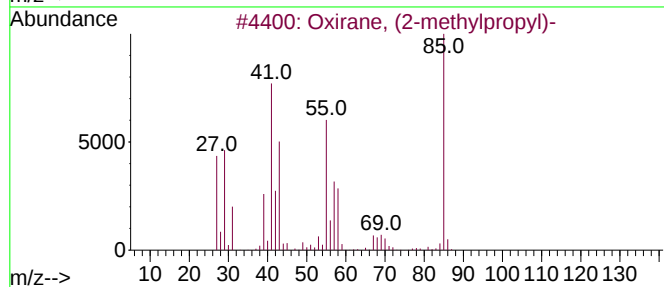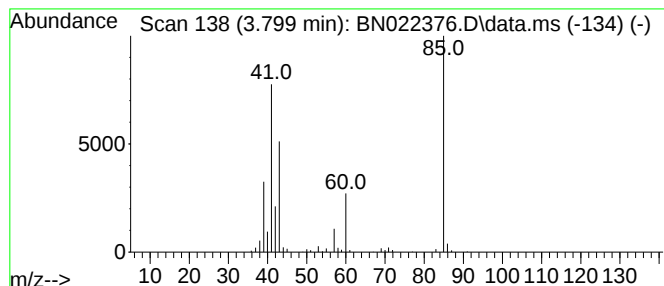

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
Data File : BN022376.D
Acq On : 28 Oct 2022 00:15
Operator : CG/JU
Sample : N5119-03
Misc :
ALS Vial : 15 Sample Multiplier: 1










Instrument :
BNA_N
ClientSampleId :
C0BC4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.	
10.540	2.58 ng/ul	160926	Naphthalene-d8	10.763	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2	Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
3	Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
4	Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	72
5	Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	58

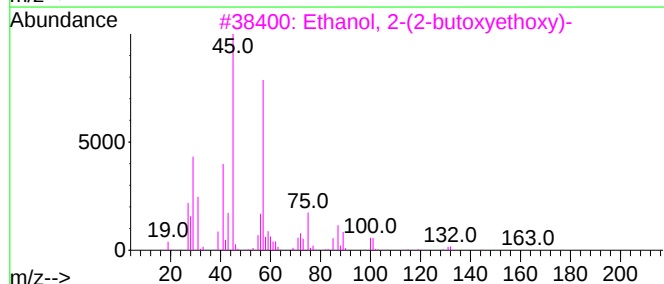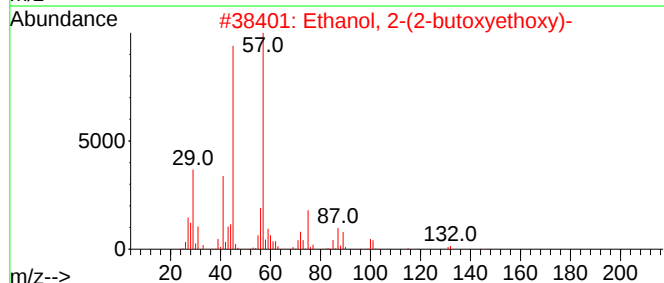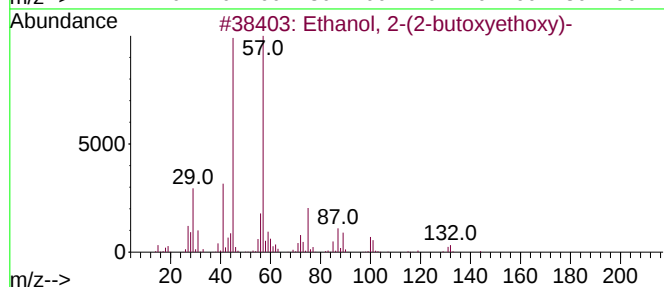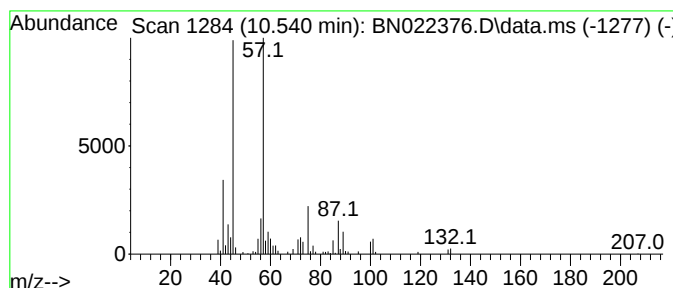

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
Data File : BN022376.D
Acq On : 28 Oct 2022 00:15
Operator : CG/JU
Sample : N5119-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BC4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	3.799	2.8	ng/ul	132178	1	7.934	933465	20.0
Ethanol, 2-(2-b...	10.540	2.6	ng/ul	160926	2	10.763	1249170	20.0