

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
 Data File : BN022381.D
 Acq On : 28 Oct 2022 12:49
 Operator : CG/JU
 Sample : PB148509BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK509

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022381.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	38	42	52	rVB	55649	76299	2.01%	0.180%
2	3.681	116	118	138	rBV	120742	202723	5.33%	0.477%
3	4.011	169	174	179	rVB	12590	17752	0.47%	0.042%
4	5.158	365	369	373	rBV4	2537	3927	0.10%	0.009%
5	7.087	690	697	716	rVB	827434	1334085	35.09%	3.141%
6	7.252	719	725	734	rBV	696261	1118996	29.43%	2.635%
7	7.452	751	759	774	rBV	825593	1329591	34.97%	3.130%
8	7.928	831	840	849	rBV	600156	976751	25.69%	2.300%
9	8.646	952	962	975	rBV	1030750	1689838	44.45%	3.979%
10	9.104	1032	1040	1053	rBV	815000	1357177	35.70%	3.195%
11	9.834	1156	1164	1172	rBV	694602	1139275	29.97%	2.682%
12	10.375	1245	1256	1273	rBV	977426	1676637	44.10%	3.947%
13	10.757	1313	1321	1330	rBV	889569	1504770	39.58%	3.543%
14	10.910	1338	1347	1357	rBV	18656	39167	1.03%	0.092%
15	11.563	1451	1458	1464	rBV4	2362	5367	0.14%	0.013%
16	11.928	1512	1520	1528	rBV5	3150	9030	0.24%	0.021%
17	12.351	1587	1592	1600	rVB	17130	28116	0.74%	0.066%
18	13.492	1780	1786	1791	rVB3	4094	6370	0.17%	0.015%
19	13.569	1795	1799	1804	rBV3	2567	4332	0.11%	0.010%
20	13.863	1845	1849	1853	rBV4	3144	5058	0.13%	0.012%
21	14.016	1868	1875	1884	rBV	1844490	2535822	66.70%	5.970%
22	14.298	1916	1923	1933	rBV	2059934	3081038	81.04%	7.254%
23	14.604	1968	1975	1984	rVB	1403137	2044508	53.78%	4.814%
24	14.810	2003	2010	2033	rBV	853338	1304995	34.32%	3.072%
25	15.016	2040	2045	2047	rBV4	3032	3960	0.10%	0.009%
26	15.598	2137	2144	2152	rBV	2651346	3690269	97.06%	8.688%
27	15.728	2159	2166	2179	rBV	863313	1200486	31.58%	2.826%
28	15.839	2181	2185	2190	rVB	11658	16633	0.44%	0.039%
29	16.381	2274	2277	2282	rBV5	2995	4351	0.11%	0.010%
30	17.110	2398	2401	2404	rBV3	3147	4292	0.11%	0.010%
31	17.145	2404	2407	2411	rVB2	2375	3898	0.10%	0.009%
32	17.357	2437	2443	2450	rBV	1569647	2225976	58.55%	5.241%
33	17.463	2454	2461	2477	rVV2	2615916	3801899	100.00%	8.951%
34	17.739	2505	2508	2513	rBV3	3094	5093	0.13%	0.012%
35	18.027	2553	2557	2562	rVB4	6250	9154	0.24%	0.022%
36	18.251	2590	2595	2600	rBV2	16834	27871	0.73%	0.066%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
 Data File : BN022381.D
 Acq On : 28 Oct 2022 12:49
 Operator : CG/JU
 Sample : PB148509BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK509

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Title : SVOA CALIBRATION

37	18.327	2605	2608	2618	rVB	12006	19760	0.52%	0.047%
38	18.680	2664	2668	2672	rBV4	7979	9416	0.25%	0.022%
39	19.327	2773	2778	2783	rBV2	30100	45535	1.20%	0.107%
40	19.392	2786	2789	2795	rVV	26513	37427	0.98%	0.088%
41	19.533	2810	2813	2820	rBV7	7119	10525	0.28%	0.025%
42	19.763	2846	2852	2859	rBV	2625436	3653515	96.10%	8.602%
43	20.504	2974	2978	2983	rBV	59438	75565	1.99%	0.178%
44	21.563	3152	3158	3163	rBV	1357457	1776758	46.73%	4.183%
45	23.857	3540	3548	3563	rVB2	1270977	2836459	74.61%	6.678%
46	24.015	3568	3575	3585	rVB	732235	1523473	40.07%	3.587%




Sum of corrected areas: 42473939

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
Data File : BN022381.D
Acq On : 28 Oct 2022 12:49
Operator : CG/JU
Sample : PB148509BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK509

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

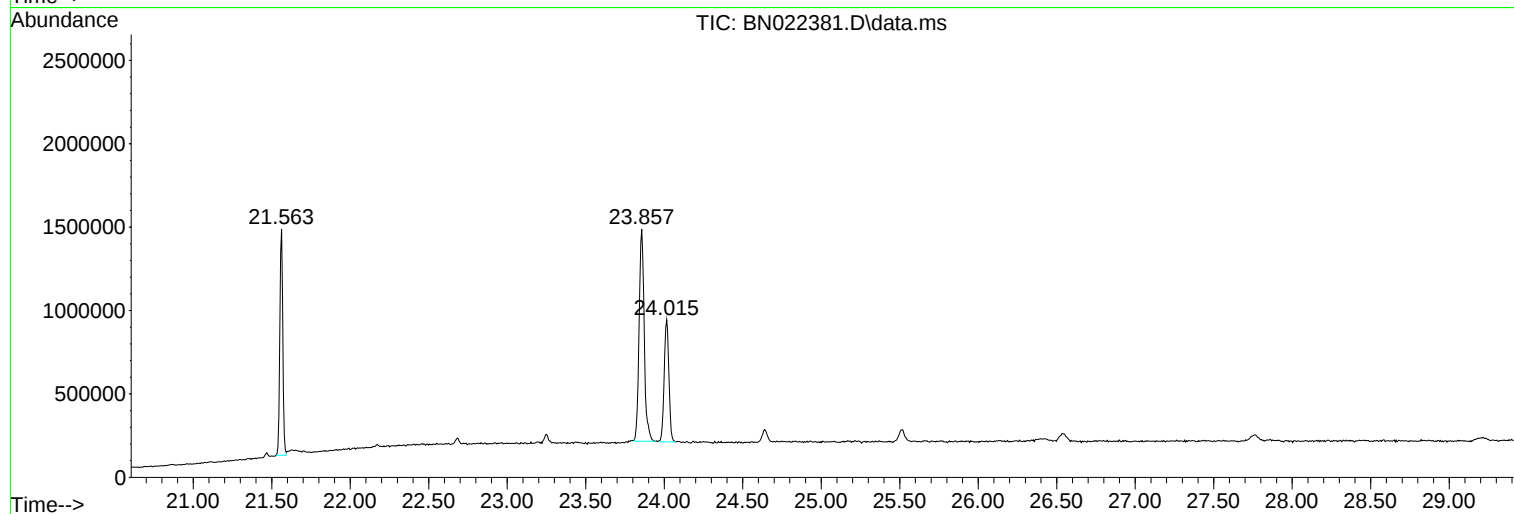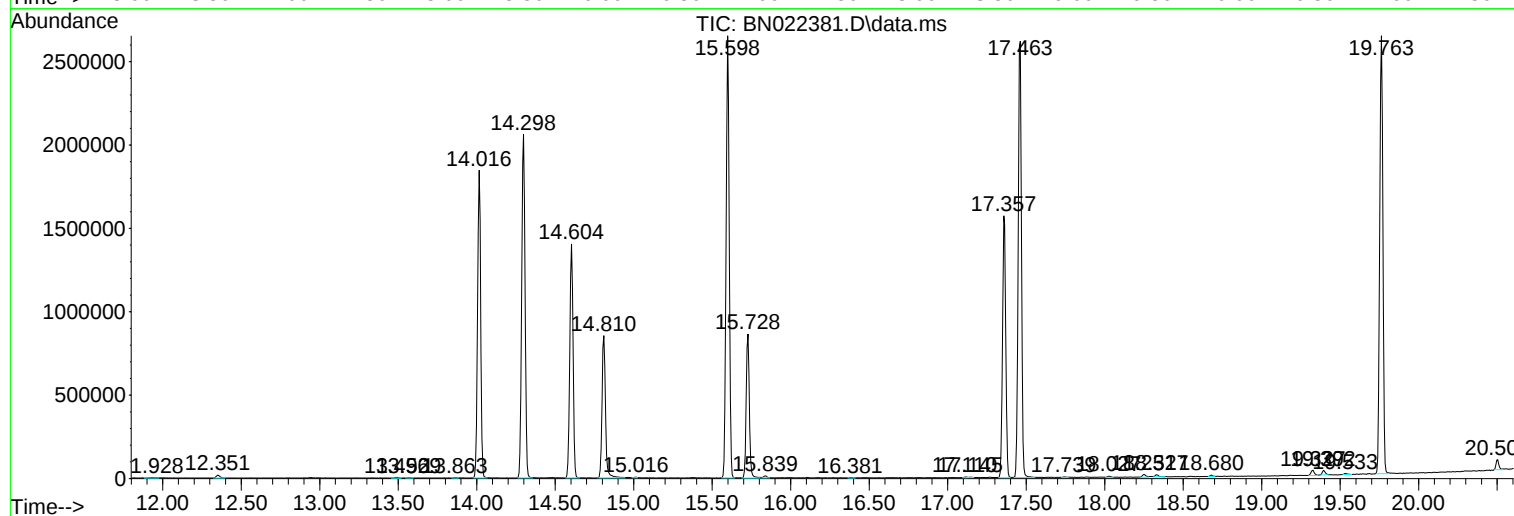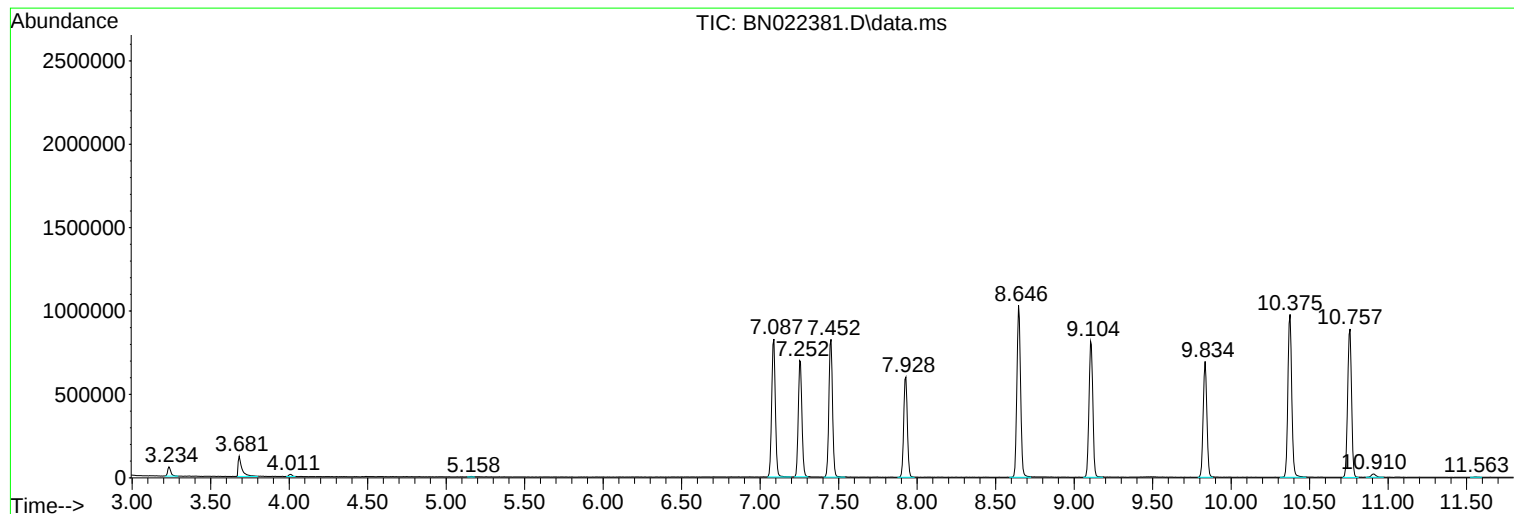

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
Data File : BN022381.D
Acq On : 28 Oct 2022 12:49
Operator : CG/JU
Sample : PB148509BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK509

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
Data File : BN022381.D
Acq On : 28 Oct 2022 12:49
Operator : CG/JU
Sample : PB148509BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK509

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc