

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
 Data File : BN022383.D
 Acq On : 28 Oct 2022 14:04
 Operator : CG/JU
 Sample : N5216-18
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHA84

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022383.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	38	42	48	rBV	25203	34923	1.55%	0.207%
2	3.687	116	119	134	rBV	46878	92702	4.11%	0.550%
3	3.905	154	156	161	rVB4	3383	4803	0.21%	0.028%
4	4.005	169	173	181	rVB	12138	17518	0.78%	0.104%
5	4.246	211	214	218	rBV3	1815	2993	0.13%	0.018%
6	5.175	368	372	378	rVB3	3577	6032	0.27%	0.036%
7	7.087	690	697	707	rVB	85314	141005	6.25%	0.837%
8	7.252	719	725	733	rBV	135605	221061	9.80%	1.312%
9	7.452	753	759	768	rBV	133326	213764	9.48%	1.268%
10	7.928	832	840	850	rBV	575149	927181	41.11%	5.501%
11	8.646	956	962	975	rBV	131378	223841	9.92%	1.328%
12	9.105	1033	1040	1052	rBV	146703	253923	11.26%	1.507%
13	9.499	1105	1107	1114	rVB4	3065	3951	0.18%	0.023%
14	9.834	1157	1164	1175	rBV	112563	191733	8.50%	1.138%
15	10.075	1203	1205	1211	rBV5	1250	2258	0.10%	0.013%
16	10.375	1249	1256	1271	rBV	165783	290066	12.86%	1.721%
17	10.546	1279	1285	1297	rBV3	10232	28078	1.24%	0.167%
18	10.752	1313	1320	1331	rBV	822888	1429902	63.40%	8.484%
19	10.899	1337	1345	1355	rBV	116579	216668	9.61%	1.286%
20	11.563	1452	1458	1460	rBV4	1596	2725	0.12%	0.016%
21	11.940	1515	1522	1523	rBV6	2605	4665	0.21%	0.028%
22	12.357	1588	1593	1597	rBV3	3024	4872	0.22%	0.029%
23	13.493	1781	1786	1791	rBV2	14840	23246	1.03%	0.138%
24	13.863	1846	1849	1854	rBV3	3402	4558	0.20%	0.027%
25	14.016	1867	1875	1886	rBV	370704	544331	24.13%	3.230%
26	14.298	1916	1923	1933	rBV2	404912	604062	26.78%	3.584%
27	14.469	1947	1952	1954	rBV3	2353	4014	0.18%	0.024%
28	14.604	1968	1975	1986	rBV	1369687	2025995	89.83%	12.021%
29	14.816	2005	2011	2020	rBV	55221	109171	4.84%	0.648%
30	14.893	2022	2024	2029	rVB5	2298	2972	0.13%	0.018%
31	15.010	2041	2044	2048	rBV5	2373	3878	0.17%	0.023%
32	15.369	2099	2105	2108	rBV4	1912	3989	0.18%	0.024%
33	15.598	2138	2144	2151	rBV	603094	818827	36.30%	4.859%
34	15.728	2160	2166	2176	rVB	116326	169619	7.52%	1.006%
35	15.863	2184	2189	2194	rBV	57233	75552	3.35%	0.448%
36	15.969	2201	2207	2210	rBV4	1557	2527	0.11%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
 Data File : BN022383.D
 Acq On : 28 Oct 2022 14:04
 Operator : CG/JU
 Sample : N5216-18
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHA84

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
 Title : SVOA CALIBRATION

37	16.116	2226	2232	2236	rBV5	1627	3379	0.15%	0.020%
38	16.316	2262	2266	2271	rVB5	1404	2306	0.10%	0.014%
39	16.487	2293	2295	2300	rVB6	1542	2486	0.11%	0.015%
40	17.116	2398	2402	2405	rBV4	2110	3487	0.15%	0.021%
41	17.145	2405	2407	2412	rVB	3318	3523	0.16%	0.021%
42	17.357	2437	2443	2454	rBV	1558221	2255425	100.00%	13.383%
43	17.457	2454	2460	2471	rBV	586767	849631	37.67%	5.041%
44	17.745	2505	2509	2510	rBV3	2265	2524	0.11%	0.015%
45	18.028	2553	2557	2561	rBV	16035	20598	0.91%	0.122%
46	18.251	2590	2595	2600	rBV3	16636	24030	1.07%	0.143%
47	18.328	2604	2608	2613	rBV	9067	12756	0.57%	0.076%
48	18.545	2642	2645	2648	rBV5	2691	4144	0.18%	0.025%
49	18.681	2664	2668	2672	rBV5	6594	8877	0.39%	0.053%
50	19.204	2753	2757	2762	rVB2	32876	37420	1.66%	0.222%
51	19.339	2774	2780	2785	rBV3	17472	27686	1.23%	0.164%
52	19.392	2787	2789	2793	rVB2	4735	5797	0.26%	0.034%
53	19.534	2809	2813	2818	rBV7	8818	14217	0.63%	0.084%
54	19.763	2846	2852	2864	rBV	638986	885197	39.25%	5.252%
55	20.498	2974	2977	2982	rBV	44464	57441	2.55%	0.341%
56	21.563	3152	3158	3164	rBV	1423633	1883299	83.50%	11.175%
57	23.851	3542	3547	3552	rBV2	259850	528134	23.42%	3.134%
58	24.016	3568	3575	3586	rVB2	759215	1513703	67.11%	8.982%




Sum of corrected areas: 16853465

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
Data File : BN022383.D
Acq On : 28 Oct 2022 14:04
Operator : CG/JU
Sample : N5216-18
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHA84

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

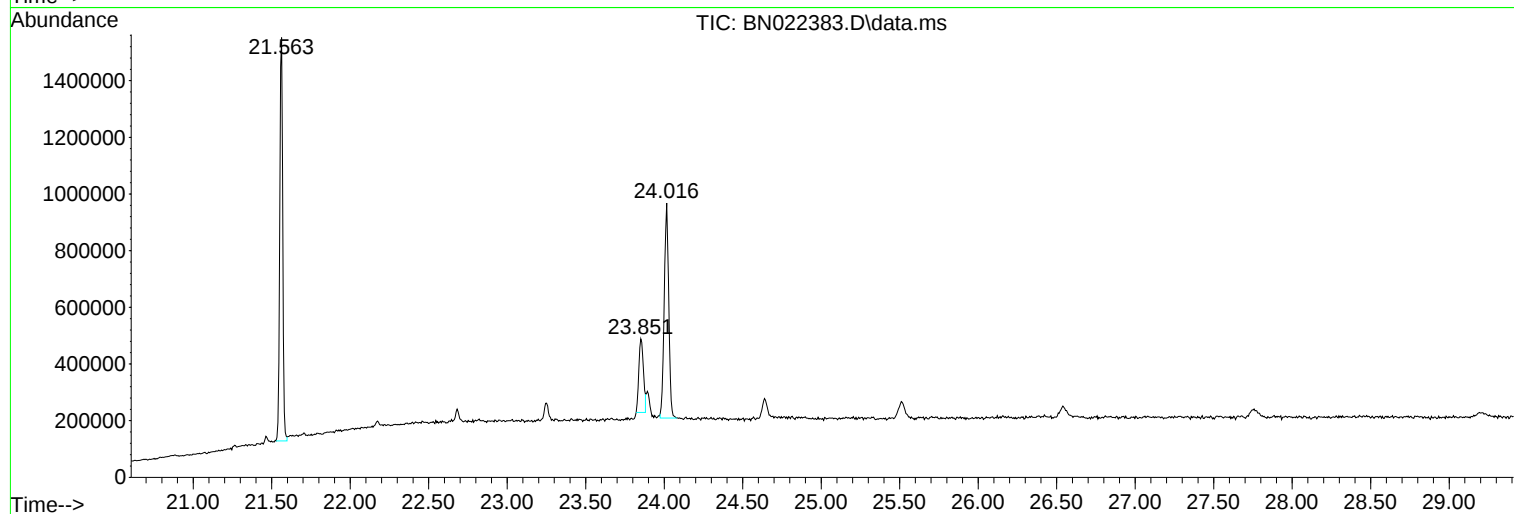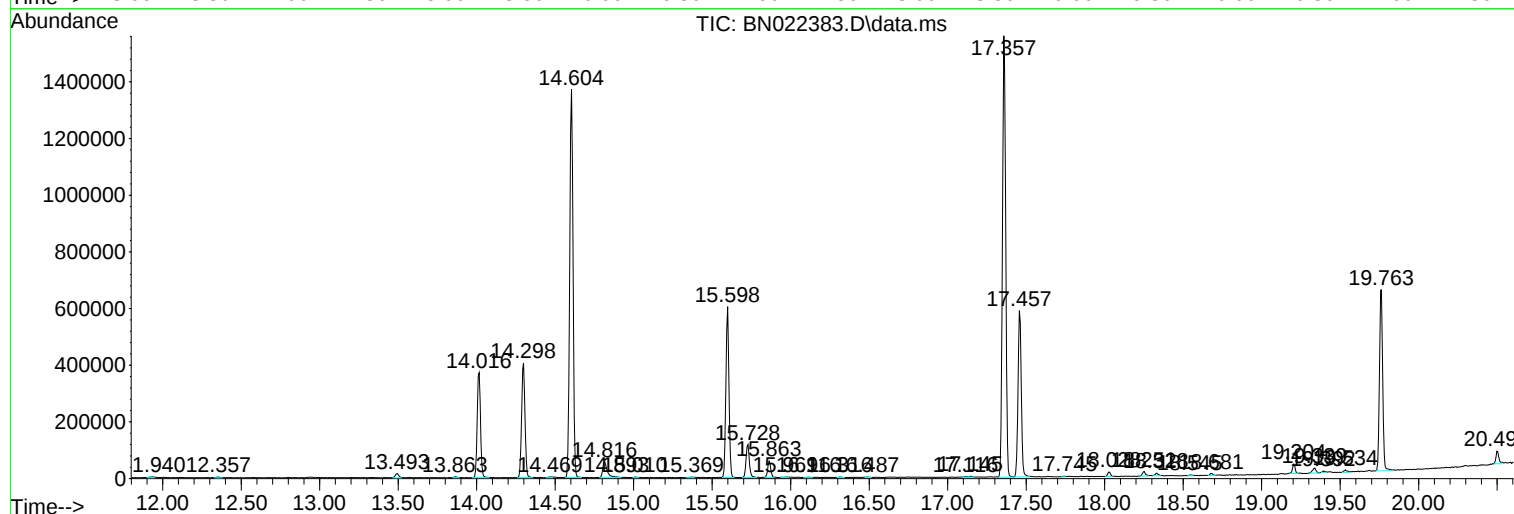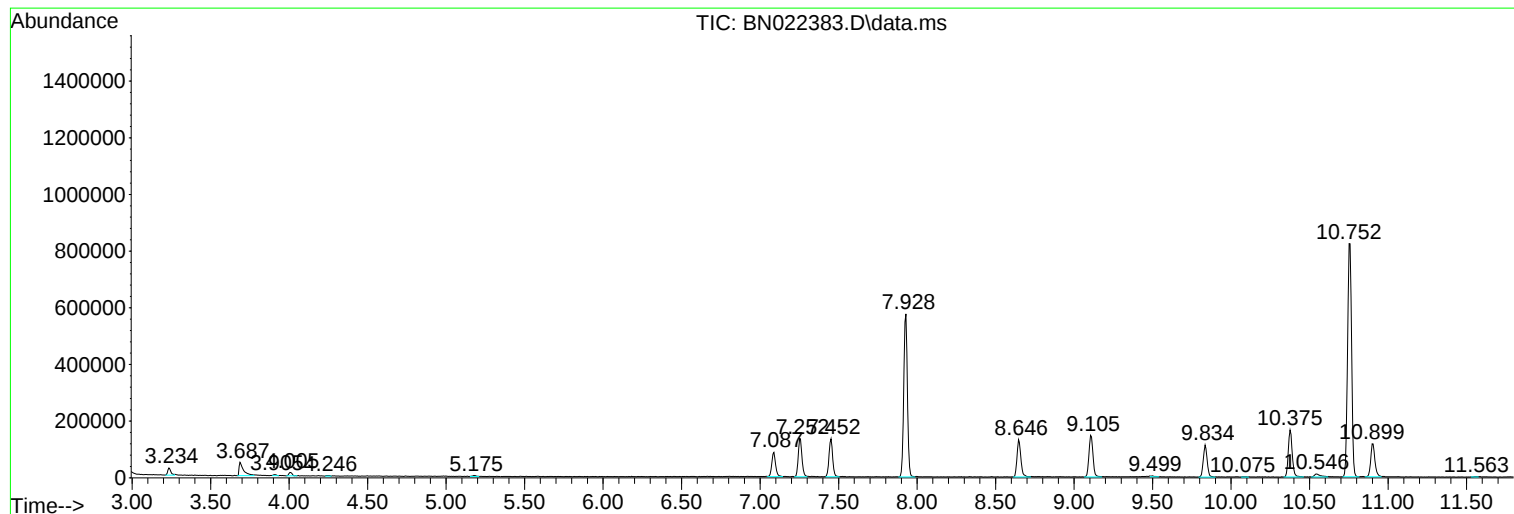

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
Data File : BN022383.D
Acq On : 28 Oct 2022 14:04
Operator : CG/JU
Sample : N5216-18
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHA84

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN102922\
Data File : BN022383.D
Acq On : 28 Oct 2022 14:04
Operator : CG/JU
Sample : N5216-18
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHA84

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN101222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc