
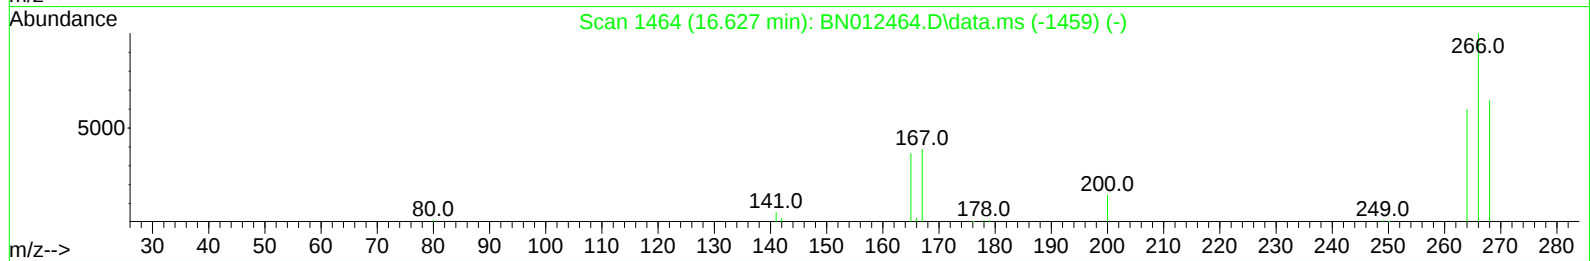
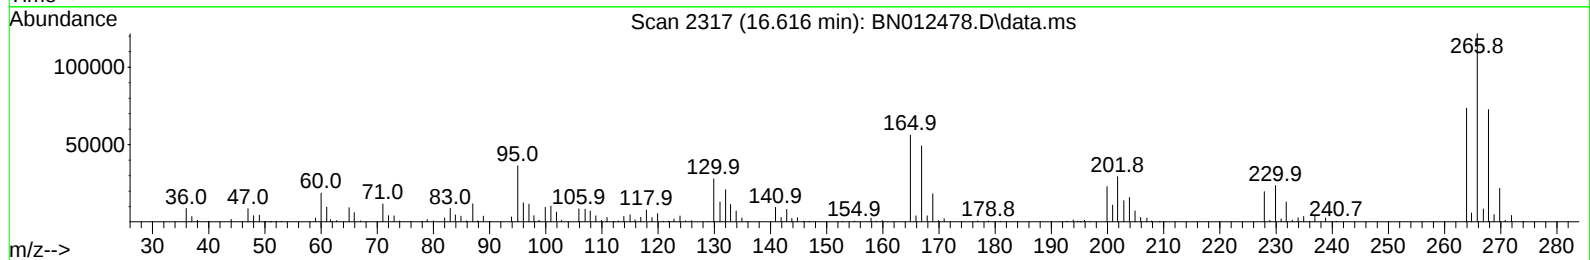


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103020\
Data File : BN012478.D
Acq On : 30 Oct 2020 20:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 02:01:41 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN103020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 30 14:49:10 2020
Response via : Initial Calibration

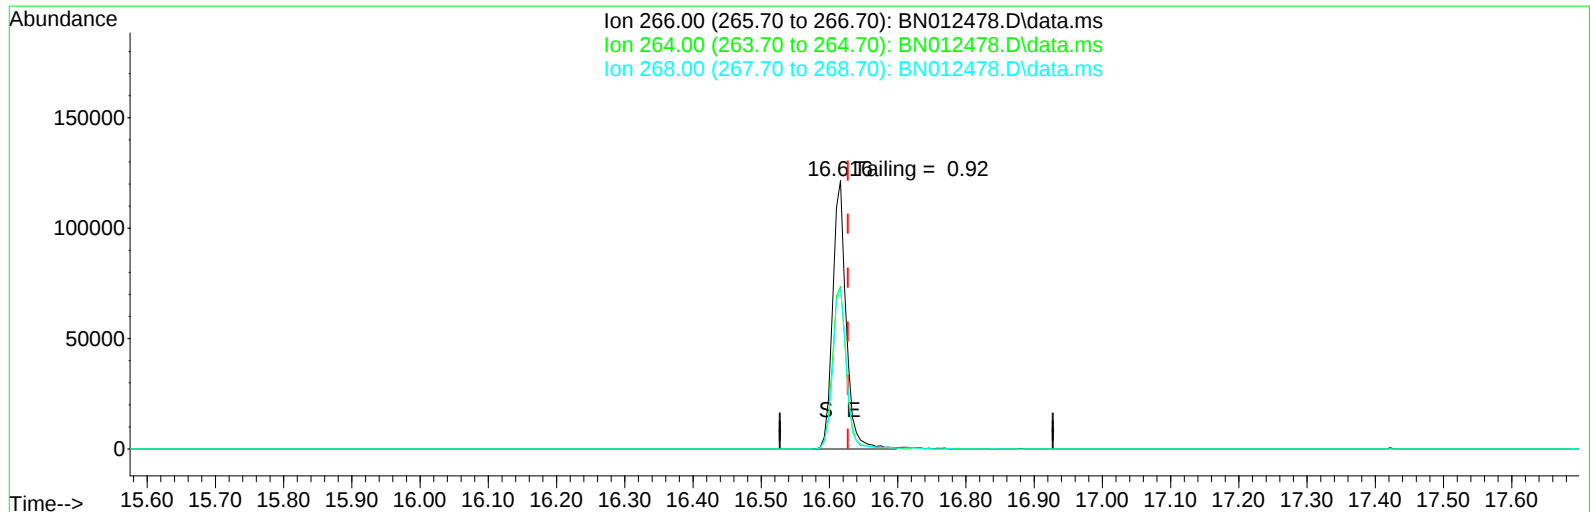

TIC: BN012478.D\data.ms

(24) Pentachlorophenol

16.616min (-0.011) 0.00 ng

response 167271

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	63.60	62.12
268.00	64.40	61.03
0.00	0.00	0.00