

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103020\
 Data File : BN012469.D
 Acq On : 30 Oct 2020 14:43
 Operator : CG/JU
 Sample : SSTDICV0.4
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 ICBVN103020

Quant Time: Oct 30 15:30:25 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN103020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 30 14:49:10 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.570	152	760	0.40	ng	# 0.00
7) Naphthalene-d8	10.339	136	3226	0.40	ng	0.00
13) Acenaphthene-d10	14.205	164	1745	0.40	ng	-0.01
19) Phenanthrene-d10	16.968	188	3543	0.40	ng	# 0.00
29) Chrysene-d12	21.174	240	3418	0.40	ng	# 0.00
36) Perylene-d12	23.344	264	3858	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.178	112	963	0.36	ng	0.00
5) Phenol-d6	6.749	99	1187	0.36	ng	0.00
8) Nitrobenzene-d5	8.717	82	1236	0.33	ng	-0.01
11) 2-Methylnaphthalene-d10	11.940	152	1906	0.36	ng	0.00
14) 2,4,6-Tribromophenol	15.715	330	417	0.35	ng	0.00
15) 2-Fluorobiphenyl	12.834	172	2364	0.36	ng	0.00
27) Fluoranthene-d10	19.003	212	3861	0.35	ng	0.00
31) Terphenyl-d14	19.618	244	2928	0.37	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.165	88	446	0.35	ng	# 77
3) n-Nitrosodimethylamine	3.479	42	1086	0.35	ng	# 72
6) bis(2-Chloroethyl)ether	7.006	93	741	0.35	ng	88
9) Naphthalene	10.390	128	3257	0.36	ng	98
10) Hexachlorobutadiene	10.668	225	668	0.35	ng	# 100
12) 2-Methylnaphthalene	12.016	142	2108	0.36	ng	# 90
16) Acenaphthylene	13.926	152	3126	0.36	ng	99
17) Acenaphthene	14.268	154	1991	0.36	ng	90
18) Fluorene	15.270	166	2493	0.36	ng	98
20) 4,6-Dinitro-2-methylph...	15.385	198	243	0.35	ng	# 8
21) 4-Bromophenyl-phenylether	16.165	248	767	0.36	ng	96
22) Hexachlorobenzene	16.275	284	954	0.35	ng	# 82
23) Atrazine	16.445	200	708	0.34	ng	93
24) Pentachlorophenol	16.628	266	414	0.34	ng	94
25) Phenanthrene	17.005	178	3731	0.35	ng	97
26) Anthracene	17.102	178	3297	0.34	ng	100
28) Fluoranthene	19.038	202	4248	0.34	ng	99
30) Pyrene	19.400	202	4378	0.37	ng	100
32) Benzo(a)anthracene	21.153	228	3745	0.35	ng	96
33) Chrysene	21.206	228	4287	0.37	ng	96
34) Bis(2-ethylhexyl)phtha...	21.099	149	2516	0.36	ng	93
35) Indeno(1,2,3-cd)pyrene	25.500	276	5950	0.35	ng	96
37) Benzo(b)fluoranthene	22.697	252	4441	0.36	ng	# 88
38) Benzo(k)fluoranthene	22.741	252	4820	0.37	ng	# 88
39) Benzo(a)pyrene	23.248	252	4292	0.36	ng	# 80
40) Dibenzo(a,h)anthracene	25.517	278	4860	0.36	ng	# 91
41) Benzo(g,h,i)perylene	26.157	276	5040	0.36	ng	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103020\
Data File : BN012469.D
Acq On : 30 Oct 2020 14:43
Operator : CG/JU
Sample : SSTDICV0.4
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
ICVBN103020

Quant Time: Oct 30 15:30:25 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN103020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 30 14:49:10 2020
Response via : Initial Calibration




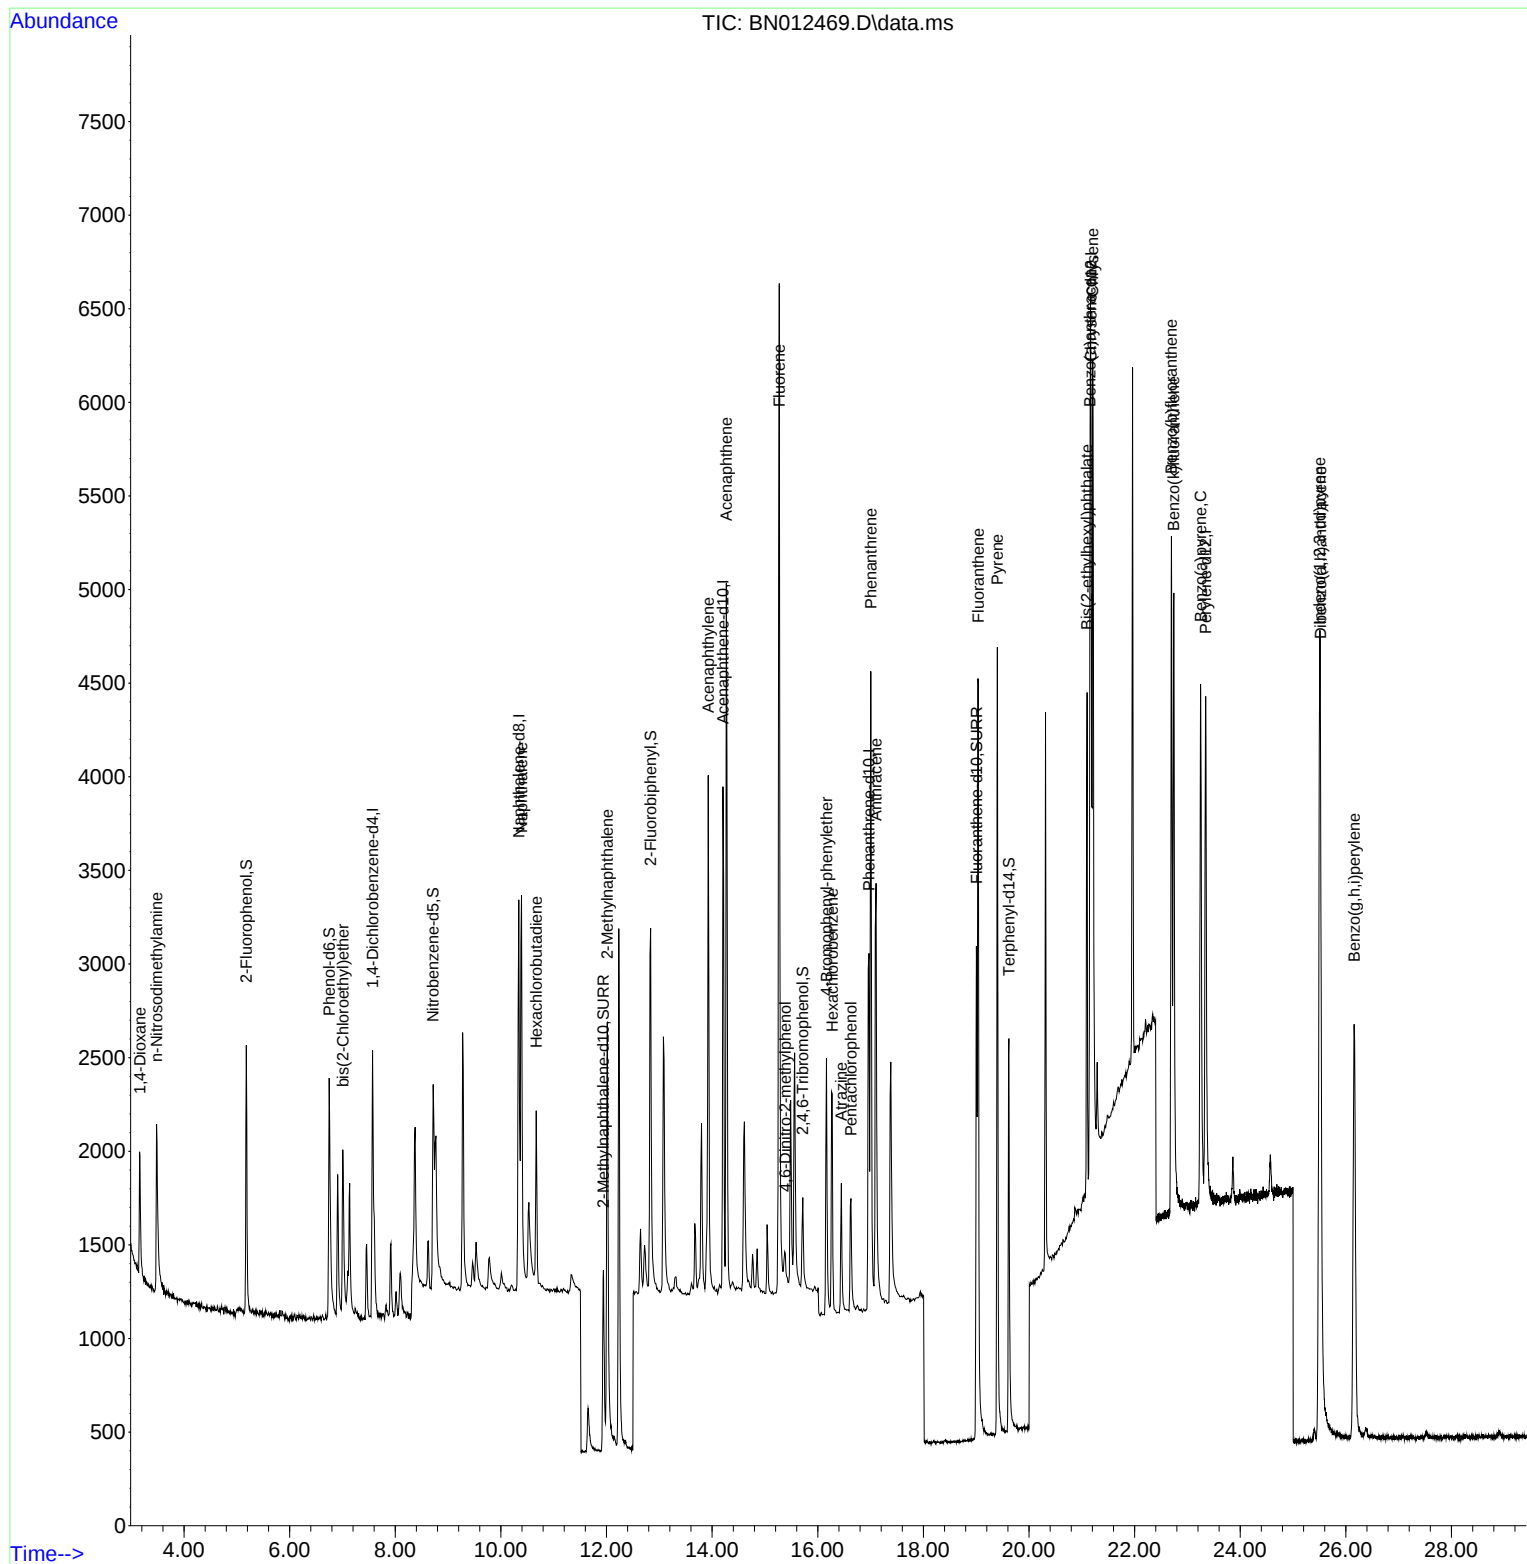




#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.570 min Scan# 570
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43




Instrument :
BNA_N
ClientSampleId :
ICVBN103020


Tgt Ion:152 Resp: 760
Ion Ratio Lower Upper
152 100
150 156.7 116.6 174.8
115 81.3 52.9 79.3#

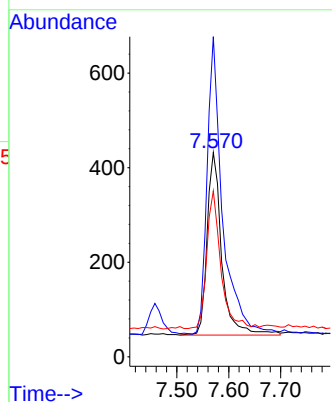

#2
1,4-Dioxane
Concen: 0.35 ng
RT: 3.165 min Scan# 23
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43

Tgt Ion: 88 Resp: 446
Ion Ratio Lower Upper
88 100
58 80.7 59.4 89.2
43 72.4 32.3 48.5#


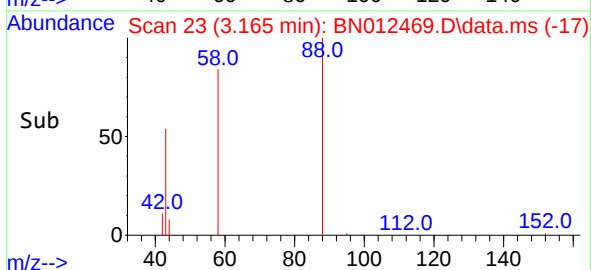






#3
n-Nitrosodimethylamine
Concen: 0.35 ng
RT: 3.479 min Scan# 62
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43




Instrument :
BNA_N
ClientSampleId :
ICVBN103020


Tgt Ion: 42 Resp: 1086
Ion Ratio Lower Upper
42 100
74 55.5 64.4 96.6#
44 8.3 2.8 4.2#

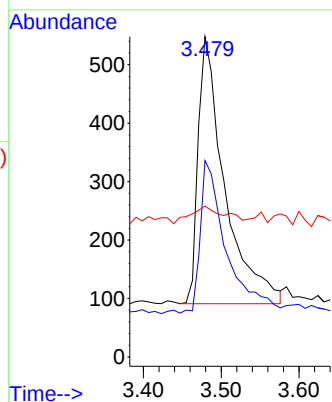

#4
2-Fluorophenol
Concen: 0.36 ng
RT: 5.178 min Scan# 273
Delta R.T. -0.008 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43

Tgt Ion: 112 Resp: 963
Ion Ratio Lower Upper
112 100
64 71.2 49.5 74.3
63 52.4 32.0 48.0#


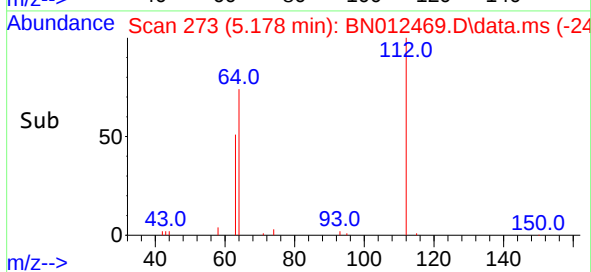






#5
Phenol-d6
Concen: 0.36 ng
RT: 6.749 min Scan# 468
Delta R.T. -0.008 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43




Instrument :
BNA_N
ClientSampleId :
ICVBN103020


Tgt Ion: 99 Resp: 1187
Ion Ratio Lower Upper
99 100
42 43.1 22.4 33.6#
71 59.8 37.8 56.6#

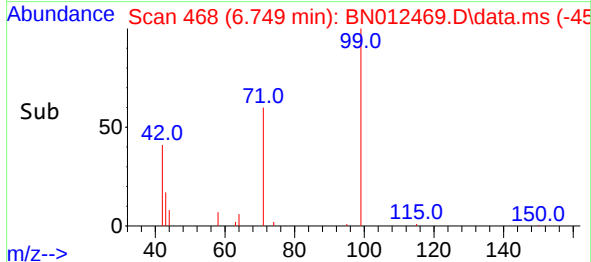

#6
bis(2-Chloroethyl)ether
Concen: 0.35 ng
RT: 7.006 min Scan# 500
Delta R.T. -0.008 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43

Tgt Ion: 93 Resp: 741
Ion Ratio Lower Upper
93 100
63 92.2 63.1 94.7
95 34.8 26.1 39.1









#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.339 min Scan# 822
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43




Instrument :
BNA_N
ClientSampleId :
ICVBN103020


Tgt Ion:	136	Resp:	3226
Ion	Ratio	Lower	Upper
136	100		
137	13.5	10.6	15.8
54	10.9	8.6	12.8
68	5.9	5.7	8.5

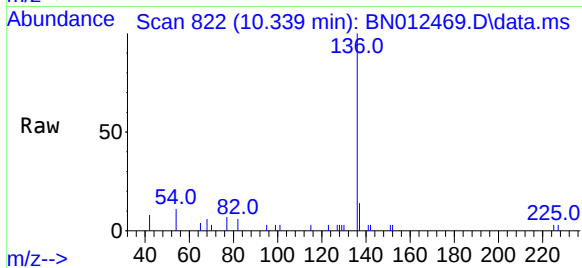

#8
Nitrobenzene-d5
Concen: 0.33 ng
RT: 8.717 min Scan# 694
Delta R.T. -0.012 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43

Tgt Ion:	82	Resp:	1236
Ion	Ratio	Lower	Upper
82	100		
128	37.5	30.6	46.0
54	76.1	48.3	72.5




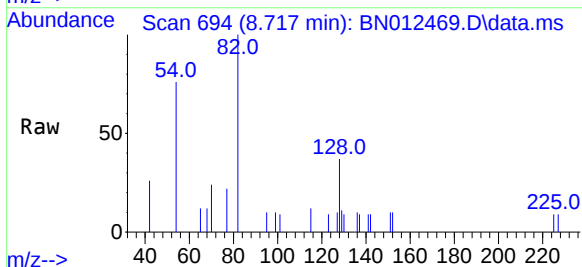




#9
Naphthalene
Concen: 0.36 ng
RT: 10.390 min Scan# 826
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43




Instrument :
BNA_N
ClientSampleId :
ICVBN103020


Tgt Ion:128 Resp: 3257
Ion Ratio Lower Upper
128 100
129 13.5 9.8 14.8
127 15.6 12.2 18.4



#10
Hexachlorobutadiene
Concen: 0.35 ng
RT: 10.668 min Scan# 848
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43

Tgt Ion:225 Resp: 668
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.9 51.0 76.6


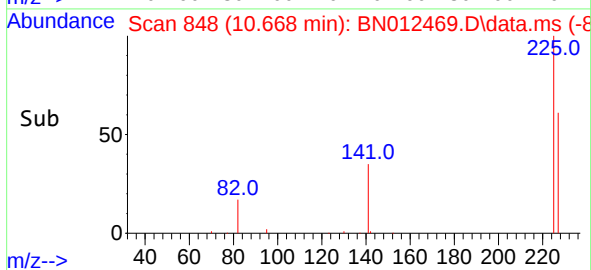






#11
2-Methylnaphthalene-d10
Concen: 0.36 ng
RT: 11.940 min Scan# 1010
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43




Instrument :
BNA_N
ClientSampleId :
ICVBN103020


Tgt Ion:152 Resp: 1906
Ion Ratio Lower Upper
152 100
151 19.7 16.7 25.1

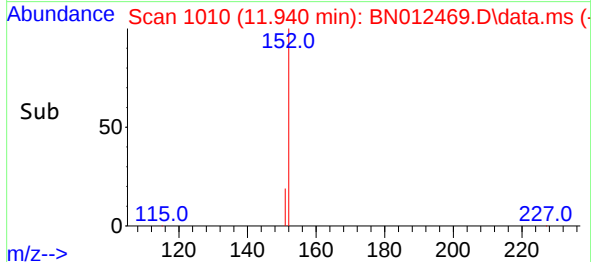

#12
2-Methylnaphthalene
Concen: 0.36 ng
RT: 12.016 min Scan# 1027
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43

Tgt Ion:142 Resp: 2108
Ion Ratio Lower Upper
142 100
141 90.2 69.4 104.2
115 58.3 35.7 53.5#

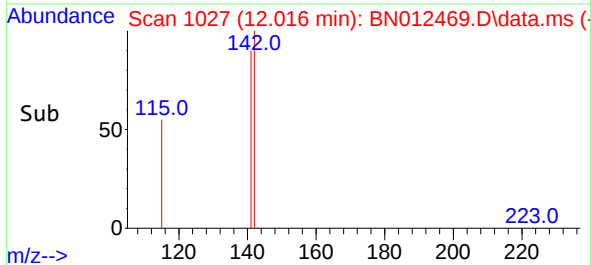







#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.205 min Scan# 1271
Delta R.T. -0.012 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43

Instrument :
BNA_N
ClientSampleId :
ICVBN103020

Tgt Ion:164 Resp: 1745




Ion	Ratio	Lower	Upper
164	100		
162	106.2	80.6	120.8
160	52.6	39.5	59.3




#14
2,4,6-Tribromophenol
Concen: 0.35 ng
RT: 15.715 min Scan# 1390
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43

Tgt Ion:330 Resp: 417

Ion	Ratio	Lower	Upper
330	100		
332	0.0	0.0	0.0
141	48.7	34.4	51.6









#15
2-Fluorobiphenyl
Concen: 0.36 ng
RT: 12.834 min Scan# 1163
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43




Instrument :
BNA_N
ClientSampleId :
ICVBN103020


Tgt Ion:	172	Resp:	2364
Ion	Ratio	Lower	Upper
172	100		
171	37.3	28.2	42.4
170	26.2	20.0	30.0

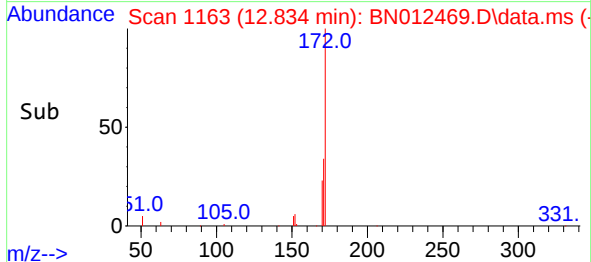

#16
Acenaphthylene
Concen: 0.36 ng
RT: 13.926 min Scan# 1249
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43

Tgt Ion:	152	Resp:	3126
Ion	Ratio	Lower	Upper
152	100		
151	19.6	15.8	23.8
153	12.7	10.6	16.0




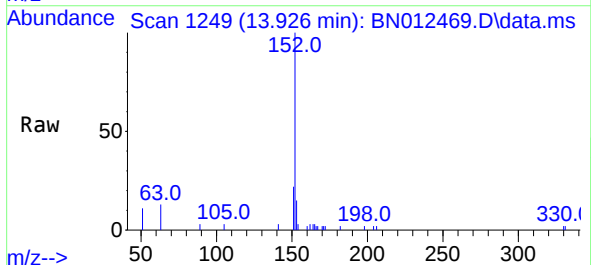




#17
Acenaphthene
Concen: 0.36 ng
RT: 14.268 min Scan# 1276
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43




Instrument :
BNA_N
ClientSampleId :
ICVBN103020


Tgt Ion:154 Resp: 1991
Ion Ratio Lower Upper
154 100
153 118.6 83.6 125.4
152 57.4 43.9 65.9

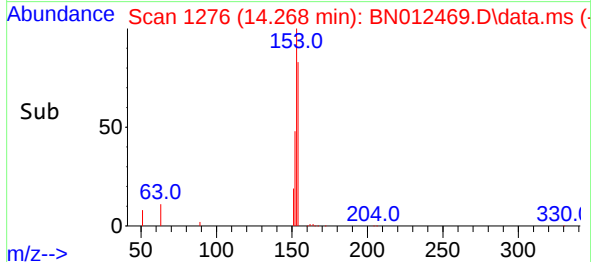

#18
Fluorene
Concen: 0.36 ng
RT: 15.270 min Scan# 1355
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43

Tgt Ion:166 Resp: 2493
Ion Ratio Lower Upper
166 100
165 100.0 78.6 118.0
167 13.8 10.7 16.1




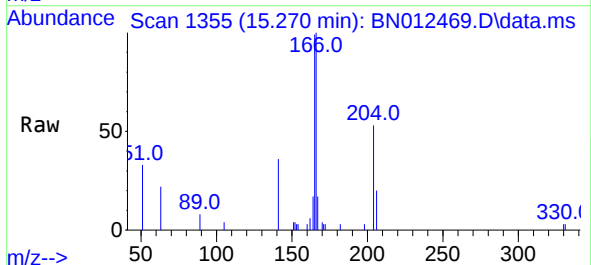




#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 16.968 min Scan# 1492
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43




Instrument :
BNA_N
ClientSampleId :
ICVBN103020


Tgt Ion:188	Resp:	3543
Ion Ratio	Lower	Upper
188	100	
94	0.0	0.0
80	8.0	5.0



#20
4,6-Dinitro-2-methylphenol
Concen: 0.35 ng
RT: 15.385 min Scan# 1364
Delta R.T. 0.013 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43

Tgt Ion:198	Resp:	243
Ion Ratio	Lower	Upper
198	100	
51	136.9	43.5
105	65.6	27.2


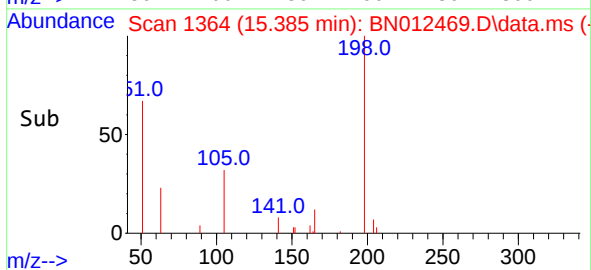




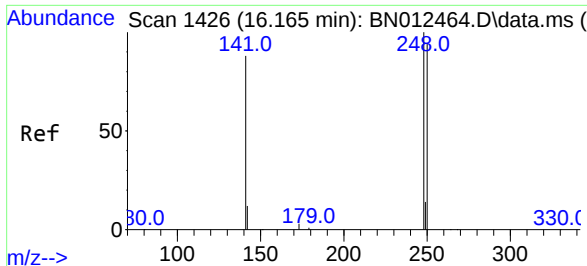

#21
4-Bromophenyl-phenylether
Concen: 0.36 ng
RT: 16.165 min Scan# 1426
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43




Instrument :
BNA_N
ClientSampleId :
ICVBN103020


Tgt Ion:	248	Resp:	767
Ion	Ratio	Lower	Upper
248	100		
250	96.6	77.3	115.9
141	80.8	57.8	86.8

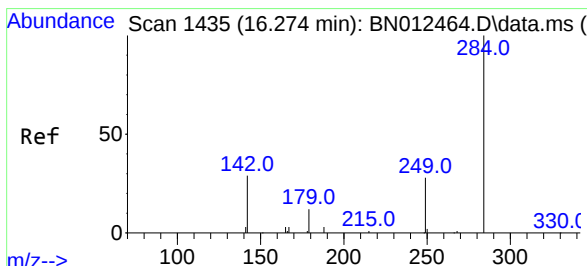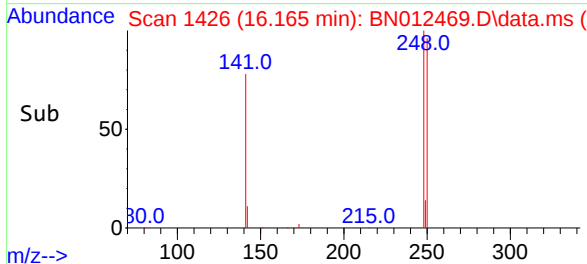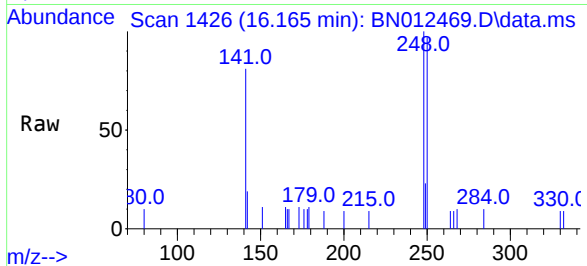

#22
Hexachlorobenzene
Concen: 0.35 ng
RT: 16.275 min Scan# 1435
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43

Tgt Ion:	284	Resp:	954
Ion	Ratio	Lower	Upper
284	100		
142	57.4	32.0	48.0#
249	31.0	27.0	40.6


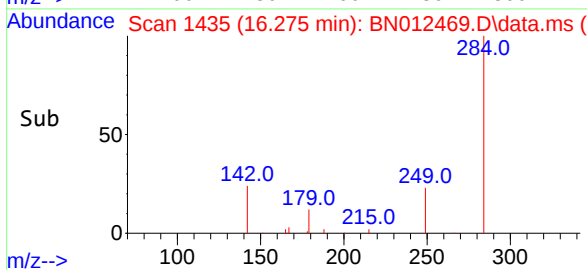

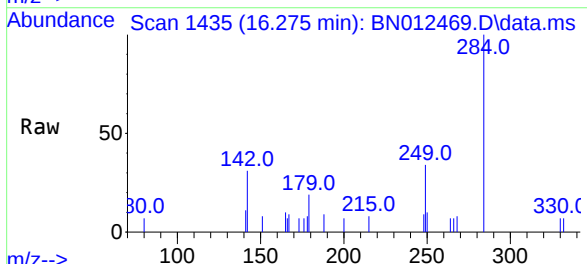




#23
Atrazine
Concen: 0.34 ng
RT: 16.445 min Scan# 1449
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43




Instrument :
BNA_N
ClientSampleId :
ICVBN103020


Tgt Ion:200 Resp: 708
Ion Ratio Lower Upper
200 100
173 30.0 22.8 34.2
215 53.7 38.1 57.1

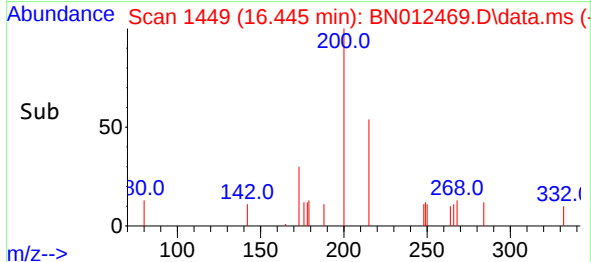

#24
Pentachlorophenol
Concen: 0.34 ng
RT: 16.628 min Scan# 1464
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43

Tgt Ion:266 Resp: 414
Ion Ratio Lower Upper
266 100
264 64.5 50.9 76.3
268 56.5 51.5 77.3


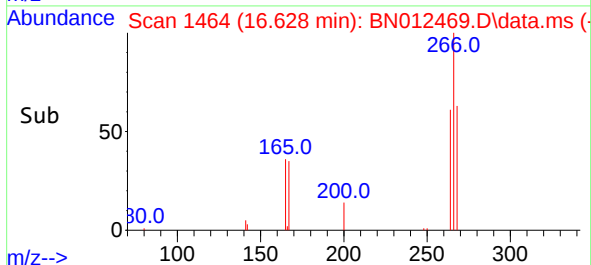
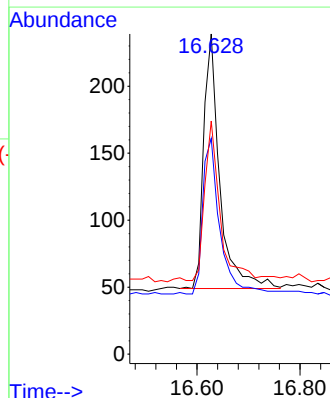
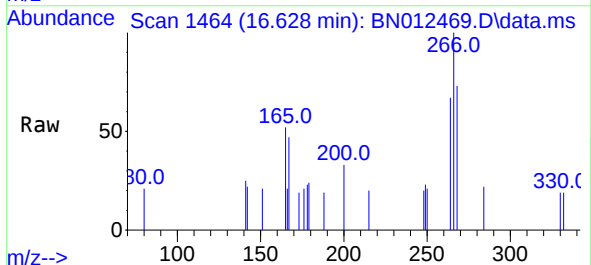




#25
Phenanthrene
Concen: 0.35 ng
RT: 17.005 min Scan# 1495
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43




Instrument :
BNA_N
ClientSampleId :
ICVBN103020


Tgt Ion:	178	Resp:	3731
Ion	Ratio	Lower	Upper
178	100		
176	20.2	14.8	22.2
179	16.0	12.4	18.6



#26
Anthracene
Concen: 0.34 ng
RT: 17.102 min Scan# 1503
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43

Tgt Ion:	178	Resp:	3297
Ion	Ratio	Lower	Upper
178	100		
176	18.3	14.8	22.2
179	15.5	12.5	18.7


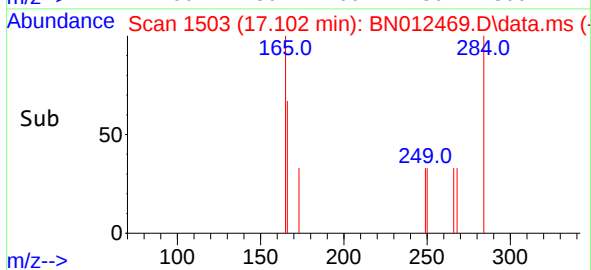






#27
Fluoranthene-d10
Concen: 0.35 ng
RT: 19.003 min Scan# 1777
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43




Instrument :
BNA_N
ClientSampleId :
ICVBN103020


Tgt Ion:212 Resp: 3861
Ion Ratio Lower Upper
212 100
106 7.4 6.8 10.2
104 4.9 4.1 6.1



#28
Fluoranthene
Concen: 0.34 ng
RT: 19.038 min Scan# 1784
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43

Tgt Ion:202 Resp: 4248
Ion Ratio Lower Upper
202 100
101 6.9 5.8 8.6
203 16.6 13.7 20.5


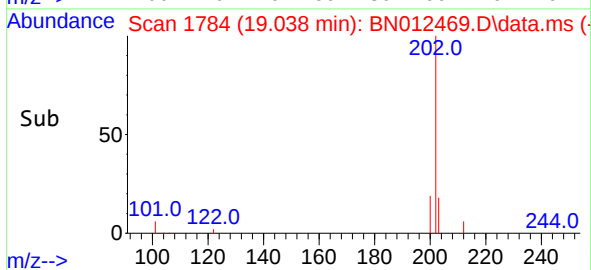






#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.174 min Scan# 2089
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43




Instrument :
BNA_N
ClientSampleId :
ICVBN103020


Tgt Ion:240 Resp: 3418
Ion Ratio Lower Upper
240 100
120 9.7 5.3 7.9#
236 26.6 21.8 32.8



#30
Pyrene
Concen: 0.37 ng
RT: 19.400 min Scan# 1857
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43

Tgt Ion:202 Resp: 4378
Ion Ratio Lower Upper
202 100
200 20.7 16.6 24.8
203 17.6 13.8 20.8


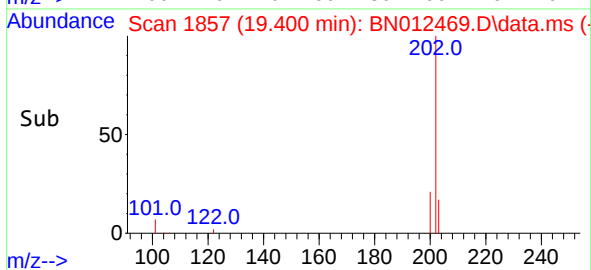






#31
Terphenyl-d14
Concen: 0.37 ng
RT: 19.618 min Scan# 1901
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43




Instrument :
BNA_N
ClientSampleId :
ICVBN103020


Tgt Ion:244 Resp: 2928
Ion Ratio Lower Upper
244 100
212 11.8 7.3 10.9#
122 11.7 7.3 10.9#



#32
Benzo(a)anthracene
Concen: 0.35 ng
RT: 21.153 min Scan# 2087
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43

Tgt Ion:228 Resp: 3745
Ion Ratio Lower Upper
228 100
226 29.8 22.3 33.5
229 21.3 15.7 23.5


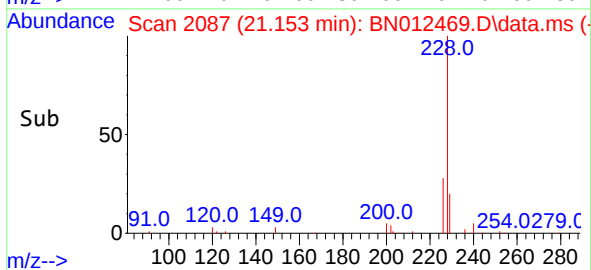




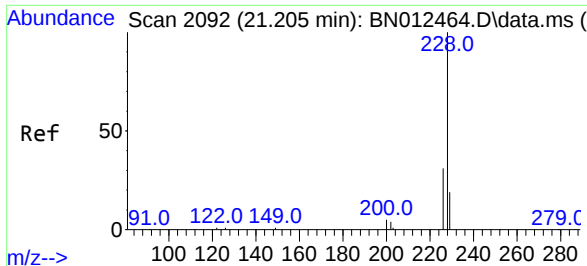

#33
Chrysene
Concen: 0.37 ng
RT: 21.206 min Scan# 2092
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43




Instrument :
BNA_N
ClientSampleId :
ICVBN103020


Tgt Ion:	228	Resp:	4287
Ion	Ratio	Lower	Upper
228	100		
226	32.2	24.2	36.2
229	21.6	15.7	23.5

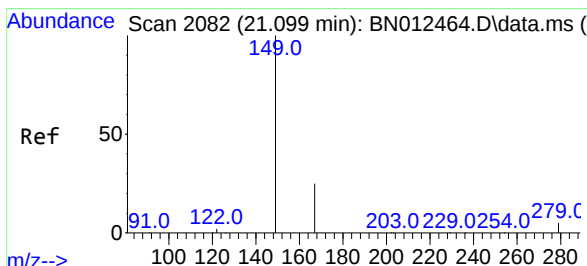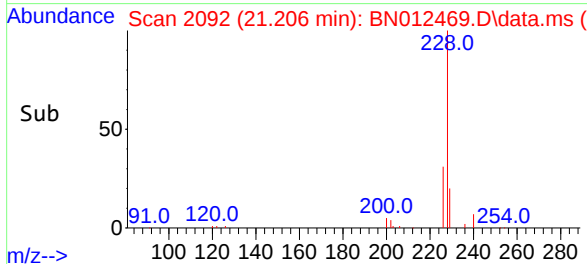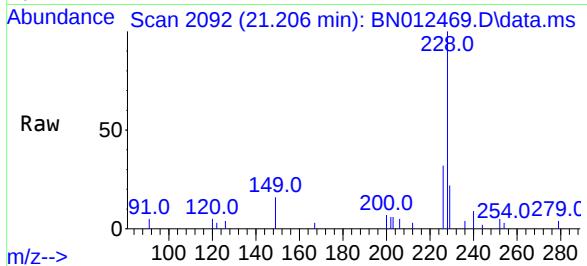

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.36 ng
RT: 21.099 min Scan# 2082
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43

Tgt Ion:	149	Resp:	2516
Ion	Ratio	Lower	Upper
149	100		
167	24.8	23.2	34.8
279	4.7	3.9	5.9


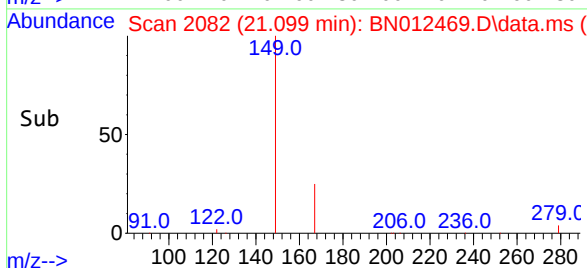
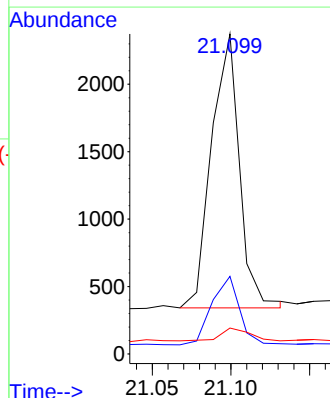
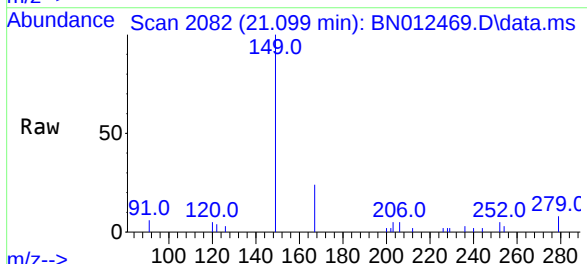




#35
Indeno(1,2,3-cd)pyrene
Concen: 0.35 ng
RT: 25.500 min Scan# 3109
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43




Instrument :
BNA_N
ClientSampleId :
ICVBN103020


Tgt Ion:276 Resp: 5950
Ion Ratio Lower Upper
276 100
138 14.3 13.3 19.9
277 23.6 20.2 30.4



#36
Perylene-d12
Concen: 0.40 ng
RT: 23.344 min Scan# 2479
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43

Tgt Ion:264 Resp: 3858
Ion Ratio Lower Upper
264 100
260 26.4 19.8 29.6
265 68.8 51.4 77.0



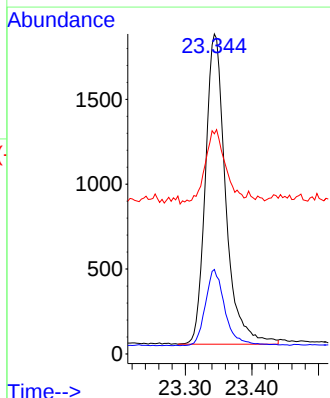





#37
Benzo(b)fluoranthene
Concen: 0.36 ng
RT: 22.697 min Scan# 2290
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43




Instrument :
BNA_N
ClientSampleId :
ICVBN103020


Tgt Ion:252 Resp: 4441
Ion Ratio Lower Upper
252 100
253 30.8 20.1 30.1#
125 13.7 7.2 10.8#

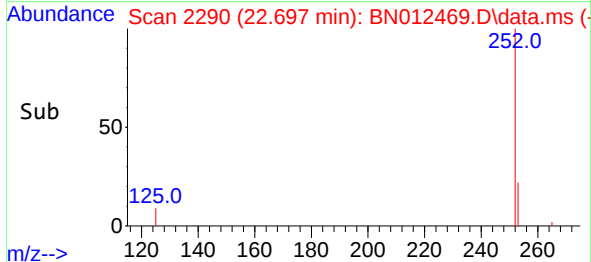

#38
Benzo(k)fluoranthene
Concen: 0.37 ng
RT: 22.741 min Scan# 2303
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43

Tgt Ion:252 Resp: 4820
Ion Ratio Lower Upper
252 100
253 31.5 19.8 29.8#
125 11.2 7.1 10.7#

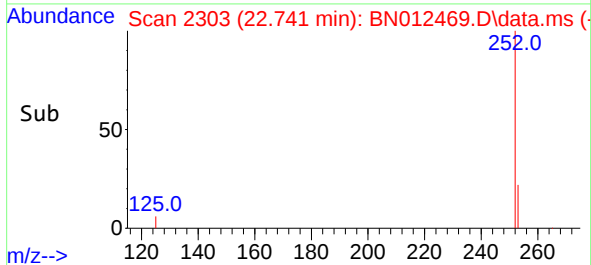



#39

Benzo(a)pyrene

Concen: 0.36 ng

RT: 23.248 min Scan# 2451

Delta R.T. 0.000 min

Lab File: BN012469.D

Acq: 30 Oct 2020 14:43





Tgt Ion:	252	Resp:	4292
Ion	Ratio	Lower	Upper
252	100		
253	36.0	21.3	31.9#
125	19.1	8.3	12.5#

Instrument :

BNA_N

ClientSampleId :

ICVBN103020



#40

Dibenzo(a,h)anthracene

Concen: 0.36 ng




RT: 25.517 min Scan# 3114


Delta R.T. 0.004 min

Lab File: BN012469.D

Acq: 30 Oct 2020 14:43

Tgt Ion:	278	Resp:	4860
Ion	Ratio	Lower	Upper
278	100		
139	13.1	9.3	13.9
279	32.9	21.6	32.4#

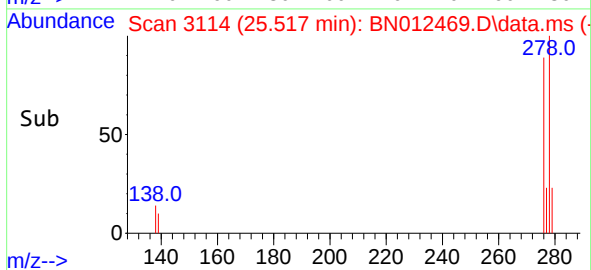

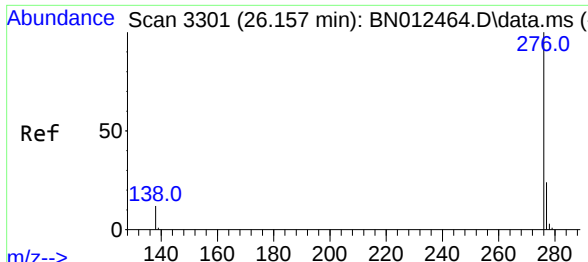

#41
Benzo(g,h,i)perylene
Concen: 0.36 ng
RT: 26.157 min Scan# 3301
Delta R.T. 0.000 min
Lab File: BN012469.D
Acq: 30 Oct 2020 14:43

Instrument :
BNA_N
ClientSampleId :
ICVBN103020

Tgt Ion:276 Resp: 5040
Ion Ratio Lower Upper
276 100
277 27.5 19.8 29.8
138 15.7 11.7 17.5

