


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103020\
 Data File : BN012460.D
 Acq On : 30 Oct 2020 09:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN103020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 30 14:49:10 2020

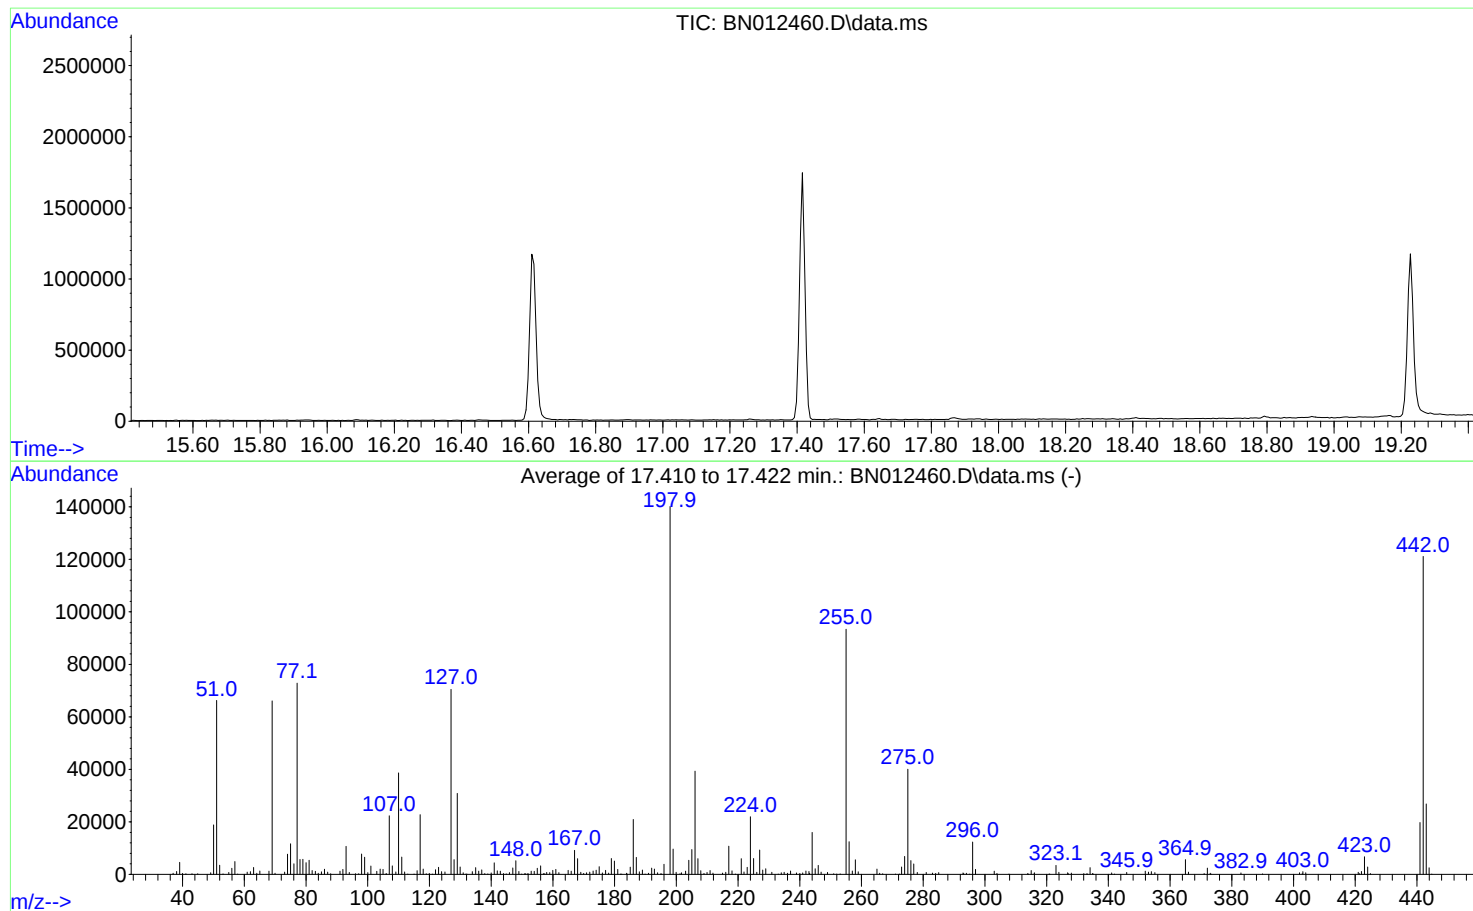

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.3	66253	PASS
68	69	0.00	2	1.9	1248	PASS
69	198	0.00	100	47.2	66101	PASS
70	69	0.00	2	0.7	450	PASS
127	198	10	80	50.3	70477	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	140131	PASS
199	198	5	9	6.9	9640	PASS
275	198	10	60	28.6	40051	PASS
365	198	1	100	4.0	5632	PASS
441	198	0.01	100	14.1	19738	PASS
442	198	50	100	86.4	121096	PASS
443	442	15	24	22.2	26853	PASS