
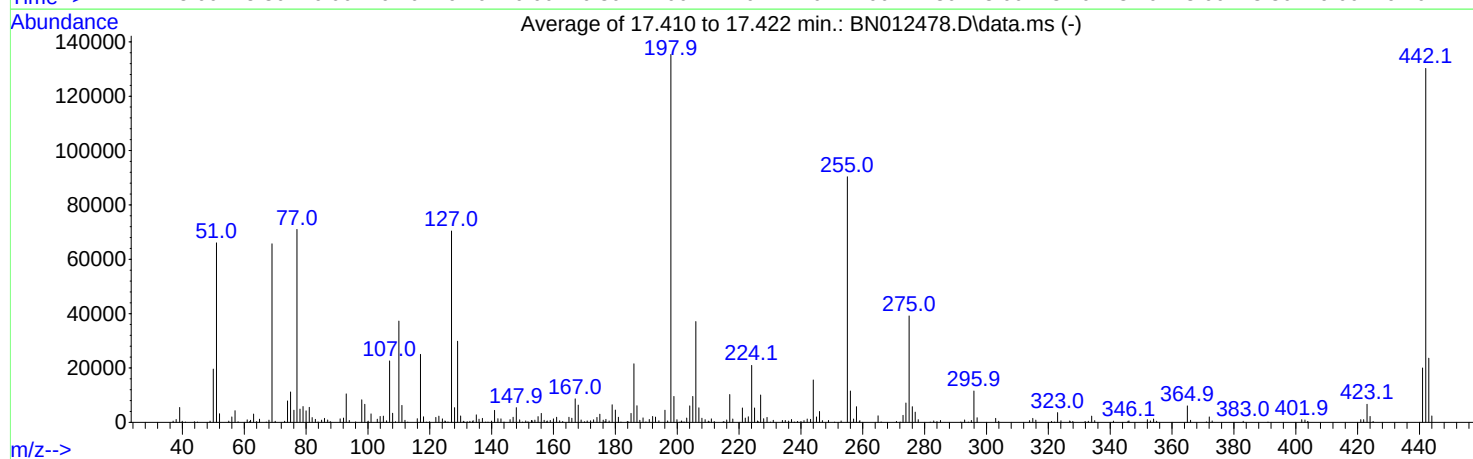


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103020\
 Data File : BN012478.D
 Acq On : 30 Oct 2020 20:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN103020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 30 14:49:10 2020

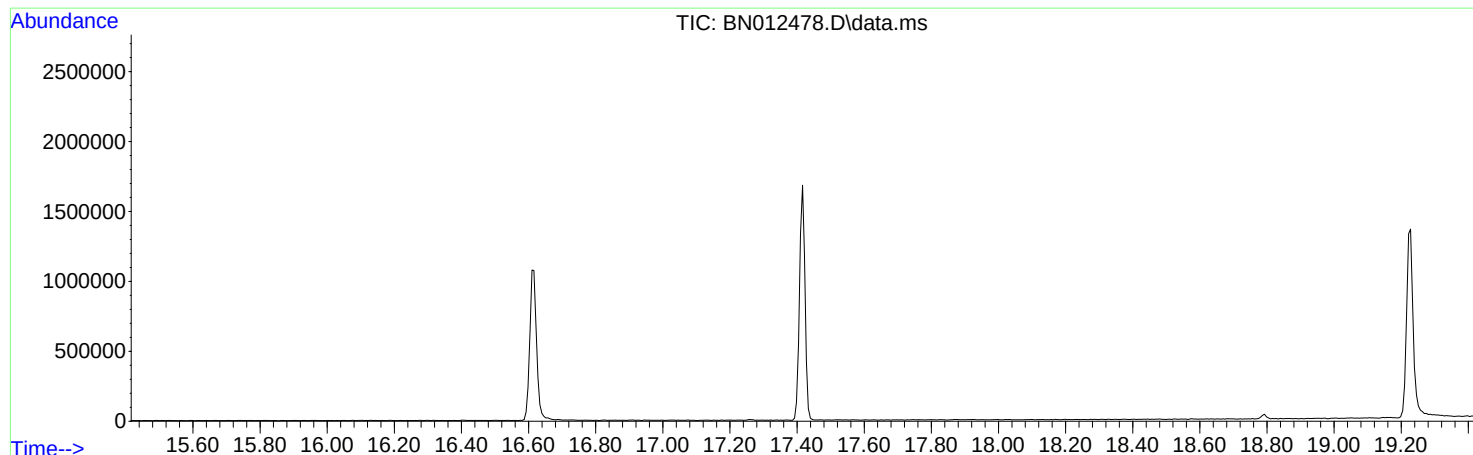

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.8	66072	PASS
68	69	0.00	2	1.3	837	PASS
69	198	0.00	100	48.5	65683	PASS
70	69	0.00	2	0.6	416	PASS
127	198	10	80	52.0	70432	PASS
197	198	0.00	2	0.4	518	PASS
198	198	100	100	100.0	135339	PASS
199	198	5	9	7.1	9566	PASS
275	198	10	60	28.9	39165	PASS
365	198	1	100	4.5	6083	PASS
441	198	0.01	100	14.8	19992	PASS
442	198	50	100	96.2	130221	PASS
443	442	15	24	18.1	23632	PASS