
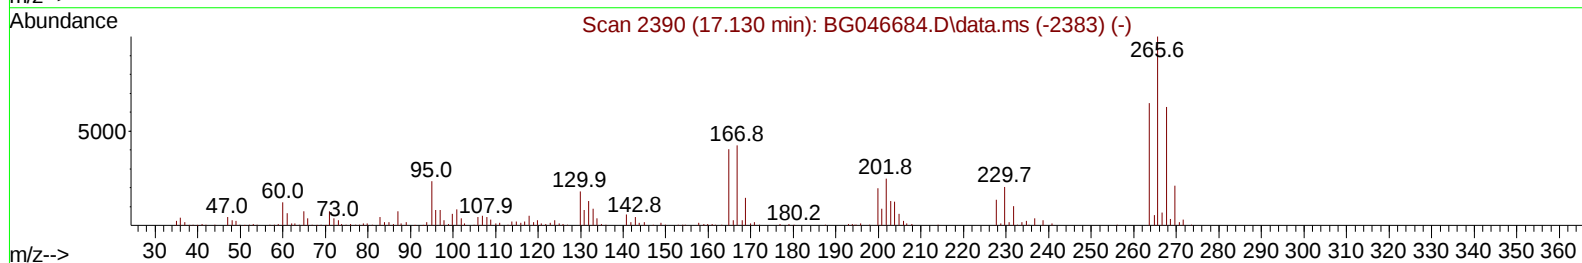
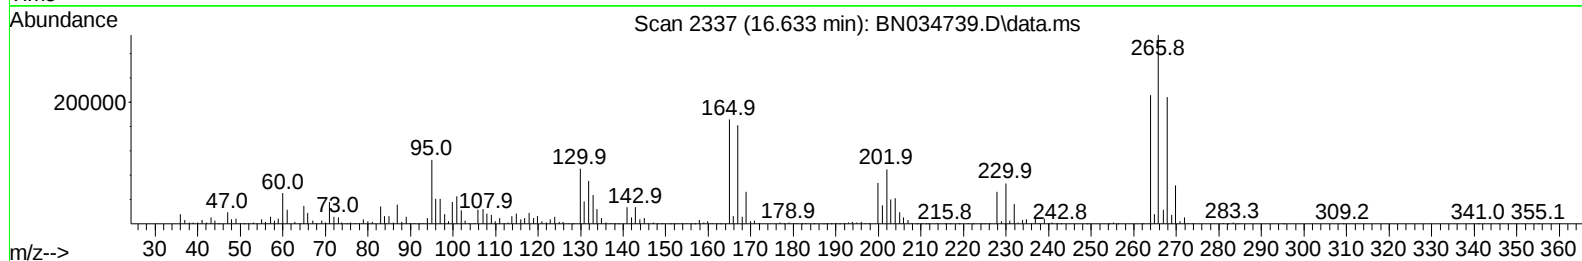


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103024\
Data File : BN034739.D
Acq On : 30 Oct 2024 08:41
Operator : RC/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 06:42:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 06:42:45 2024
Response via : Initial Calibration

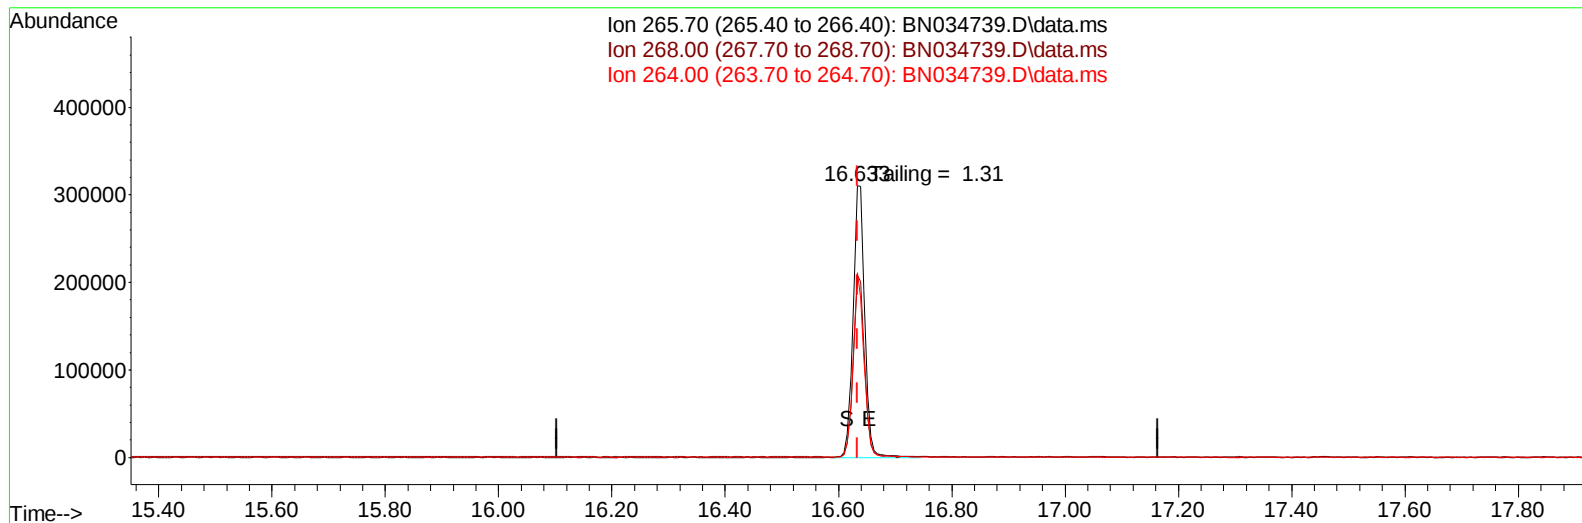

TIC: BN034739.D\data.ms

(70) Pentachlorophenol (C)




16.633min (0.000) 23615.75 ng

response 445905

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.99
264.00	61.60	68.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103024\
Data File : BN034739.D
Acq On : 30 Oct 2024 08:41
Operator : RC/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 06:42:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 04 06:42:45 2024
Response via : Initial Calibration

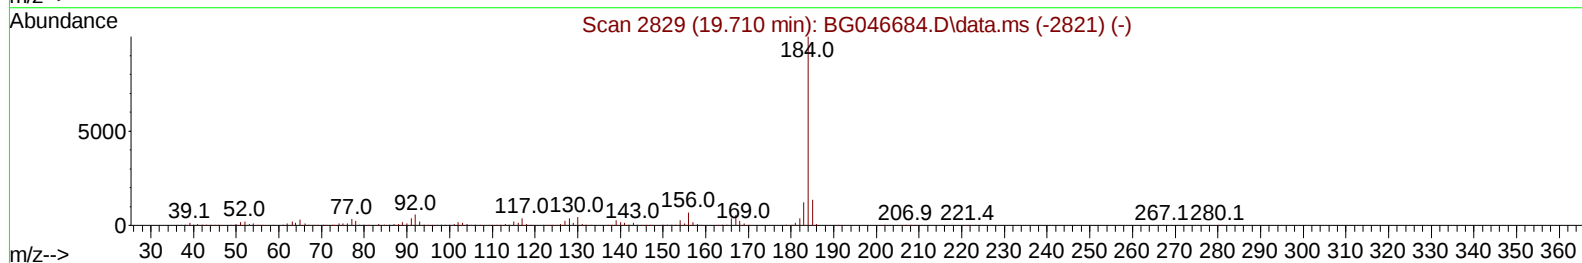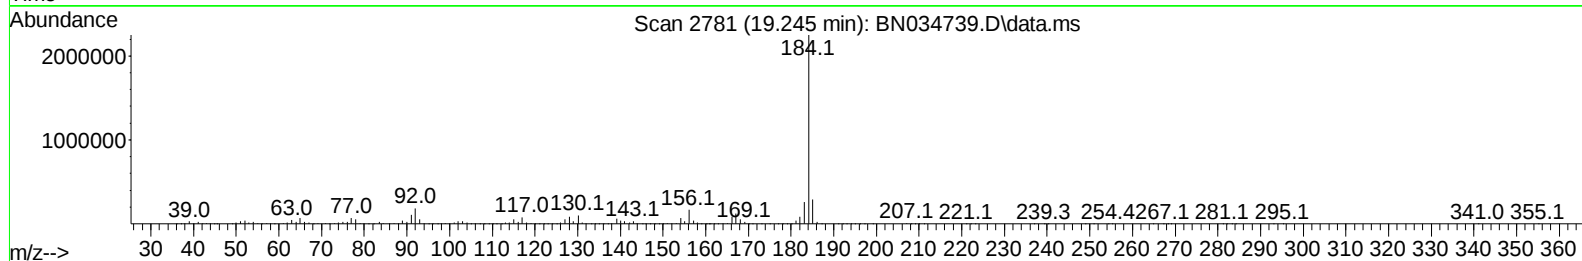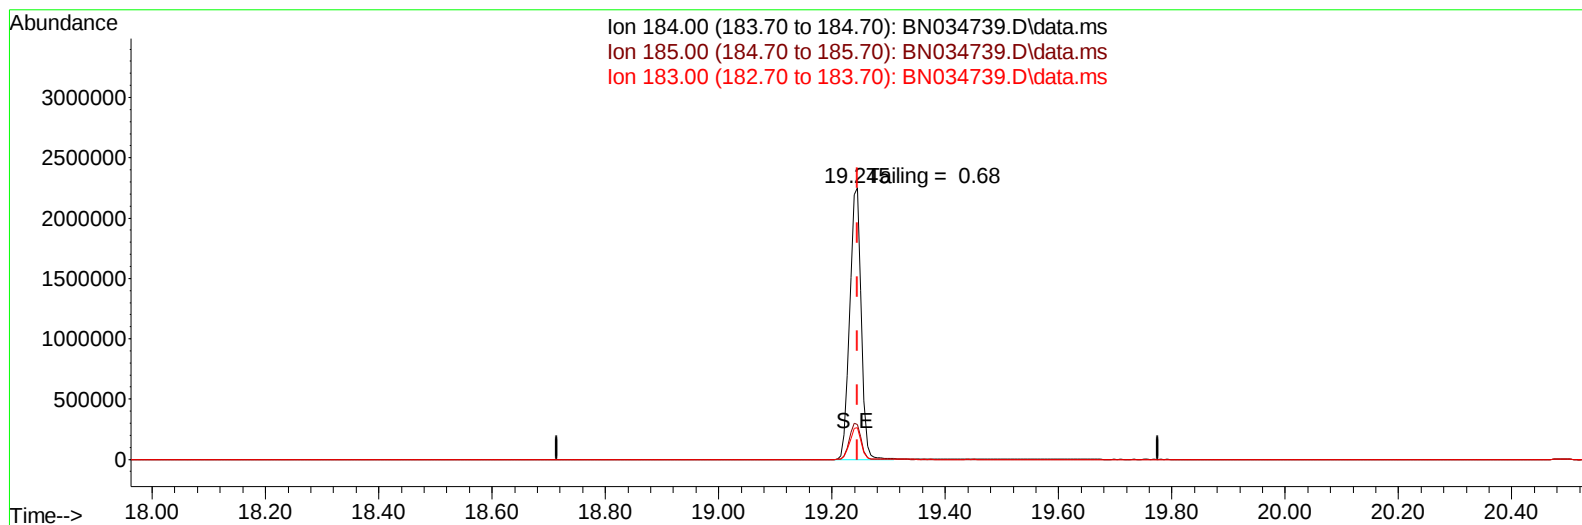

TIC: BN034739.D\data.ms

(77) Benzidine

19.245min (0.000) 766500.86 ng

response 3189736

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	12.97
183.00	13.20	11.61
0.00	0.00	0.00