

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
 Data File : BN022400.D
 Acq On : 31 Oct 2022 13:23
 Operator : CG/JU
 Sample : N5276-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4W2

Quant Time: Nov 01 01:11:30 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 01 01:09:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.927	152	4554	0.400	ng/ul	0.00
4) Naphthalene-d8	10.756	136	15060	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.605	164	8471	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.357	188	17285	0.400	ng/ul	0.00
17) Chrysene-d12	21.564	240	9794	0.400	ng/ul	0.00
23) Perylene-d12	24.014	264	7568	0.400	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.236	96	23817	4.024	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.356	152	5902	0.259	ng/ul	0.00
18) Fluoranthene-d10	19.393	212	12862	0.391	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.278	88	1226	0.202	ng/ul#	88
20) Pyrene	19.760	202	1805	0.040	ng/ul#	1
26) Benzo(a)pyrene	23.853	252	2566	0.085	ng/ul#	44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
Data File : BN022400.D
Acq On : 31 Oct 2022 13:23
Operator : CG/JU
Sample : N5276-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4W2

Quant Time: Nov 01 01:11:30 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 01 01:09:32 2022
Response via : Initial Calibration




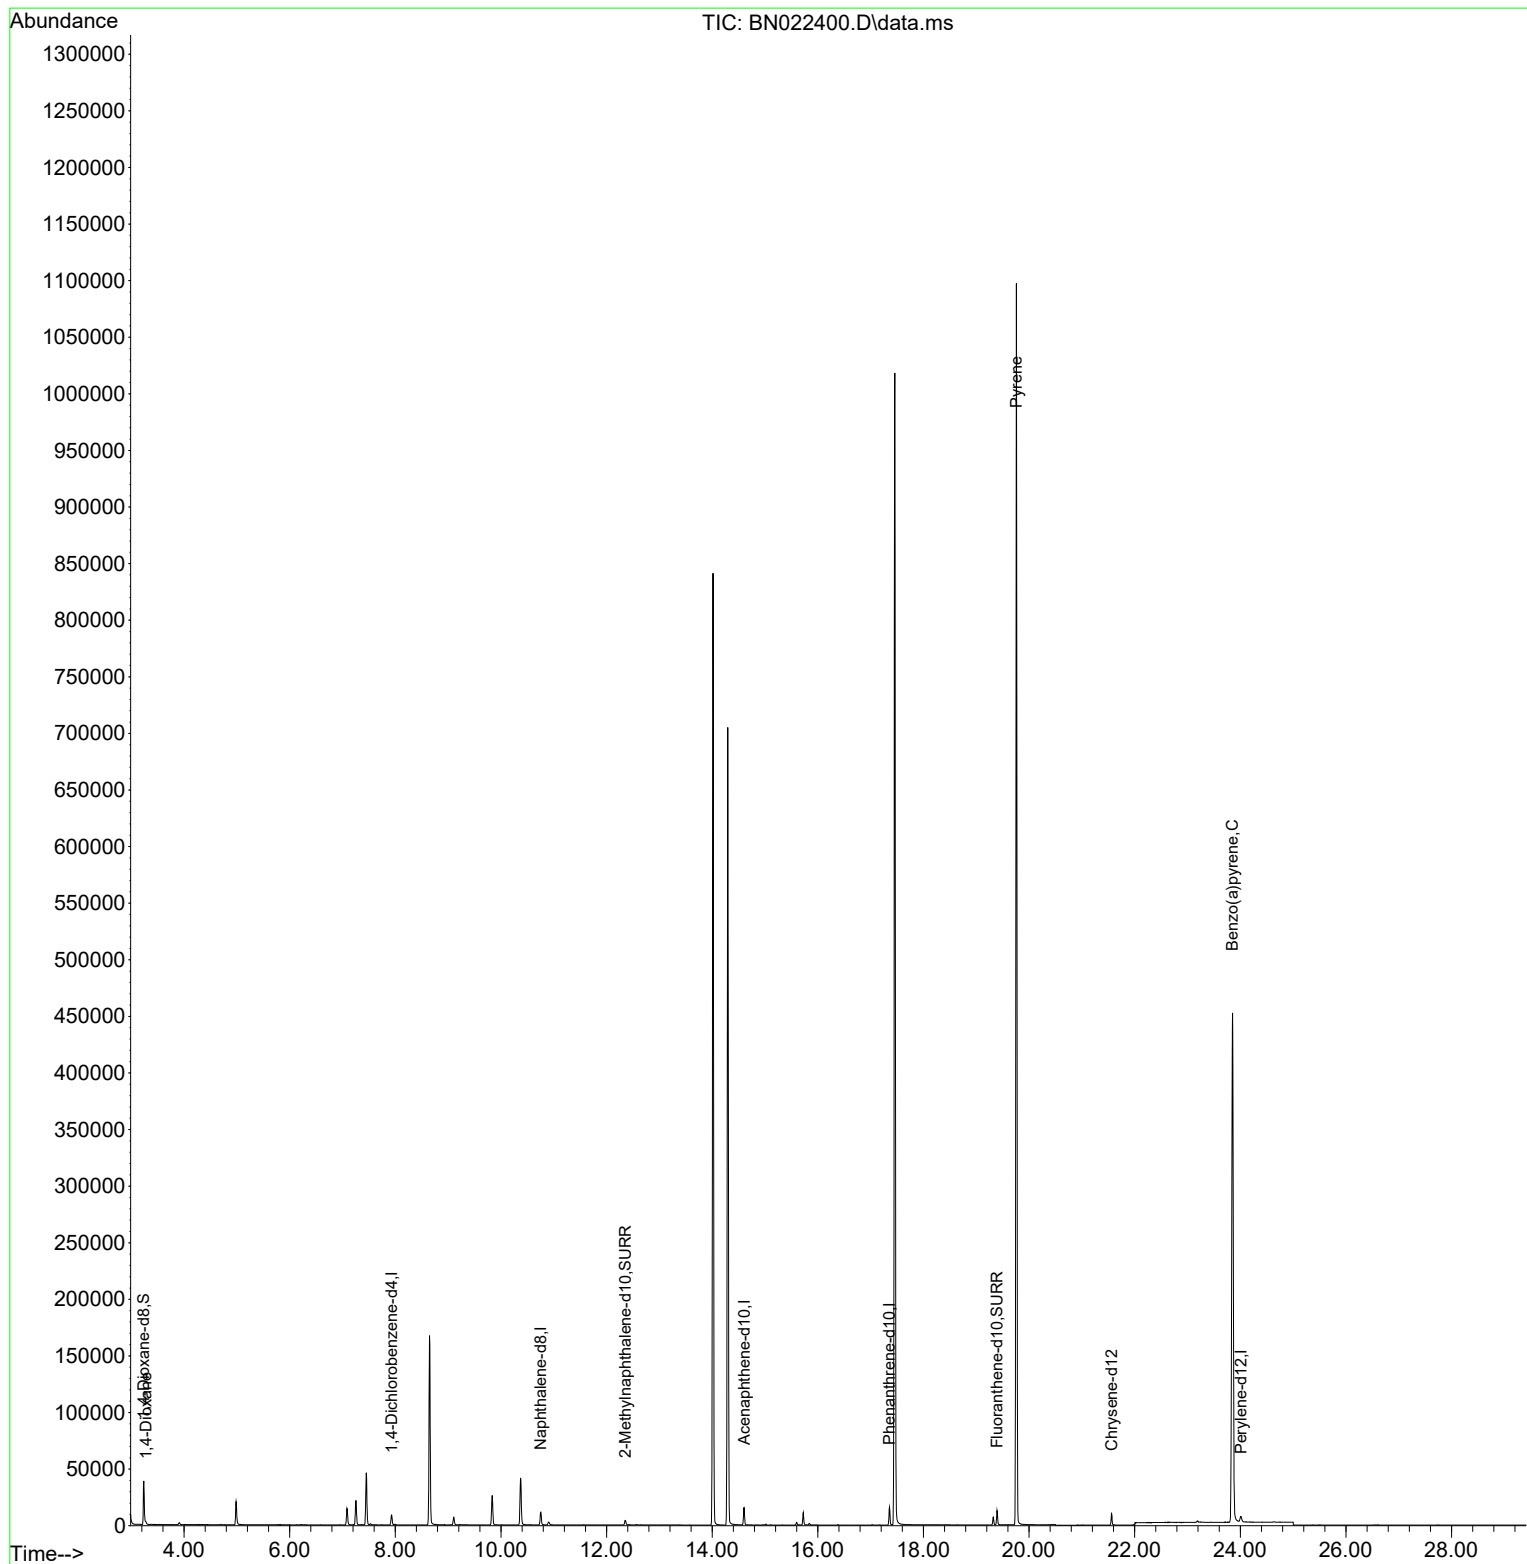


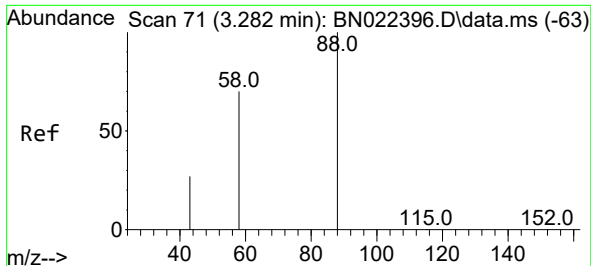

#2
1,4-Dioxane
Concen: 0.202 ng/ul
RT: 3.278 min Scan# 71
Delta R.T. -0.004 min
Lab File: BN022400.D
Acq: 31 Oct 2022 13:23




Instrument :
BNA_N
ClientSampleId :
EW4W2


Tgt Ion: 88 Resp: 1226
Ion Ratio Lower Upper
88 100
43 48.2 27.4 41.2#
58 63.7 48.2 72.2

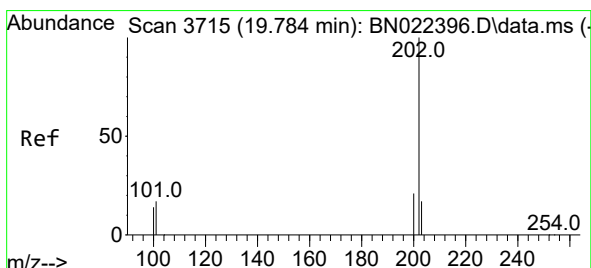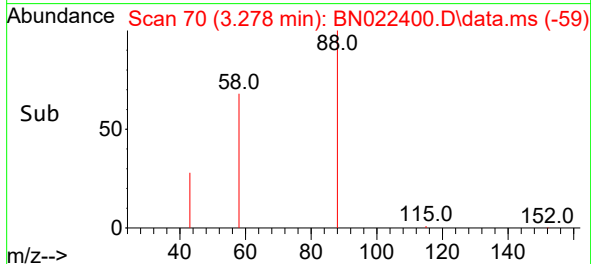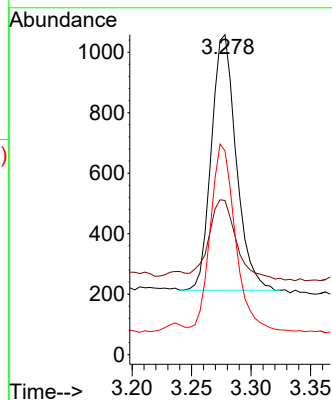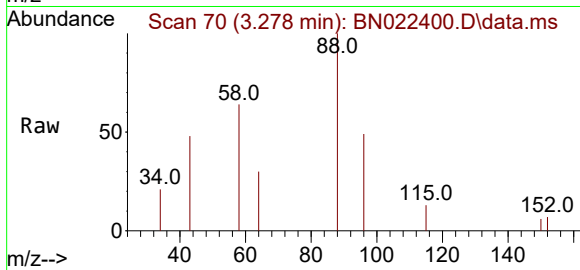

#20
Pyrene
Concen: 0.040 ng/ul
RT: 19.760 min Scan# 3710
Delta R.T. -0.023 min
Lab File: BN022400.D
Acq: 31 Oct 2022 13:23

Tgt Ion: 202 Resp: 1805
Ion Ratio Lower Upper
202 100
101 176.0 13.1 19.7#
100 1282.6 10.6 16.0#

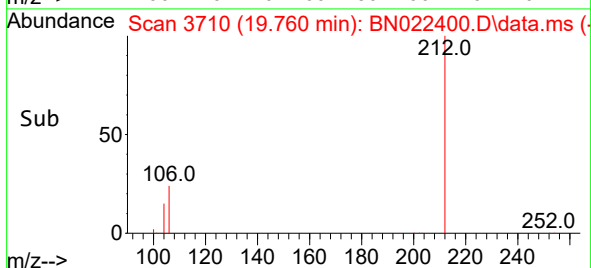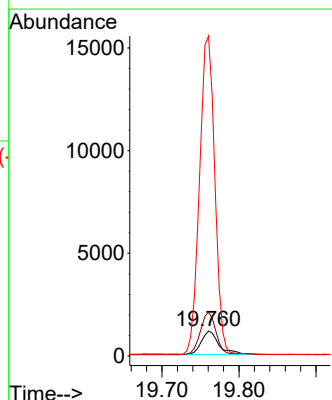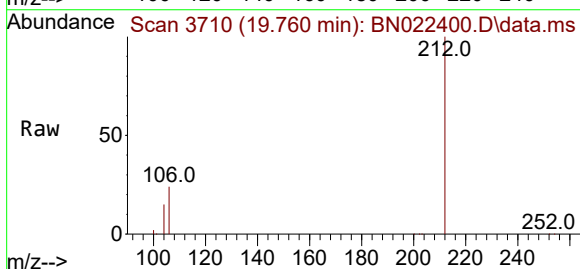

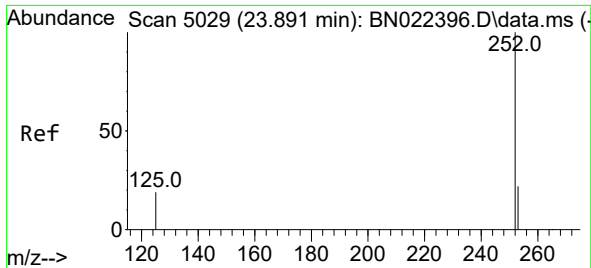

#26

Benzo(a)pyrene

Concen: 0.085 ng/ul

RT: 23.853 min Scan# 50

Delta R.T. -0.038 min

Lab File: BN022400.D


Acq: 31 Oct 2022 13:23

Instrument :

BNA_N

ClientSampleId :

EW4W2

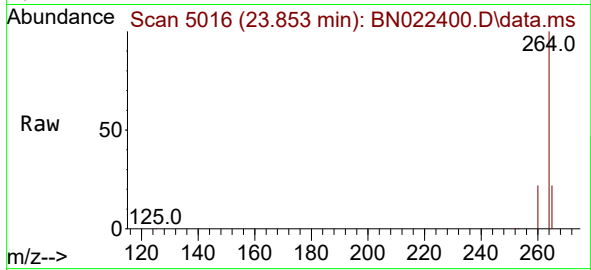

Tgt Ion:252 Resp: 2566

Ion Ratio Lower Upper

252 100

253 50.6 21.0 31.6#

125 54.1 17.9 26.9#

