

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
 Data File : BN022401.D
 Acq On : 31 Oct 2022 14:00
 Operator : CG/JU
 Sample : N5277-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4W2

Quant Time: Nov 01 01:11:35 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 01 01:09:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	3750	0.400	ng/ul	0.00
4) Naphthalene-d8	10.750	136	12240	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.600	164	6909	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.353	188	14331	0.400	ng/ul	0.00
17) Chrysene-d12	21.559	240	8422	0.400	ng/ul	0.00
23) Perylene-d12	24.008	264	6324	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.236	96	20621	4.231	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.351	152	5788	0.313	ng/ul	0.00
18) Fluoranthene-d10	19.389	212	13255	0.469	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.274	88	899	0.180	ng/ul#	85
20) Pyrene	19.761	202	1833	0.047	ng/ul#	1
26) Benzo(a)pyrene	23.847	252	2710	0.107	ng/ul#	46


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
Data File : BN022401.D
Acq On : 31 Oct 2022 14:00
Operator : CG/JU
Sample : N5277-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4W2

Quant Time: Nov 01 01:11:35 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 01 01:09:32 2022
Response via : Initial Calibration




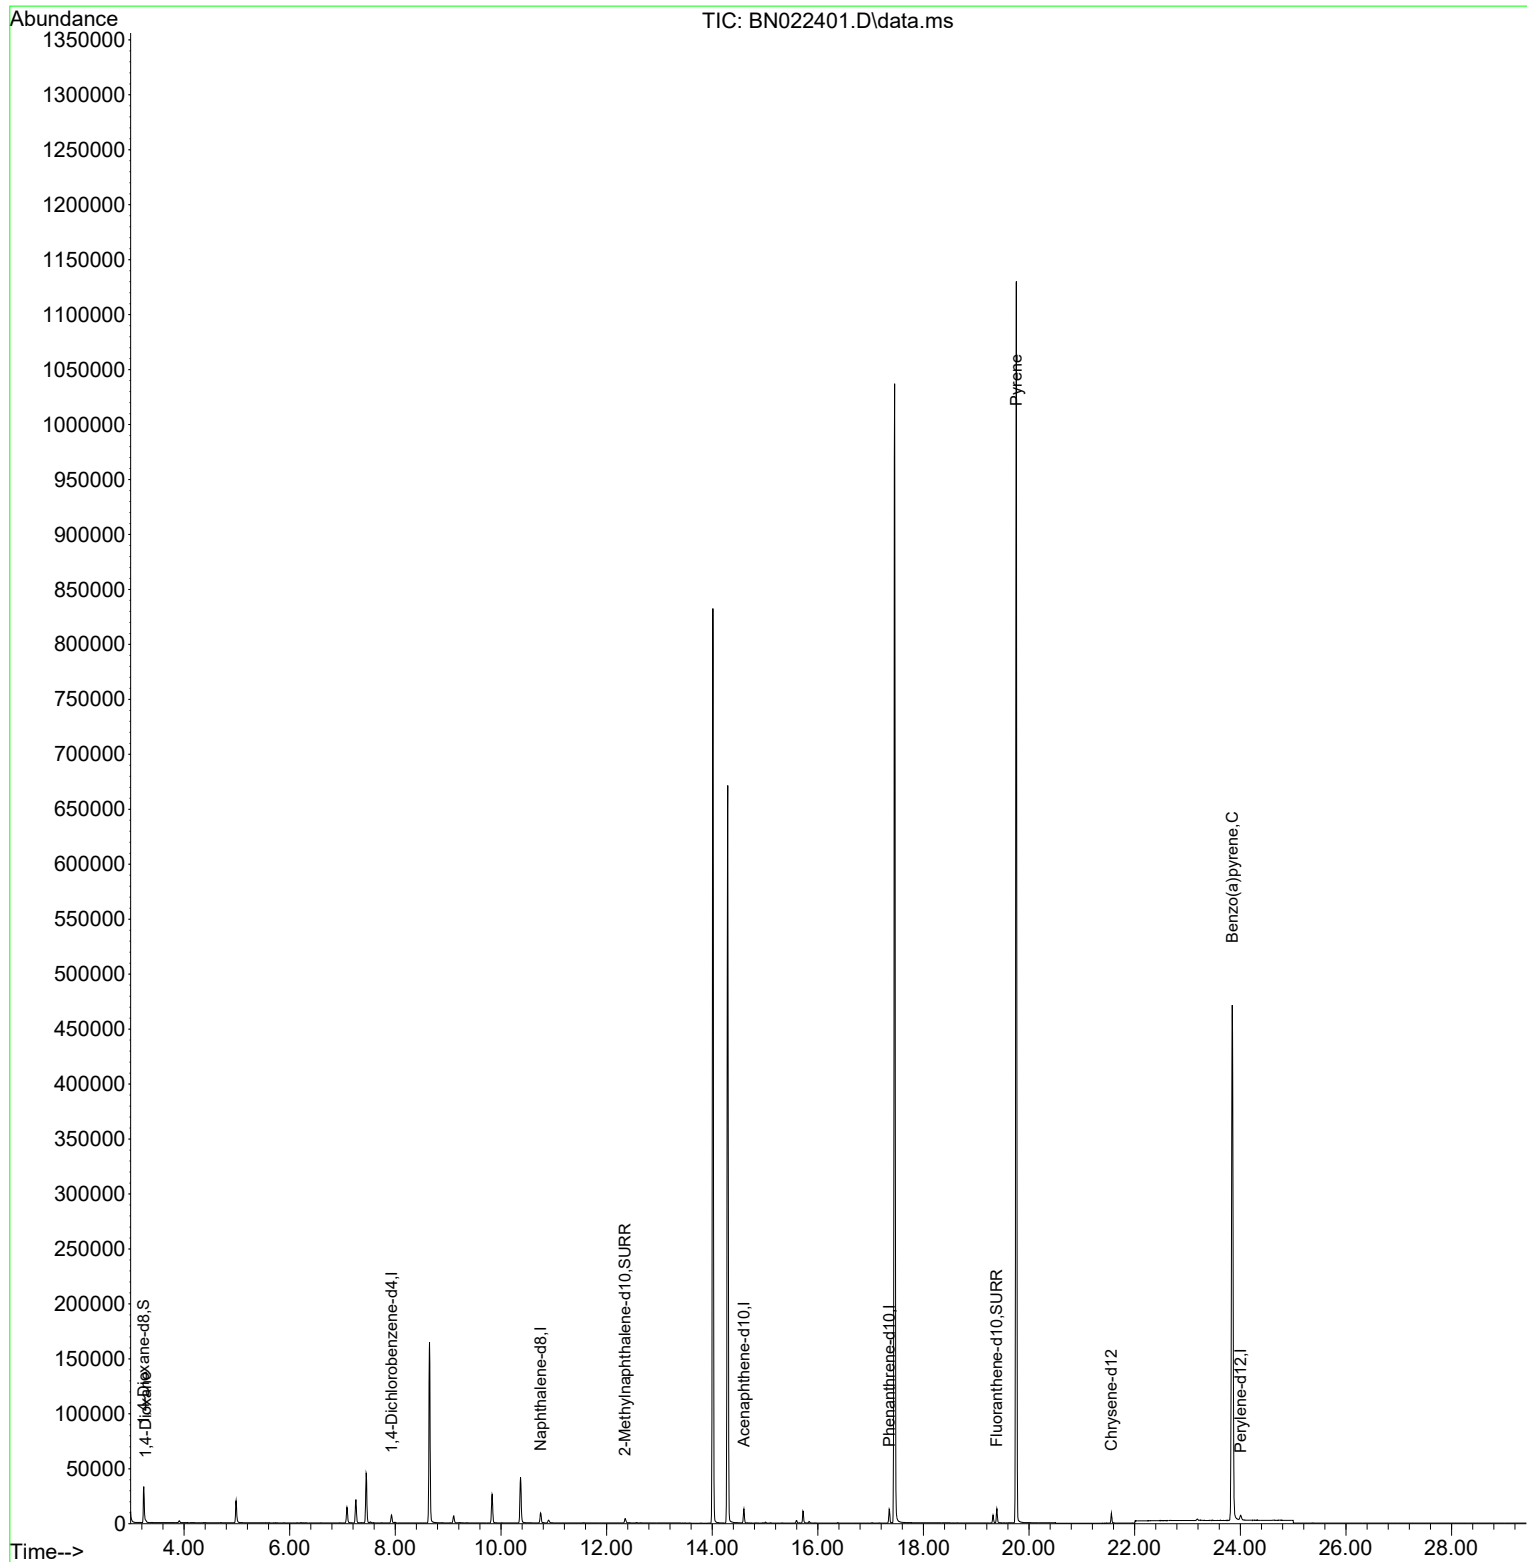


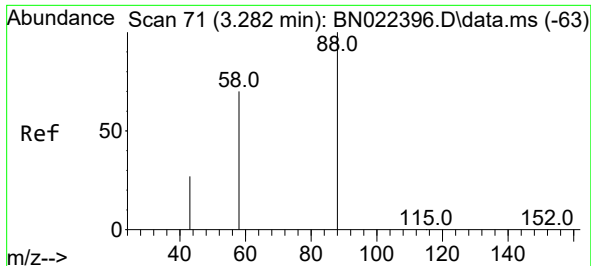

#2
 1,4-Dioxane
 Concen: 0.180 ng/ul
 RT: 3.274 min Scan# 61
 Delta R.T. -0.008 min
 Lab File: BN022401.D
 Acq: 31 Oct 2022 14:00




Instrument :
 BNA_N
 ClientSampleId :
 EW4W2


Tgt Ion: 88 Resp: 899
 Ion Ratio Lower Upper
 88 100
 43 52.1 27.4 41.2#
 58 64.7 48.2 72.2

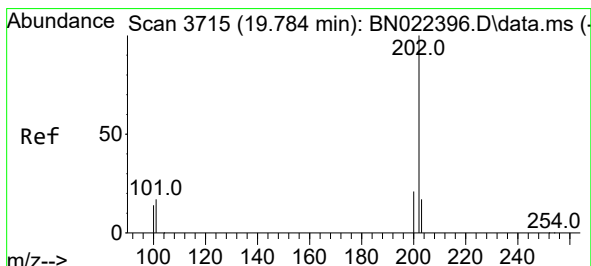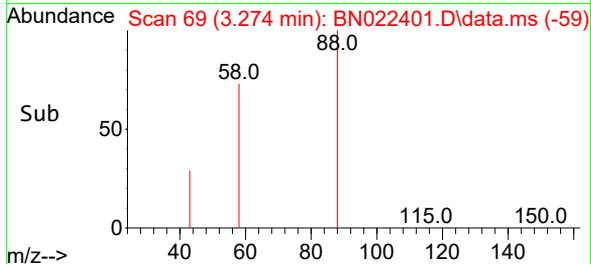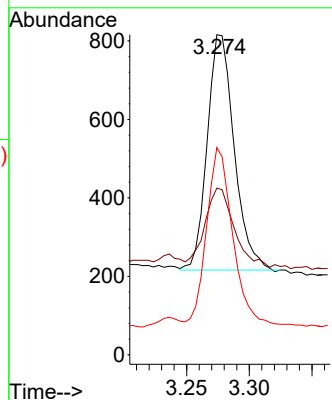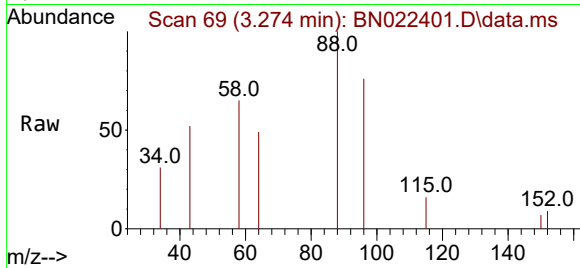

#20
 Pyrene
 Concen: 0.047 ng/ul
 RT: 19.761 min Scan# 3710
 Delta R.T. -0.023 min
 Lab File: BN022401.D
 Acq: 31 Oct 2022 14:00


Tgt Ion: 202 Resp: 1833
 Ion Ratio Lower Upper
 202 100
 101 169.8 13.1 19.7#
 100 1185.5 10.6 16.0#

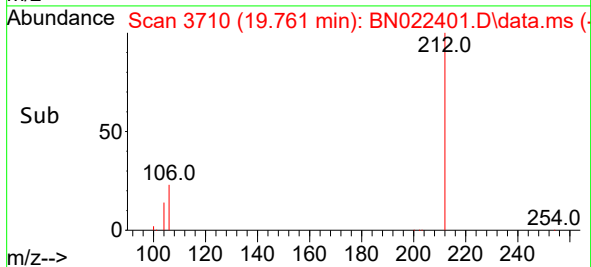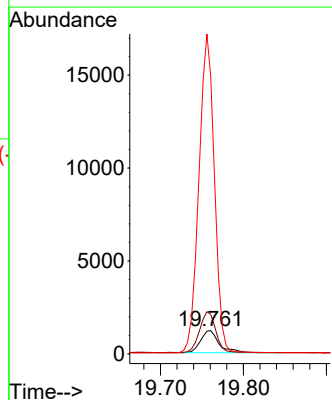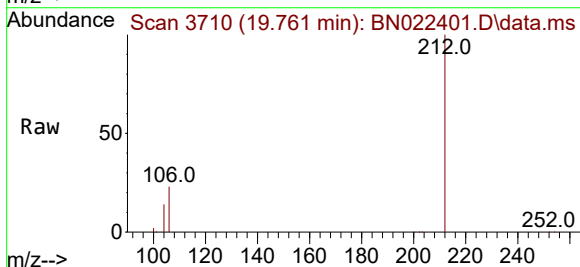

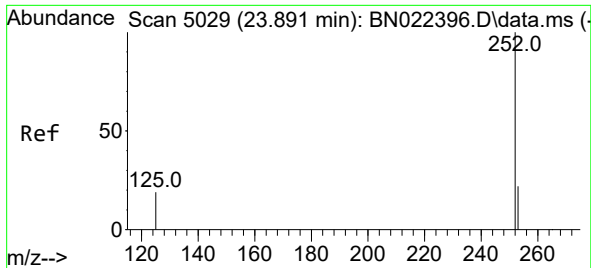

#26
Benzo(a)pyrene
Concen: 0.107 ng/ul
RT: 23.847 min Scan# 50
Delta R.T. -0.044 min
Lab File: BN022401.D
Acq: 31 Oct 2022 14:00

Instrument :
BNA_N
ClientSampleId :
EW4W2

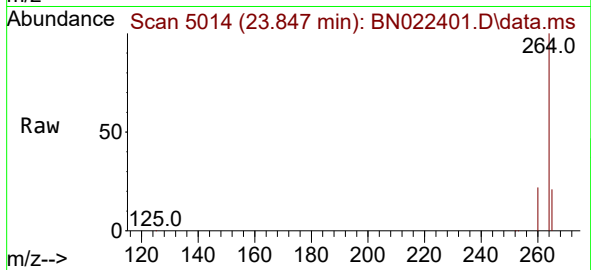

Tgt Ion:252 Resp: 2710
Ion Ratio Lower Upper
252 100
253 50.4 21.0 31.6#
125 52.4 17.9 26.9#

