

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
 Data File : BN022403.D
 Acq On : 31 Oct 2022 15:34
 Operator : CG/JU
 Sample : N5277-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4W3

Quant Time: Nov 01 01:11:46 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 01 01:09:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	4291	0.400	ng/ul	0.00
4) Naphthalene-d8	10.756	136	14115	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.600	164	7858	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.358	188	15488	0.400	ng/ul	0.00
17) Chrysene-d12	21.559	240	8828	0.400	ng/ul	0.00
23) Perylene-d12	24.005	264	6950	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.236	96	21830	3.915	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.351	152	6714	0.314	ng/ul	0.00
18) Fluoranthene-d10	19.393	212	13651	0.461	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.278	88	959	0.167	ng/ul#	87
20) Pyrene	19.761	202	1813	0.045	ng/ul#	1
26) Benzo(a)pyrene	23.847	252	2781	0.100	ng/ul#	50


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
Data File : BN022403.D
Acq On : 31 Oct 2022 15:34
Operator : CG/JU
Sample : N5277-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4W3

Quant Time: Nov 01 01:11:46 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 01 01:09:32 2022
Response via : Initial Calibration




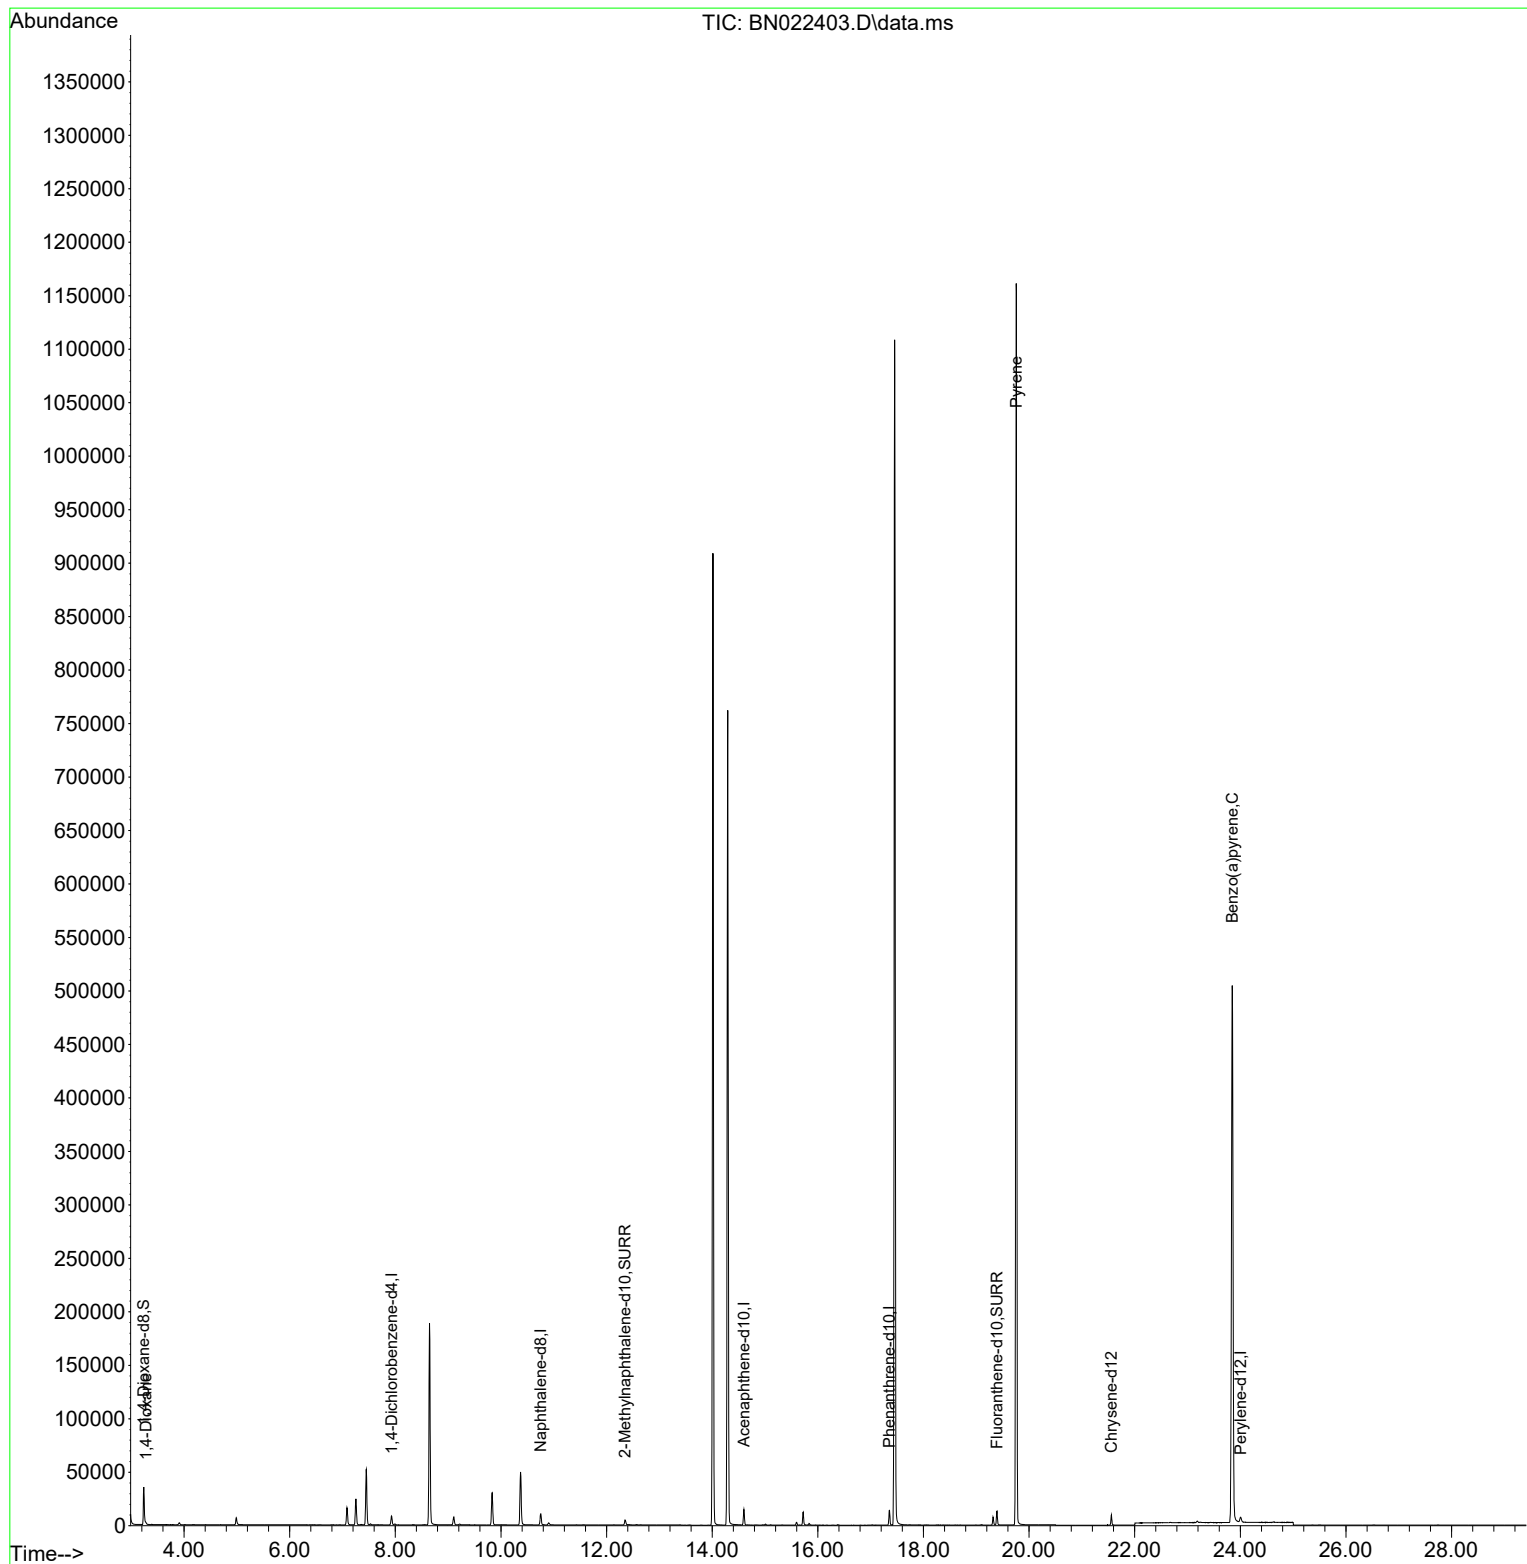


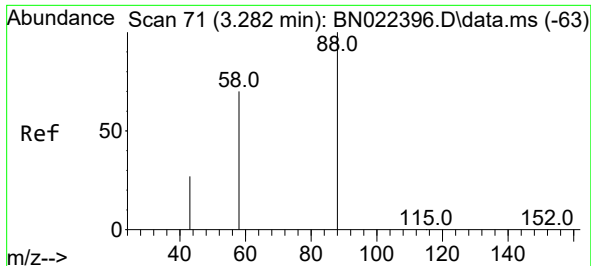

#2
1,4-Dioxane
Concen: 0.167 ng/ul
RT: 3.278 min Scan# 71
Delta R.T. -0.004 min
Lab File: BN022403.D
Acq: 31 Oct 2022 15:34




Instrument :
BNA_N
ClientSampleId :
EW4W3


Tgt Ion: 88 Resp: 959
Ion Ratio Lower Upper
88 100
43 51.4 27.4 41.2#
58 62.5 48.2 72.2

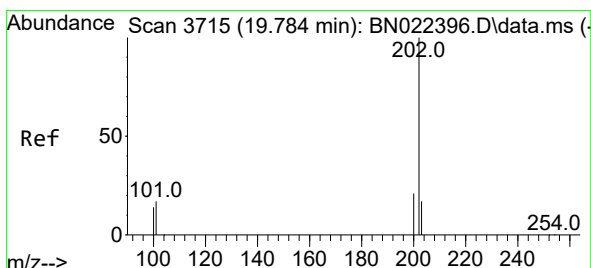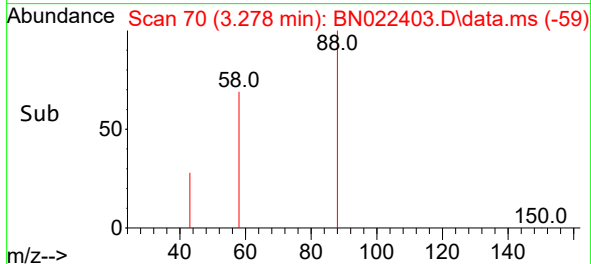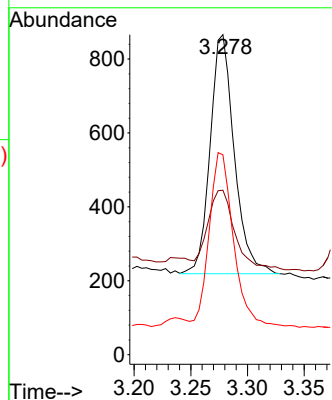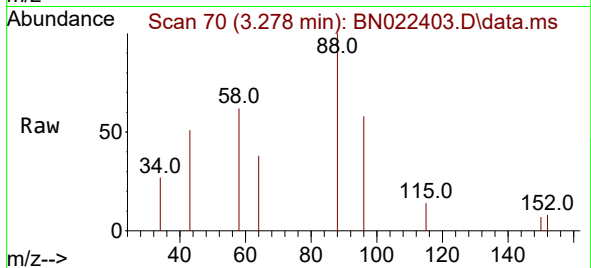

#20
Pyrene
Concen: 0.045 ng/ul
RT: 19.761 min Scan# 3710
Delta R.T. -0.023 min
Lab File: BN022403.D
Acq: 31 Oct 2022 15:34


Tgt Ion: 202 Resp: 1813
Ion Ratio Lower Upper
202 100
101 175.9 13.1 19.7#
100 1234.9 10.6 16.0#

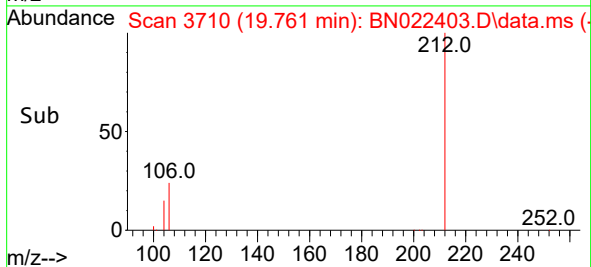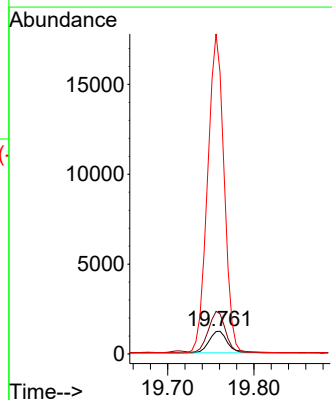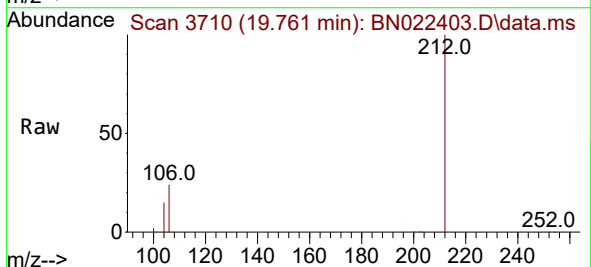

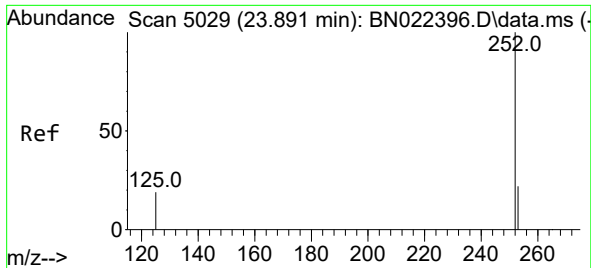

#26
Benzo(a)pyrene
Concen: 0.100 ng/ul
RT: 23.847 min Scan# 50
Delta R.T. -0.044 min
Lab File: BN022403.D
Acq: 31 Oct 2022 15:34

Instrument :
BNA_N
ClientSampleId :
EW4W3

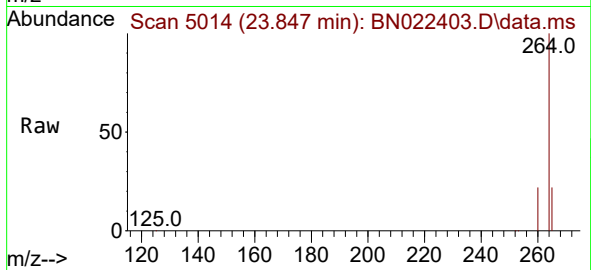

Tgt Ion:252 Resp: 2781
Ion Ratio Lower Upper
252 100
253 48.2 21.0 31.6#
125 50.6 17.9 26.9#

