

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
 Data File : BN022405.D
 Acq On : 31 Oct 2022 17:28
 Operator : CG/JU
 Sample : N5277-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4W4

Quant Time: Nov 01 01:11:56 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 01 01:09:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	4507	0.400	ng/ul	0.00
4) Naphthalene-d8	10.756	136	14989	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.600	164	8462	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.357	188	16665	0.400	ng/ul	0.00
17) Chrysene-d12	21.559	240	9553	0.400	ng/ul	0.00
23) Perylene-d12	24.005	264	7071	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.236	96	23100	3.944	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.356	152	6742	0.297	ng/ul	0.00
18) Fluoranthene-d10	19.393	212	13276	0.414	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.278	88	1047	0.174	ng/ul#	87
20) Pyrene	19.761	202	1788	0.041	ng/ul#	1
26) Benzo(a)pyrene	23.847	252	2619	0.093	ng/ul#	48


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
Data File : BN022405.D
Acq On : 31 Oct 2022 17:28
Operator : CG/JU
Sample : N5277-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4W4

Quant Time: Nov 01 01:11:56 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 01 01:09:32 2022
Response via : Initial Calibration




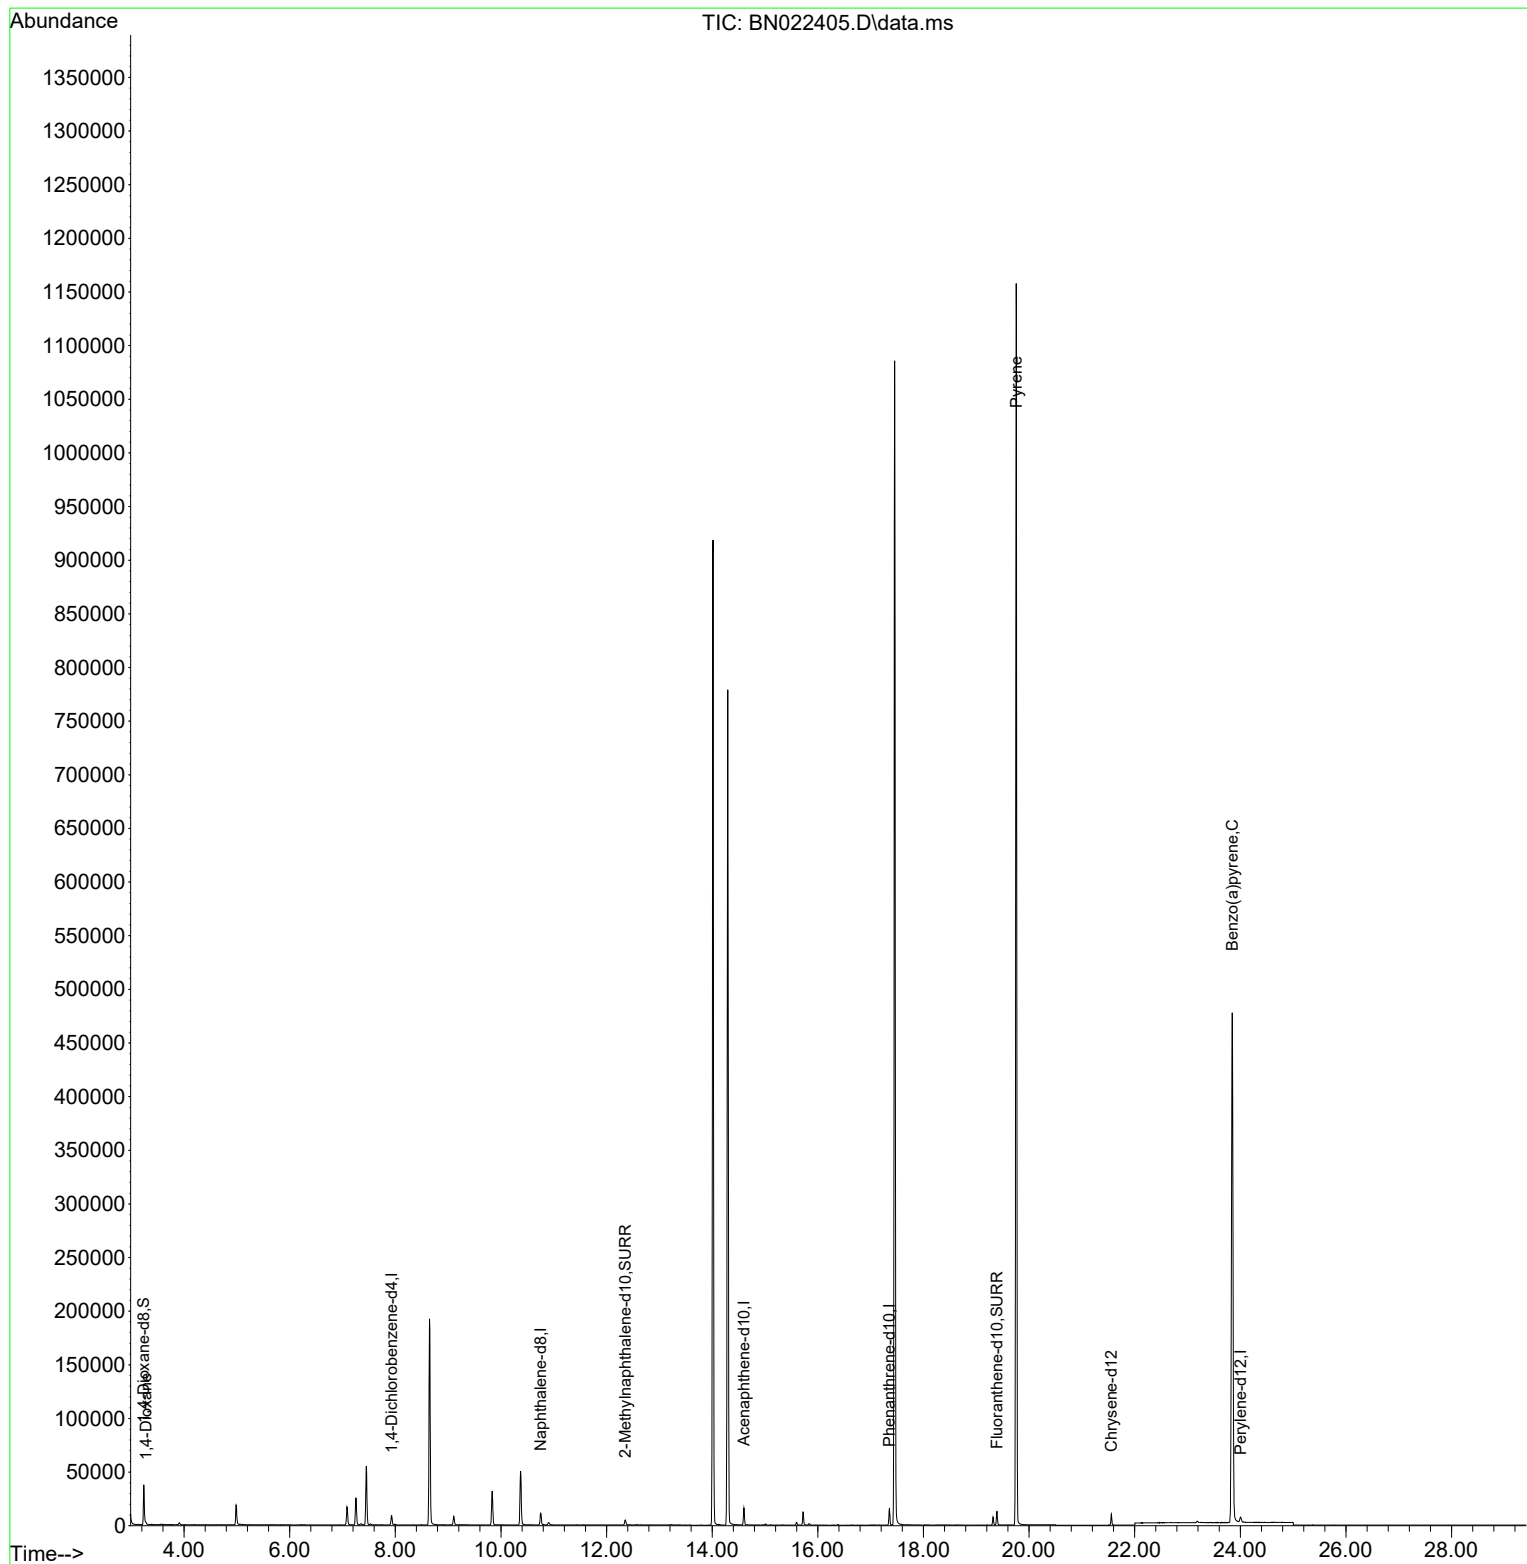


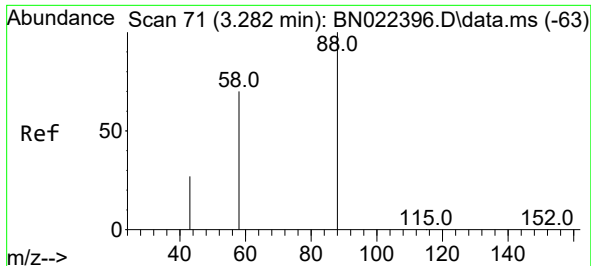

#2
1,4-Dioxane
Concen: 0.174 ng/ul
RT: 3.278 min Scan# 71
Delta R.T. -0.004 min
Lab File: BN022405.D
Acq: 31 Oct 2022 17:28




Instrument :
BNA_N
ClientSampleId :
EW4W4


Tgt Ion: 88 Resp: 1047
Ion Ratio Lower Upper
88 100
43 49.9 27.4 41.2#
58 63.6 48.2 72.2

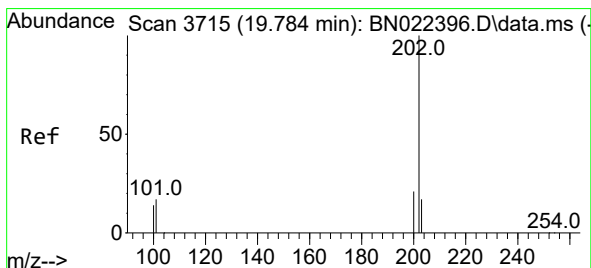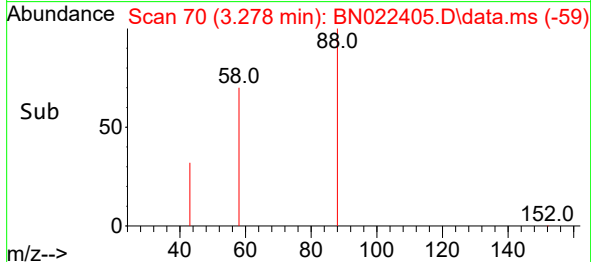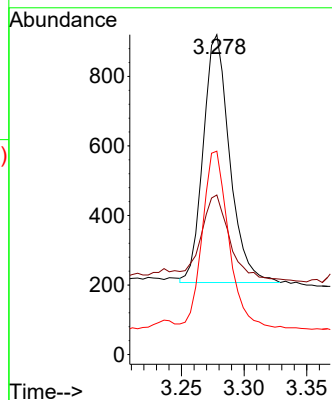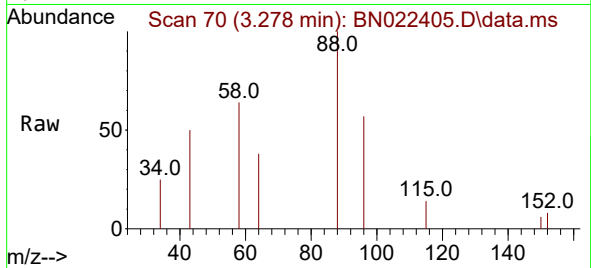

#20
Pyrene
Concen: 0.041 ng/ul
RT: 19.761 min Scan# 3710
Delta R.T. -0.023 min
Lab File: BN022405.D
Acq: 31 Oct 2022 17:28

Tgt Ion: 202 Resp: 1788
Ion Ratio Lower Upper
202 100
101 167.0 13.1 19.7#
100 1175.9 10.6 16.0#

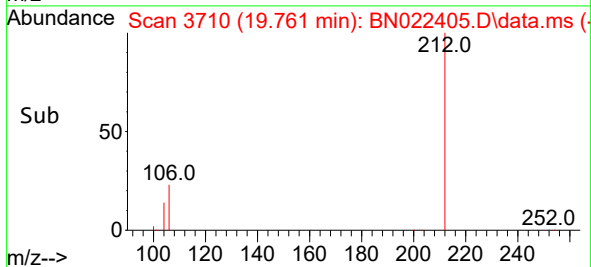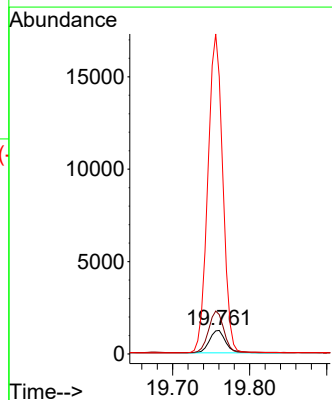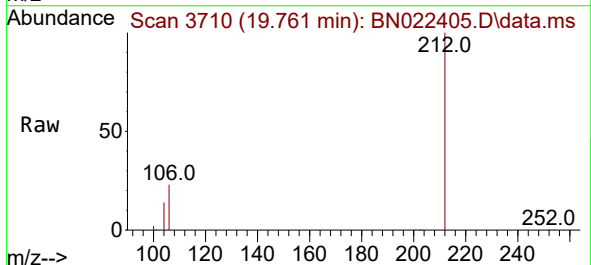

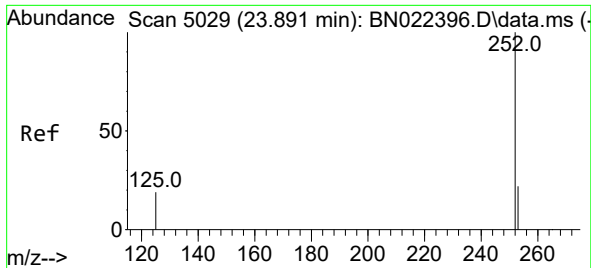

#26

Benzo(a)pyrene

Concen: 0.093 ng/ul

RT: 23.847 min Scan# 50

Delta R.T. -0.044 min

Lab File: BN022405.D


Acq: 31 Oct 2022 17:28

Instrument :

BNA_N

ClientSampleId :

EW4W4

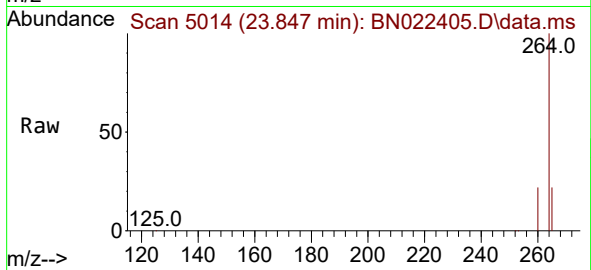

Tgt Ion:252 Resp: 2619

Ion Ratio Lower Upper

252 100

253 49.1 21.0 31.6#

125 51.9 17.9 26.9#

