

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
 Data File : BN022409.D
 Acq On : 31 Oct 2022 20:38
 Operator : CG/JU
 Sample : PB148646BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK646

Quant Time: Nov 01 01:12:23 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 01 01:09:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	4354	0.400	ng/ul	0.00
4) Naphthalene-d8	10.756	136	14550	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.600	164	8155	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.358	188	16318	0.400	ng/ul	0.00
17) Chrysene-d12	21.559	240	9518	0.400	ng/ul	0.00
23) Perylene-d12	24.002	264	6999	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.236	96	32263	5.702	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.356	152	6372	0.289	ng/ul	0.00
18) Fluoranthene-d10	19.394	212	11080	0.347	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.595	166	2162	0.060	ng/ul#	14
20) Pyrene	19.756	202	1601	0.037	ng/ul#	1
26) Benzo(a)pyrene	23.842	252	2433	0.087	ng/ul#	46


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
Data File : BN022409.D
Acq On : 31 Oct 2022 20:38
Operator : CG/JU
Sample : PB148646BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK646

Quant Time: Nov 01 01:12:23 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 01 01:09:32 2022
Response via : Initial Calibration




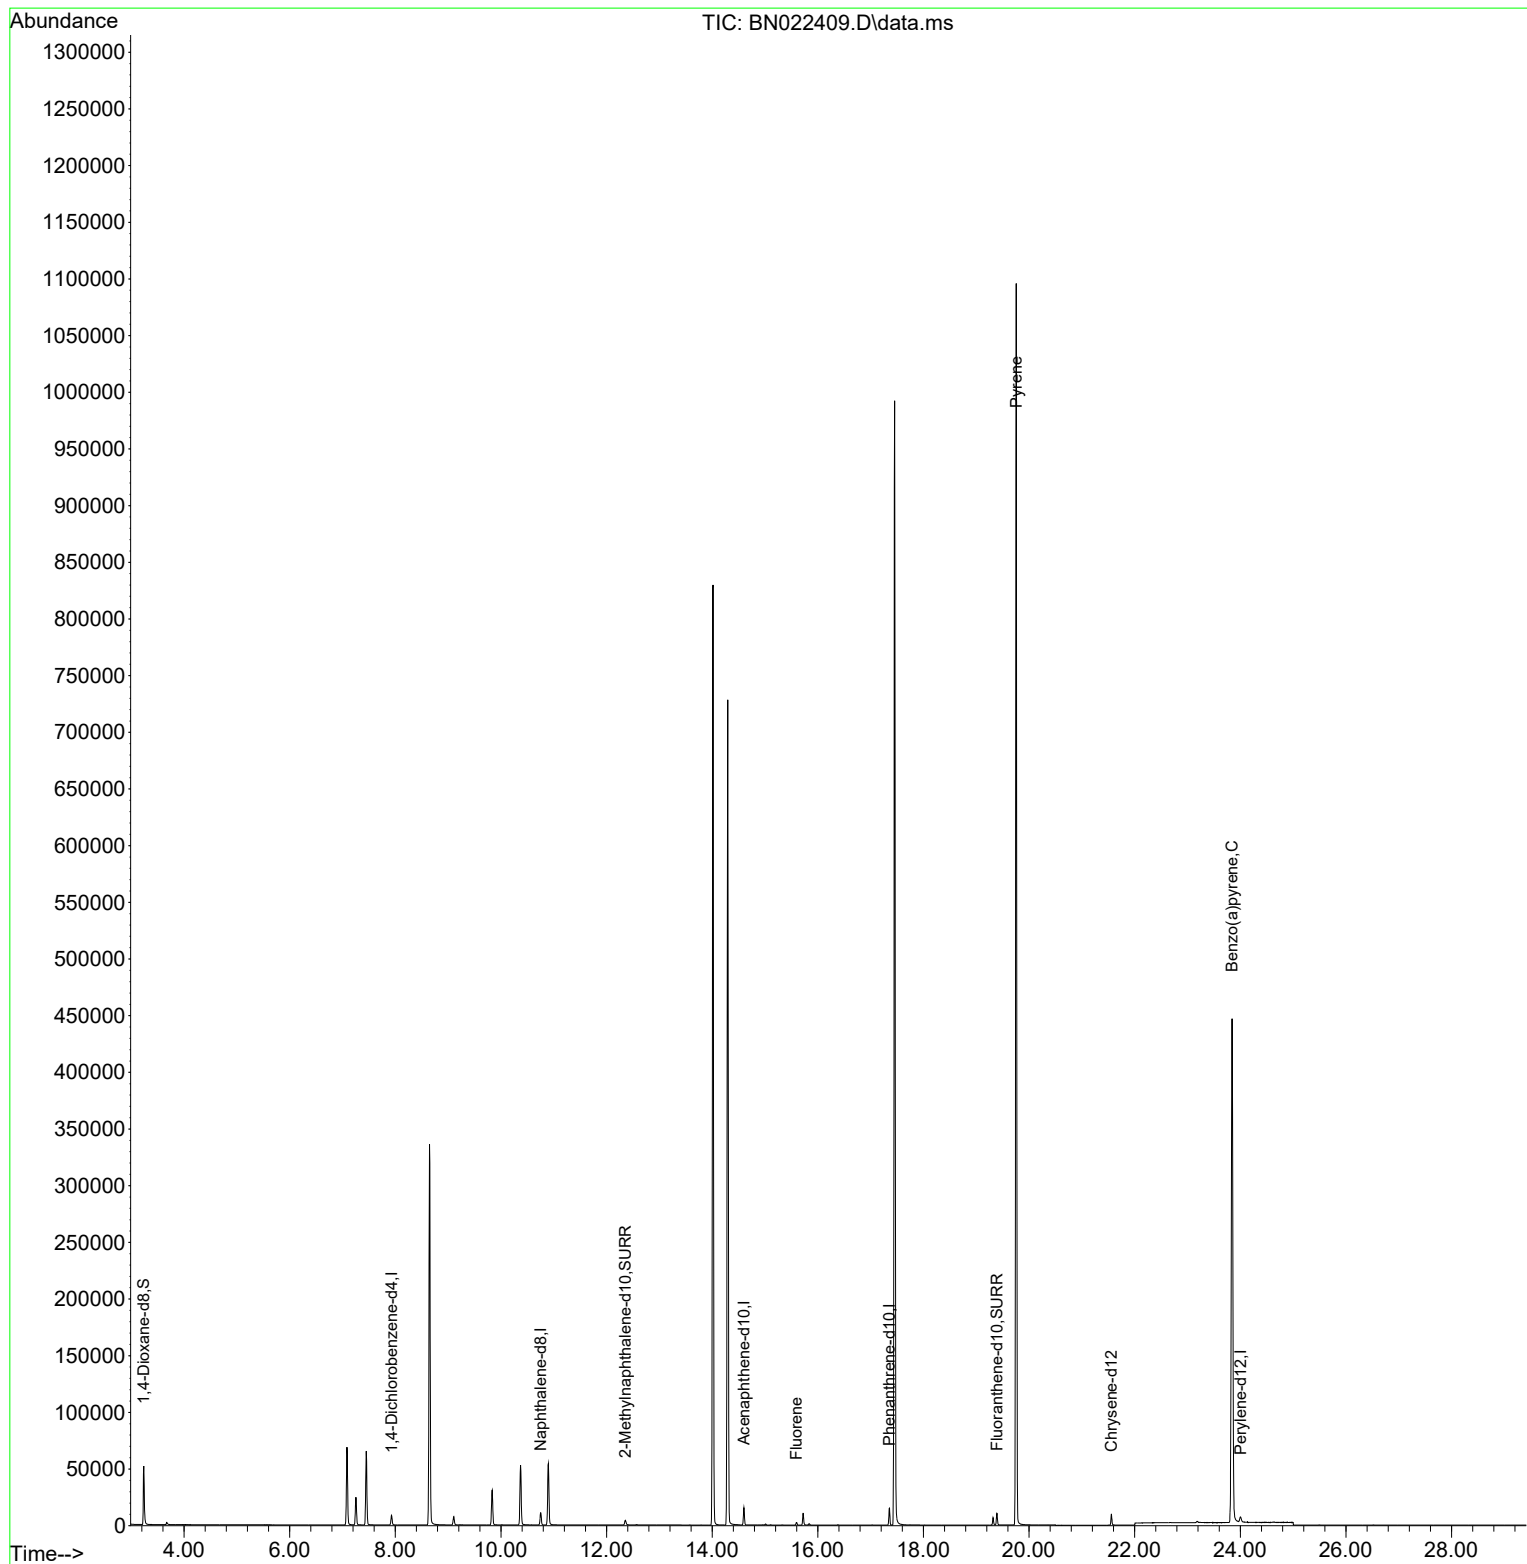


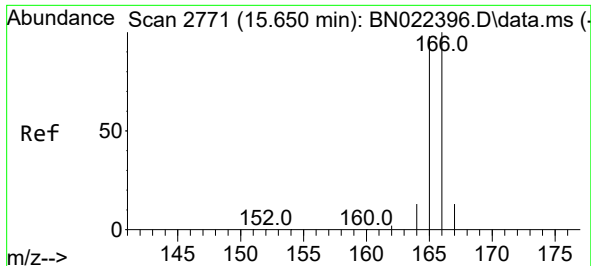

#12
Fluorene
Concen: 0.060 ng/ul
RT: 15.595 min Scan# 21
Delta R.T. -0.055 min
Lab File: BN022409.D
Acq: 31 Oct 2022 20:38




Instrument :
BNA_N
ClientSampleId :
SBLK646


Tgt Ion:166 Resp: 2162
Ion Ratio Lower Upper
166 100
165 7.0 78.2 117.2#
167 31.8 11.0 16.4#

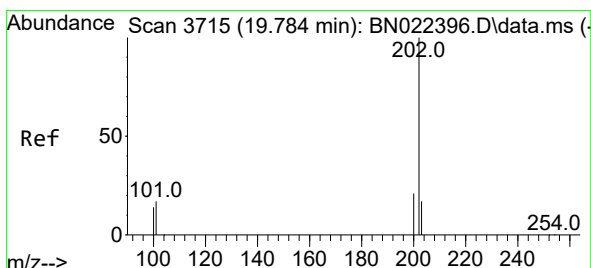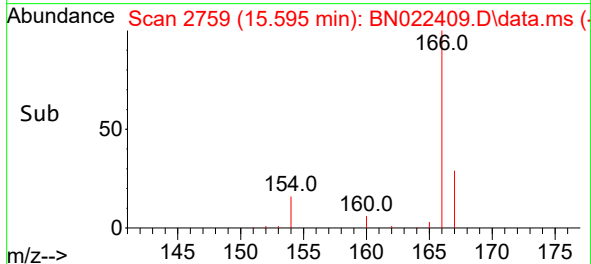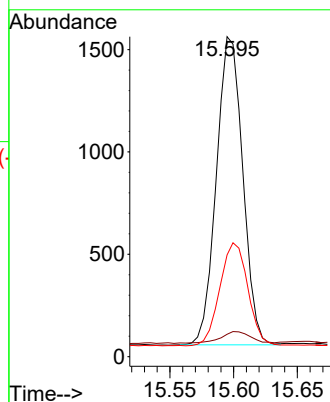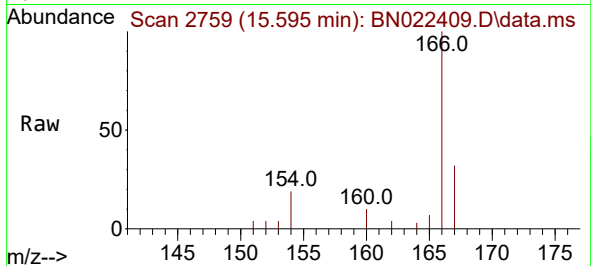

#20
Pyrene
Concen: 0.037 ng/ul
RT: 19.756 min Scan# 3709
Delta R.T. -0.028 min
Lab File: BN022409.D
Acq: 31 Oct 2022 20:38


Tgt Ion:202 Resp: 1601
Ion Ratio Lower Upper
202 100
101 181.5 13.1 19.7#
100 1339.5 10.6 16.0#

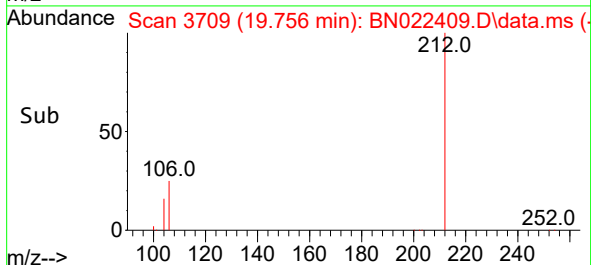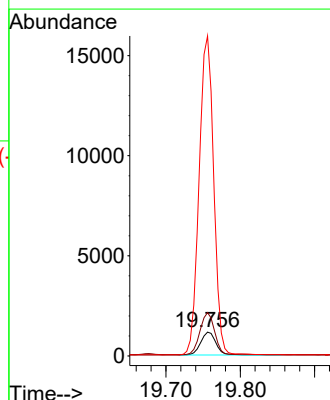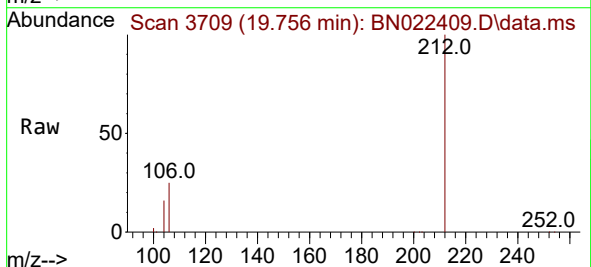

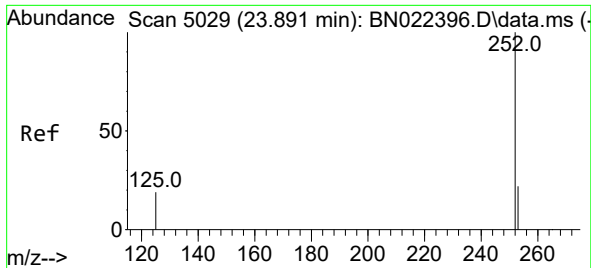

#26
Benzo(a)pyrene
Concen: 0.087 ng/ul
RT: 23.842 min Scan# 50
Delta R.T. -0.050 min
Lab File: BN022409.D
Acq: 31 Oct 2022 20:38

Instrument :
BNA_N
ClientSampleId :
SBLK646

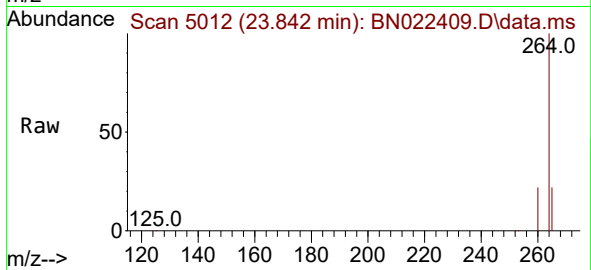

Tgt Ion:252 Resp: 2433
Ion Ratio Lower Upper
252 100
253 49.9 21.0 31.6#
125 53.3 17.9 26.9#

