

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
 Data File : BN022434.D
 Acq On : 01 Nov 2022 12:50
 Operator : CG/JU
 Sample : N5276-17
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4X7

Quant Time: Nov 02 00:53:27 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 01 01:09:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.927	152	4915	0.400	ng/ul	0.00
4) Naphthalene-d8	10.750	136	16721	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.600	164	9358	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.353	188	18365	0.400	ng/ul	0.00
17) Chrysene-d12	21.556	240	9996	0.400	ng/ul	0.00
23) Perylene-d12	23.999	264	7629	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.236	96	27575	4.317	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.351	152	9356	0.370	ng/ul	0.00
18) Fluoranthene-d10	19.389	212	16238	0.484	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.274	88	1216	0.185	ng/ul#	86
20) Pyrene	19.756	202	2405	0.052	ng/ul#	1
26) Benzo(a)pyrene	23.841	252	3146	0.103	ng/ul#	52


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
Data File : BN022434.D
Acq On : 01 Nov 2022 12:50
Operator : CG/JU
Sample : N5276-17
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4X7

Quant Time: Nov 02 00:53:27 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 01 01:09:32 2022
Response via : Initial Calibration




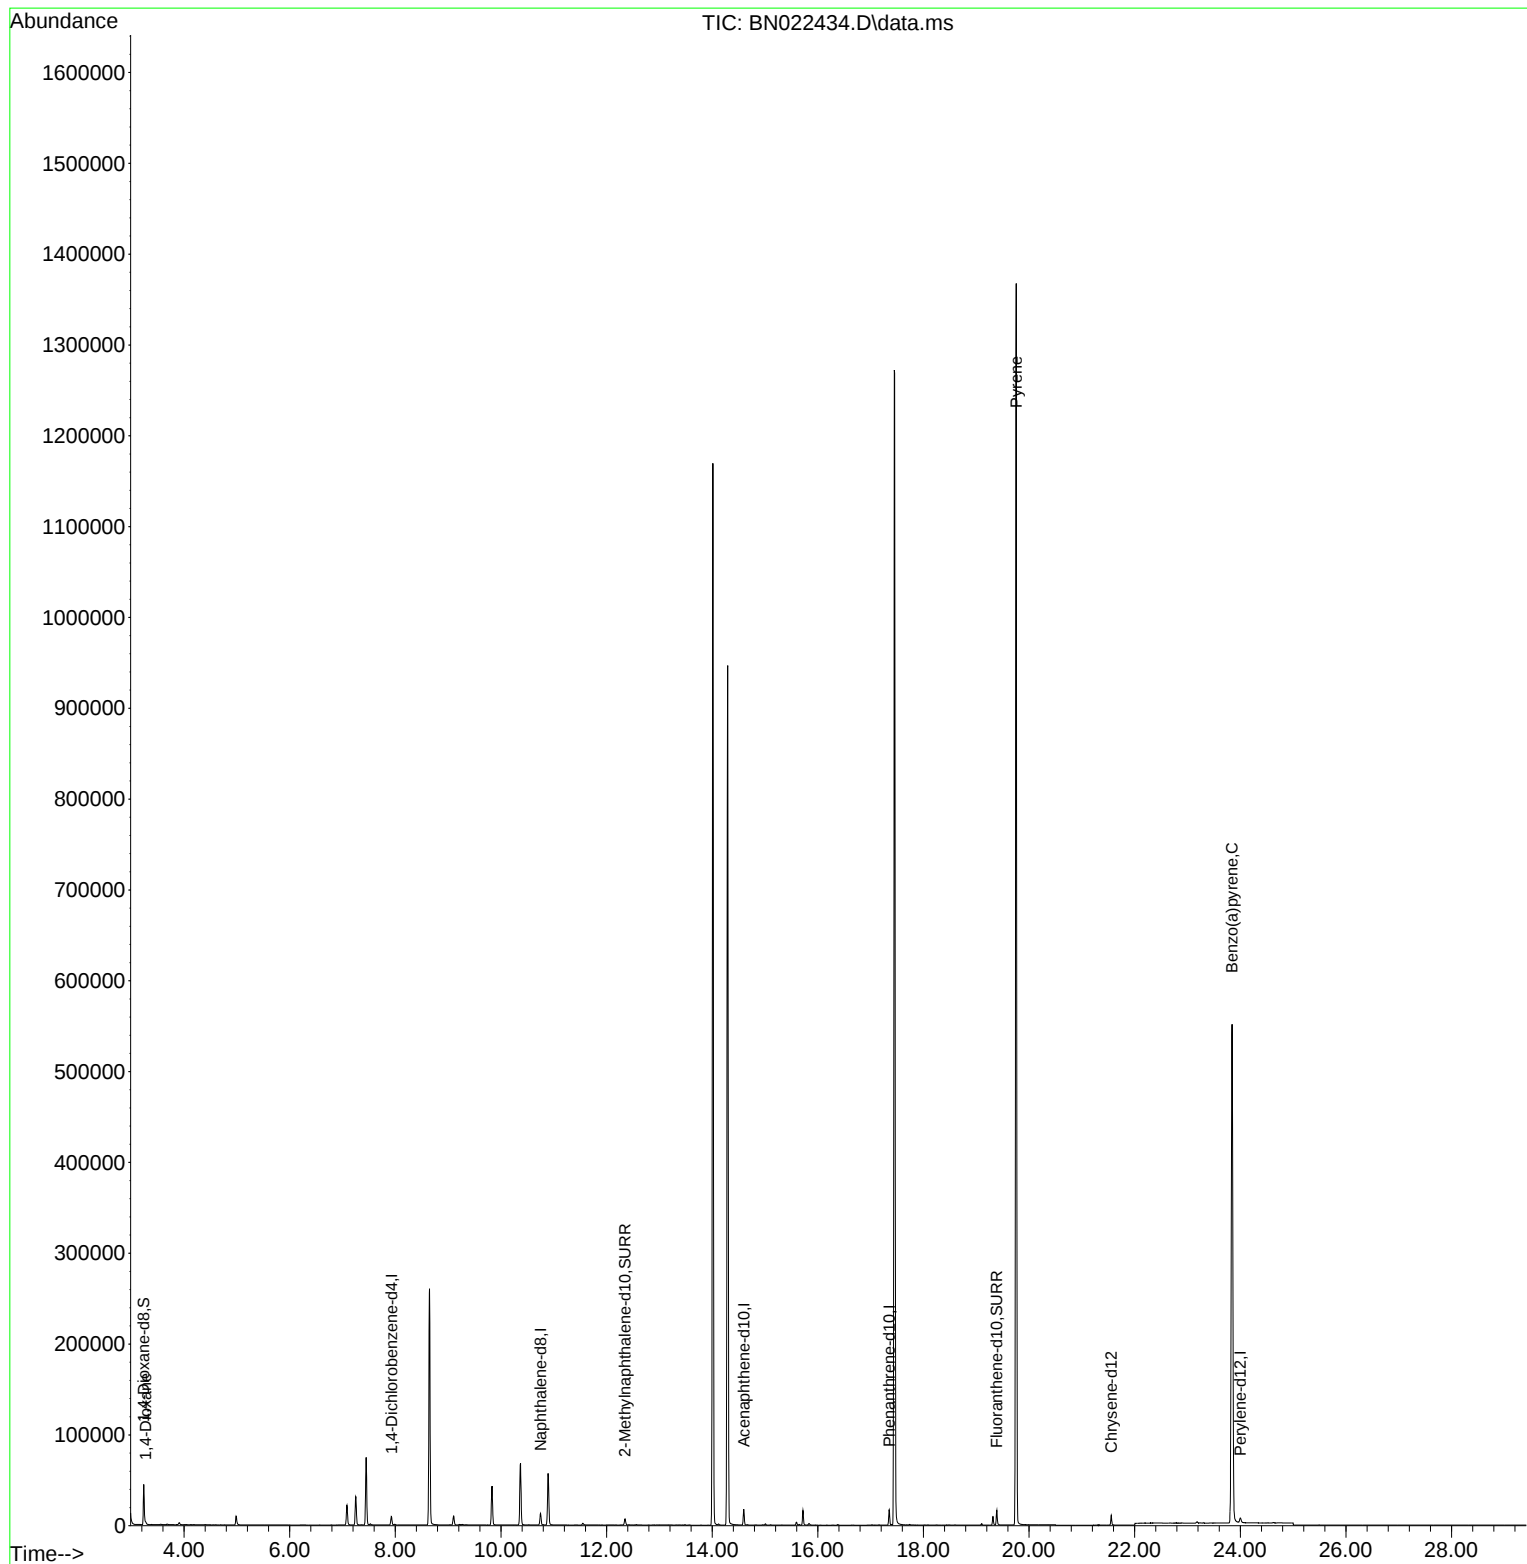


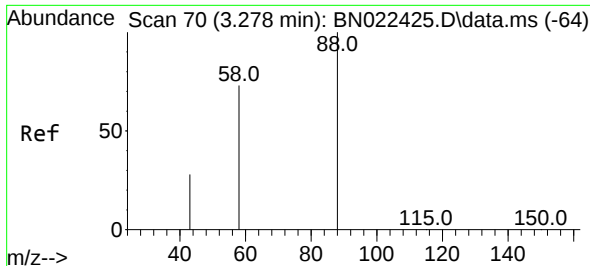

#2
 1,4-Dioxane
 Concen: 0.185 ng/ul
 RT: 3.274 min Scan# 61
 Delta R.T. -0.009 min
 Lab File: BN022434.D
 Acq: 01 Nov 2022 12:50




Instrument :
 BNA_N
 ClientSampleId :
 EW4X7


Tgt Ion: 88 Resp: 1216
 Ion Ratio Lower Upper
 88 100
 43 49.2 27.4 41.2#
 58 65.6 48.2 72.2

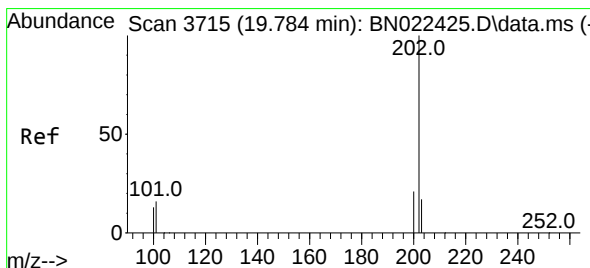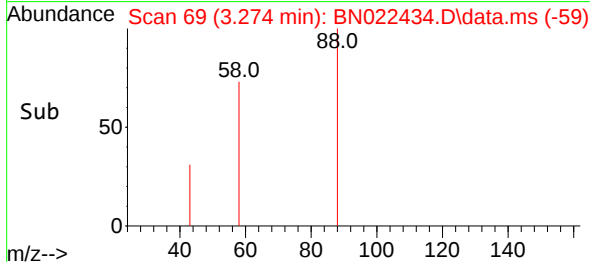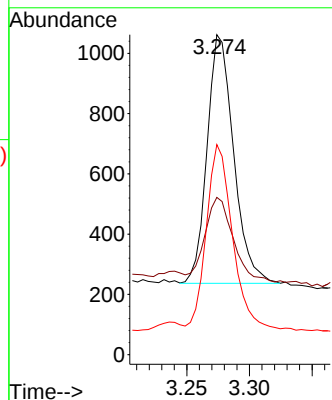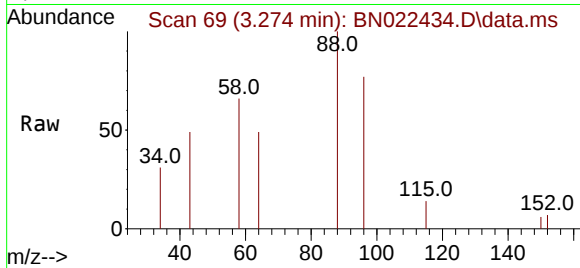

#20
 Pyrene
 Concen: 0.052 ng/ul
 RT: 19.756 min Scan# 3709
 Delta R.T. -0.028 min
 Lab File: BN022434.D
 Acq: 01 Nov 2022 12:50


Tgt Ion: 202 Resp: 2405
 Ion Ratio Lower Upper
 202 100
 101 175.2 13.1 19.7#
 100 1283.5 10.6 16.0#

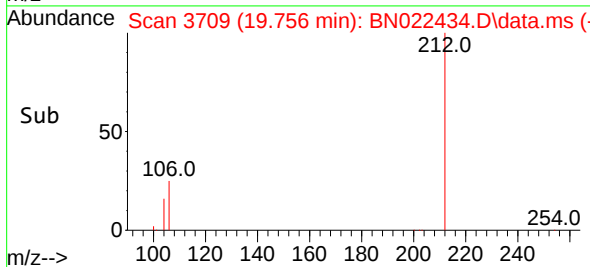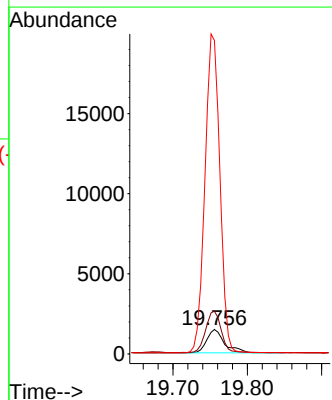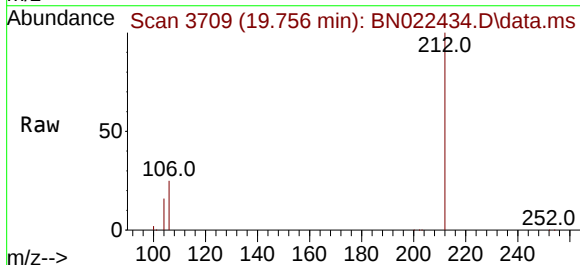

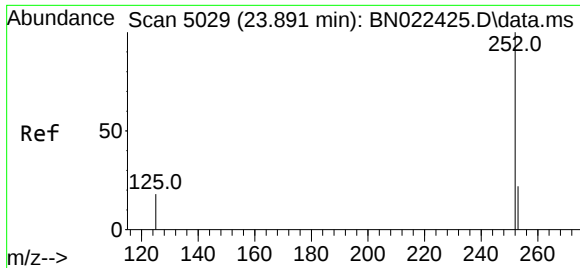

#26
Benzo(a)pyrene
Concen: 0.103 ng/ul
RT: 23.841 min Scan# 5012
Delta R.T. -0.050 min
Lab File: BN022434.D
Acq: 01 Nov 2022 12:50

Instrument :
BNA_N
ClientSampleId :
EW4X7

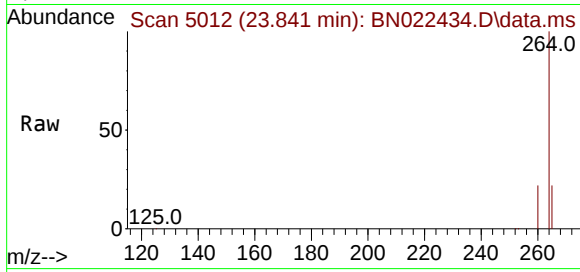

Tgt Ion:	252	Resp:	3146
Ion	Ratio	Lower	Upper
252	100		
253	48.8	21.0	31.6#
125	48.2	17.9	26.9#

