

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
 Data File : BN022435.D
 Acq On : 01 Nov 2022 13:28
 Operator : CG/JU
 Sample : N5276-18
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4X8

Quant Time: Nov 02 00:53:39 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 01 01:09:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	4890	0.400	ng/ul	0.00
4) Naphthalene-d8	10.672	136	3079	0.400	ng/ul	-0.08
9) Acenaphthene-d10	0.000	164	0	0.000	ng/ul	-14.60
13) Phenanthrene-d10	17.352	188	17580	0.400	ng/ul	0.00
17) Chrysene-d12	21.556	240	9112	0.400	ng/ul	0.00
23) Perylene-d12	24.003	264	7302	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.236	96	24781	3.899	ng/ul	0.00
6) 2-Methylnaphthalene-d10	0.000	152	0	0.000	ng/ul	
18) Fluoranthene-d10	19.388	212	13685	0.447	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.278	88	1636	0.251	ng/ul#	31
20) Pyrene	19.755	202	1674	0.040	ng/ul#	1
26) Benzo(a)pyrene	23.842	252	2473	0.085	ng/ul#	35


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
Data File : BN022435.D
Acq On : 01 Nov 2022 13:28
Operator : CG/JU
Sample : N5276-18
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4X8

Quant Time: Nov 02 00:53:39 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 01 01:09:32 2022
Response via : Initial Calibration




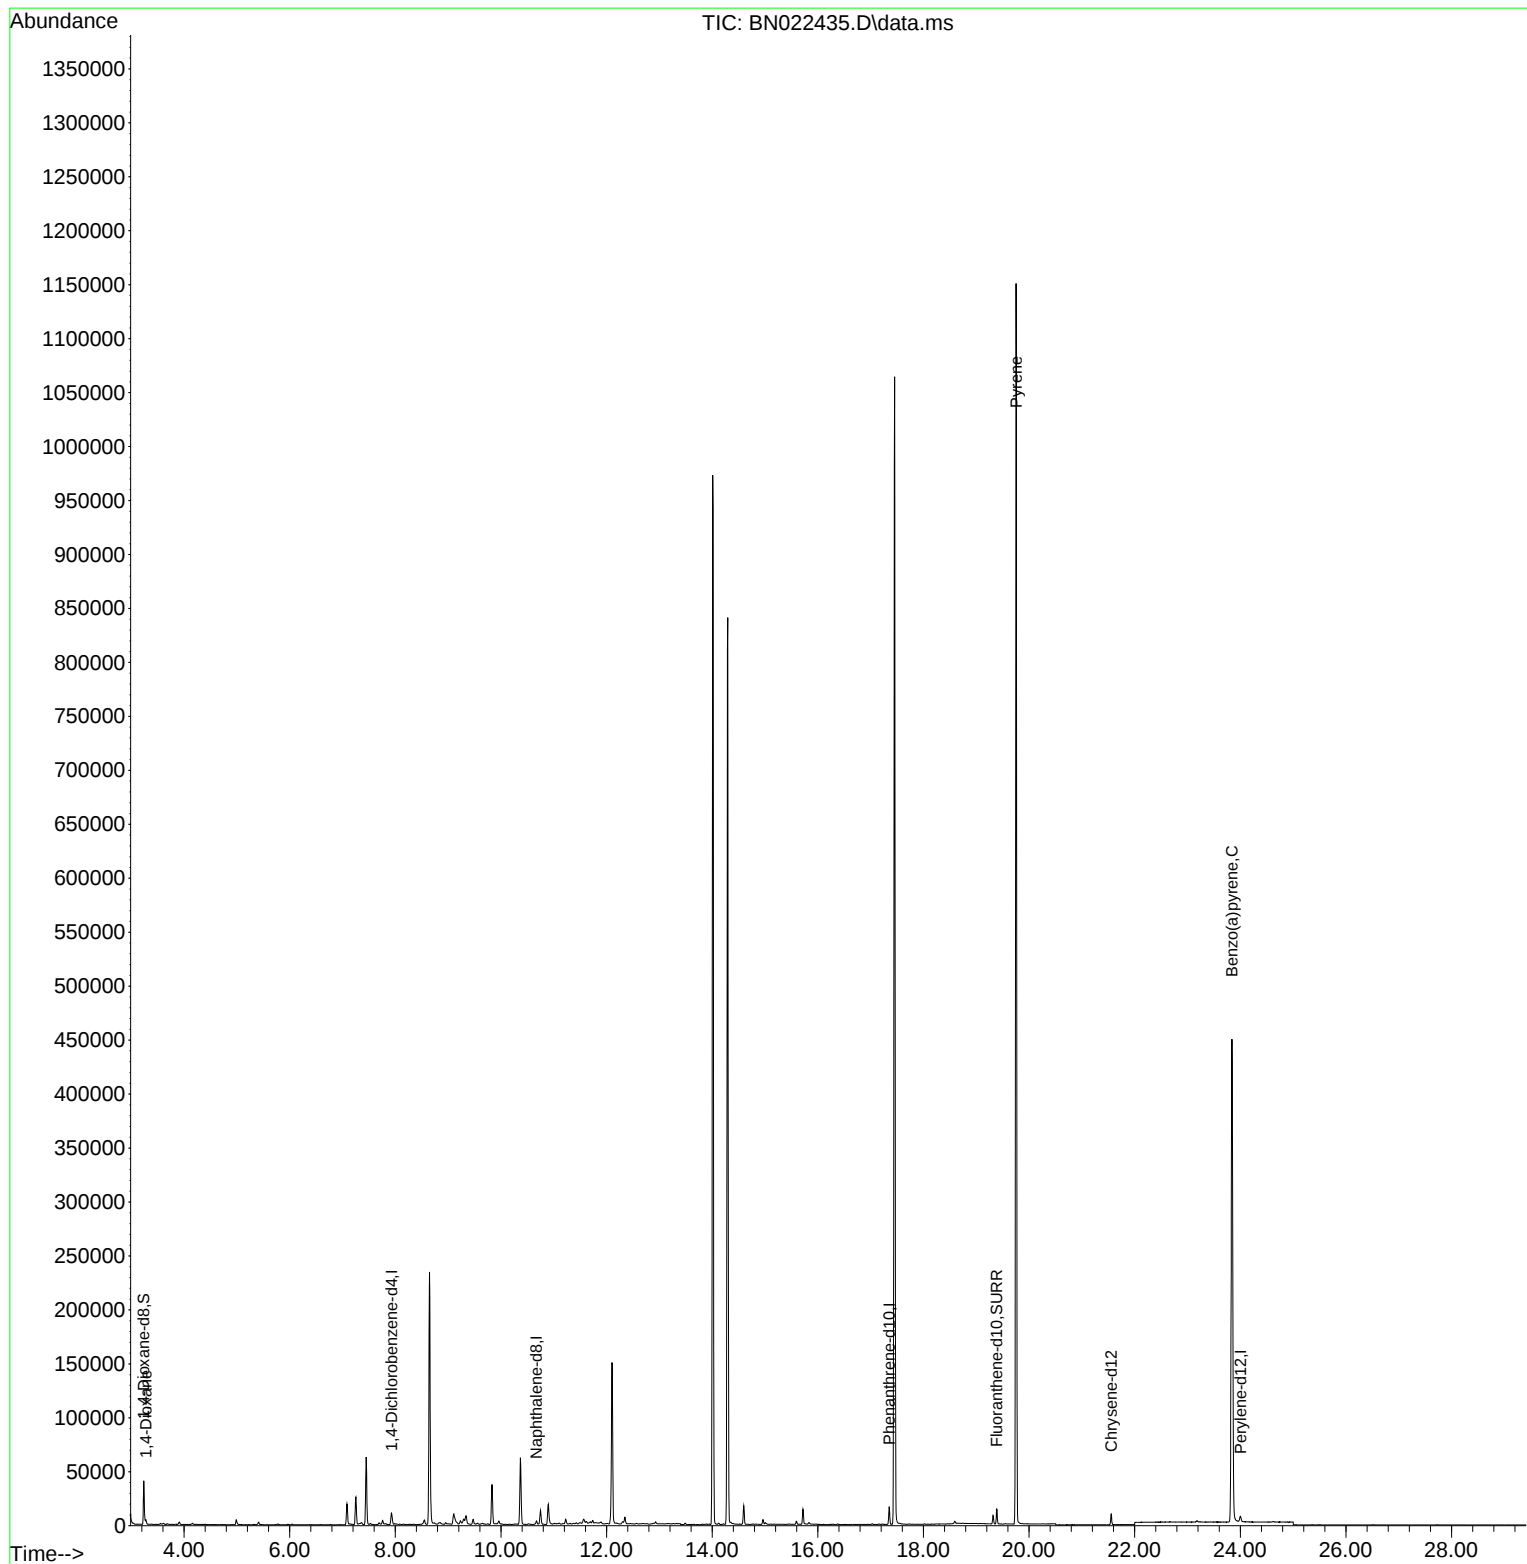


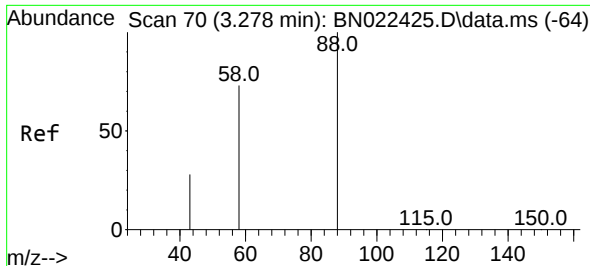

#2
1,4-Dioxane
Concen: 0.251 ng/ul
RT: 3.278 min Scan# 70
Delta R.T. -0.004 min
Lab File: BN022435.D
Acq: 01 Nov 2022 13:28




Instrument :
BNA_N
ClientSampleId :
EW4X8


Tgt Ion: 88 Resp: 1636
Ion Ratio Lower Upper
88 100
43 123.4 27.4 41.2#
58 74.8 48.2 72.2#

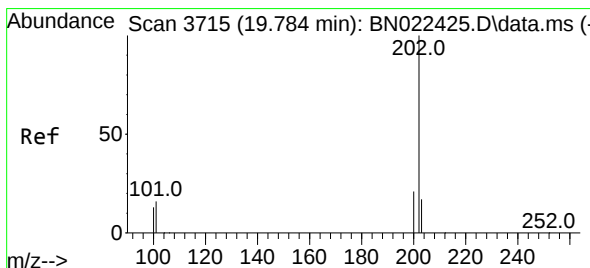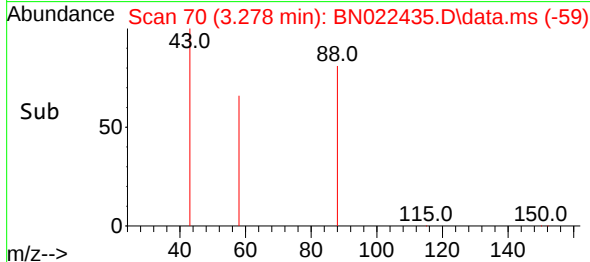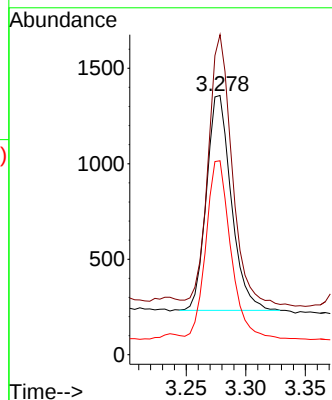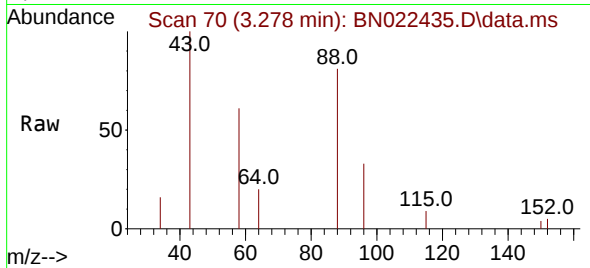

#20
Pyrene
Concen: 0.040 ng/ul
RT: 19.755 min Scan# 3709
Delta R.T. -0.029 min
Lab File: BN022435.D
Acq: 01 Nov 2022 13:28


Tgt Ion: 202 Resp: 1674
Ion Ratio Lower Upper
202 100
101 178.8 13.1 19.7#
100 1262.0 10.6 16.0#

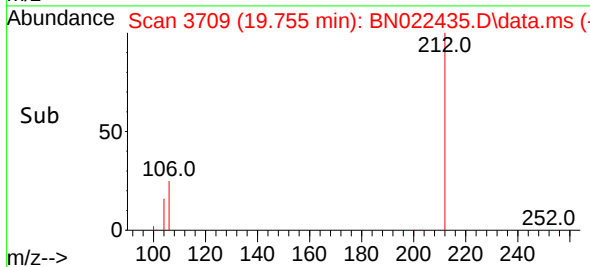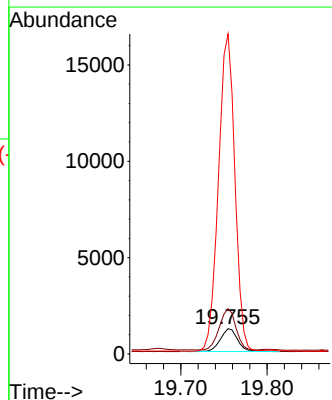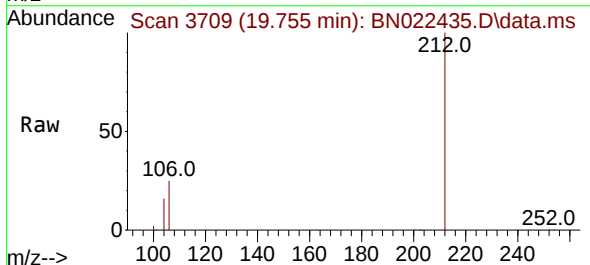

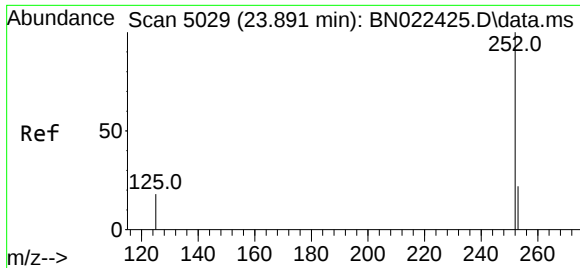

#26
Benzo(a)pyrene
Concen: 0.085 ng/ul
RT: 23.842 min Scan# 5012
Delta R.T. -0.049 min
Lab File: BN022435.D
Acq: 01 Nov 2022 13:28

Instrument :
BNA_N
ClientSampleId :
EW4X8

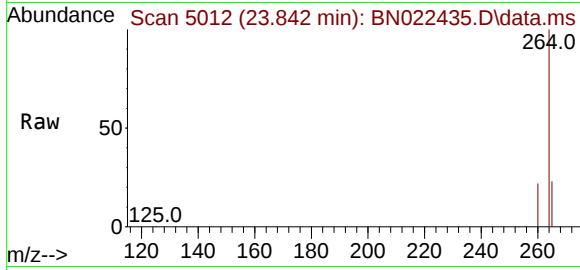

Tgt Ion:252 Resp: 2473
Ion Ratio Lower Upper
252 100
253 57.0 21.0 31.6#
125 56.8 17.9 26.9#

