

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
 Data File : BN022439.D
 Acq On : 01 Nov 2022 16:00
 Operator : CG/JU
 Sample : N5277-16
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4X7

Quant Time: Nov 02 00:54:29 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 01 01:09:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.927	152	4182	0.400	ng/ul	0.00
4) Naphthalene-d8	10.750	136	16394	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.600	164	9423	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.353	188	19078	0.400	ng/ul	0.00
17) Chrysene-d12	21.558	240	11722	0.400	ng/ul	0.00
23) Perylene-d12	24.002	264	8763	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.236	96	25541	4.699	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.350	152	8911	0.359	ng/ul	0.00
18) Fluoranthene-d10	19.389	212	17412	0.442	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.274	88	1147	0.206	ng/ul#	83
20) Pyrene	19.756	202	2540	0.047	ng/ul#	1
26) Benzo(a)pyrene	23.844	252	3492	0.100	ng/ul#	56


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
Data File : BN022439.D
Acq On : 01 Nov 2022 16:00
Operator : CG/JU
Sample : N5277-16
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4X7

Quant Time: Nov 02 00:54:29 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 01 01:09:32 2022
Response via : Initial Calibration




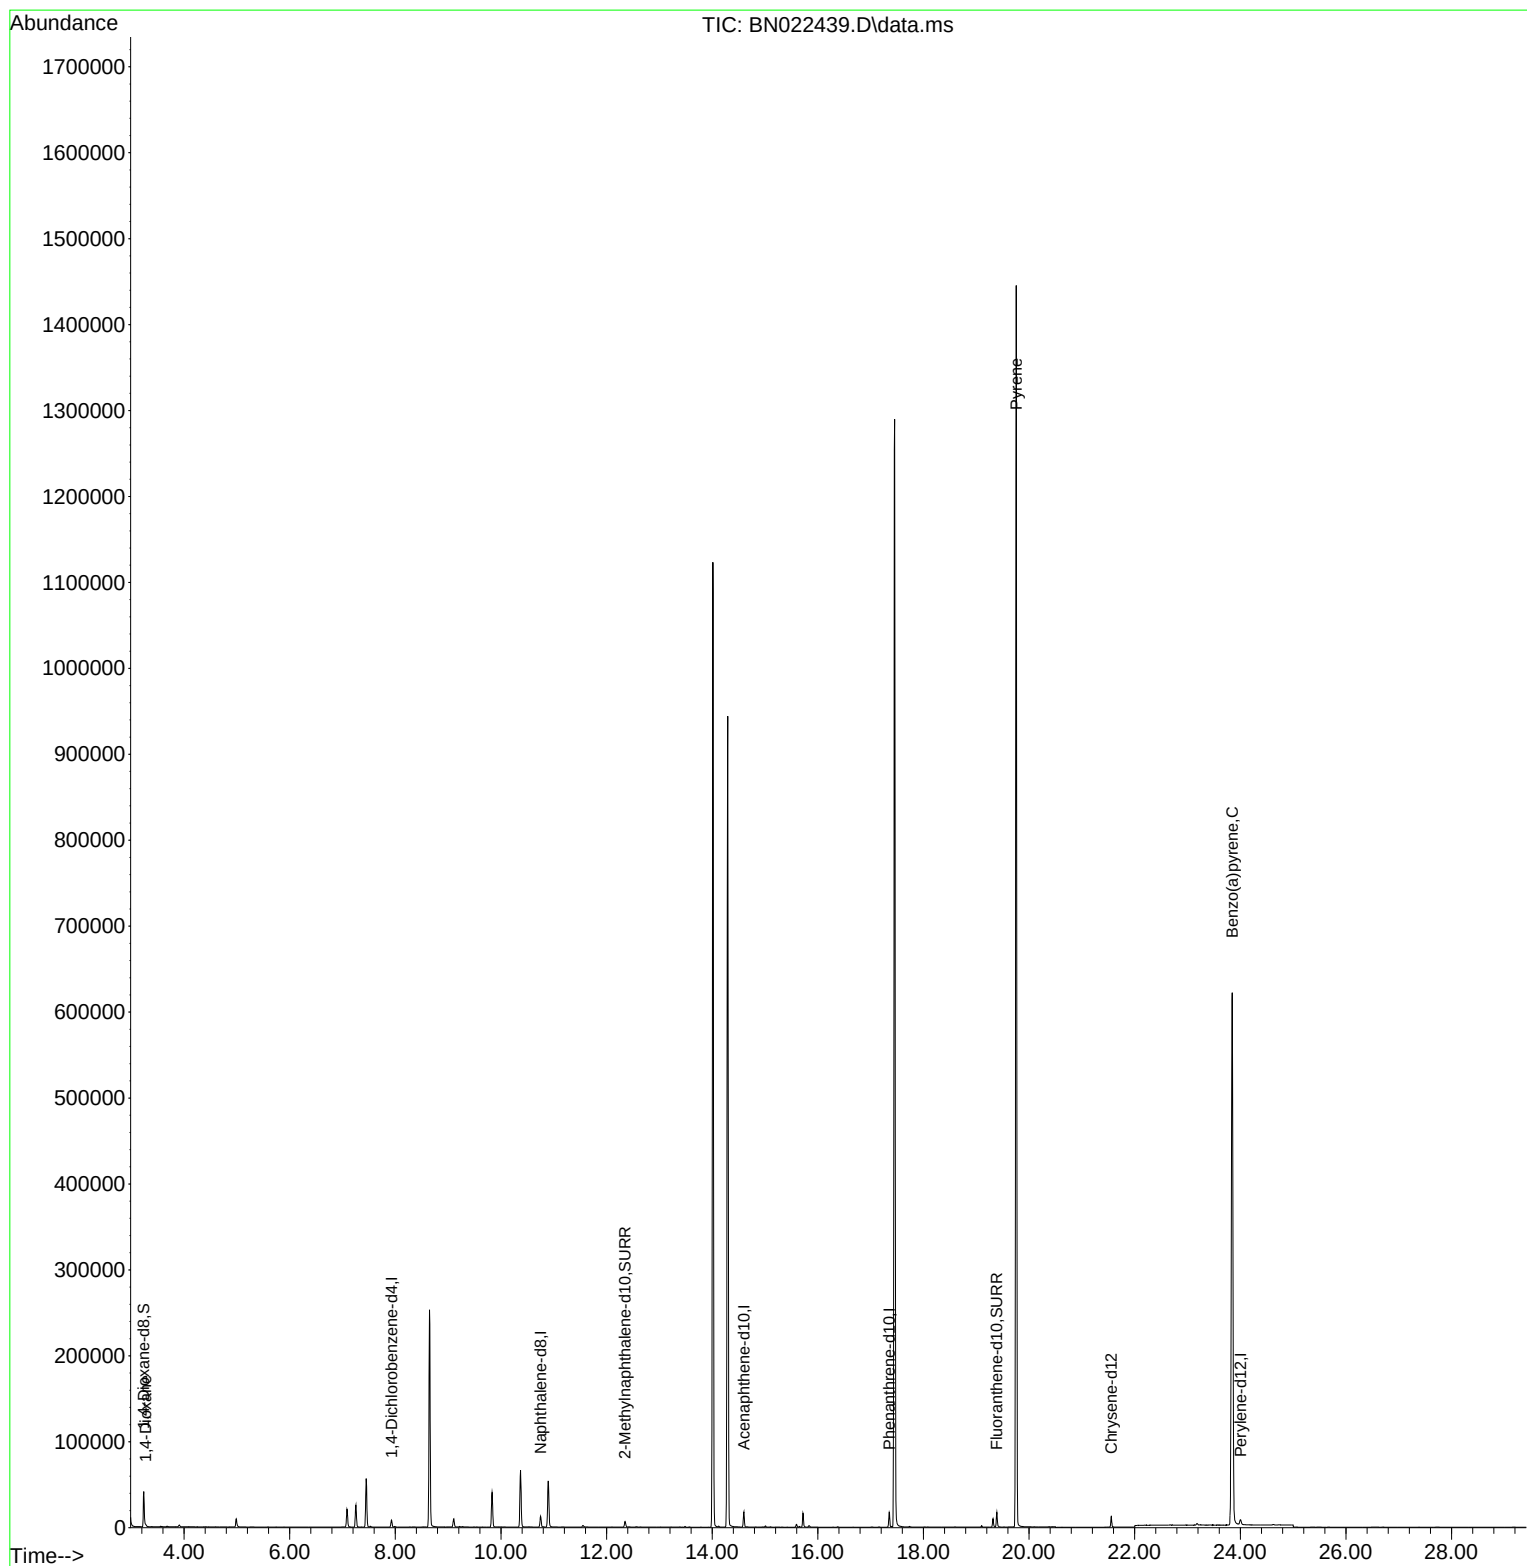


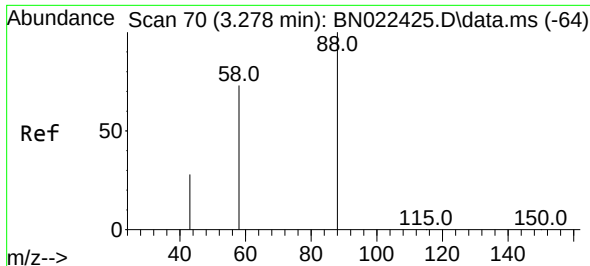

#2
 1,4-Dioxane
 Concen: 0.206 ng/ul
 RT: 3.274 min Scan# 61
 Delta R.T. -0.009 min
 Lab File: BN022439.D
 Acq: 01 Nov 2022 16:00




Instrument :
 BNA_N
 ClientSampleId :
 EW4X7


Tgt Ion: 88 Resp: 1147
 Ion Ratio Lower Upper
 88 100
 43 51.8 27.4 41.2#
 58 67.1 48.2 72.2

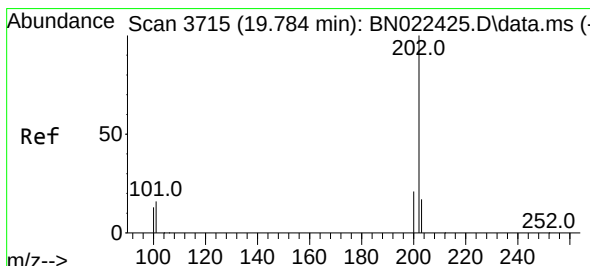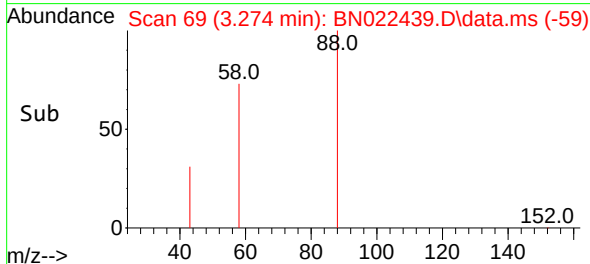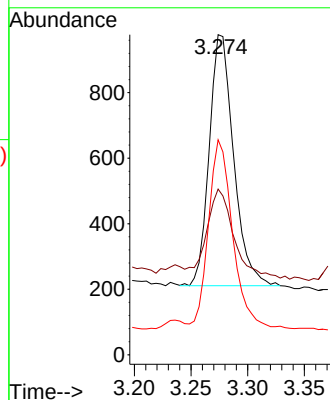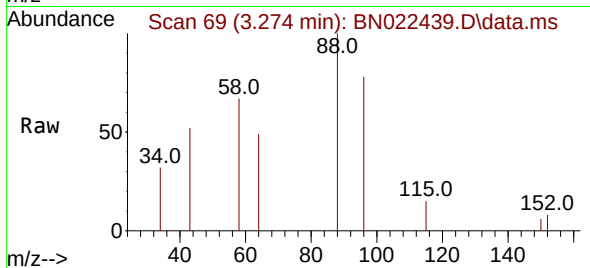

#20
 Pyrene
 Concen: 0.047 ng/ul
 RT: 19.756 min Scan# 3709
 Delta R.T. -0.028 min
 Lab File: BN022439.D
 Acq: 01 Nov 2022 16:00


Tgt Ion: 202 Resp: 2540
 Ion Ratio Lower Upper
 202 100
 101 183.4 13.1 19.7#
 100 1368.9 10.6 16.0#

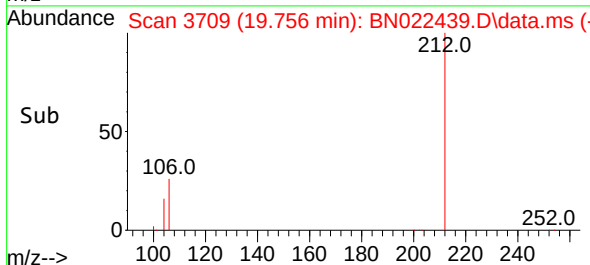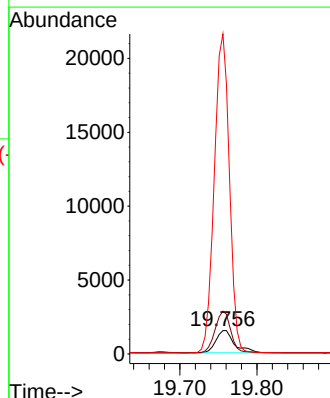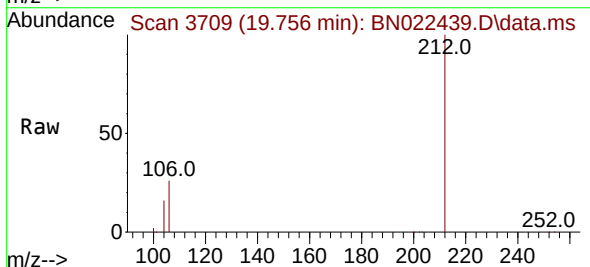

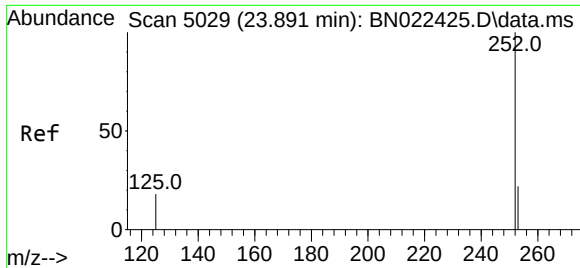

#26
Benzo(a)pyrene
Concen: 0.100 ng/ul
RT: 23.844 min Scan# 5013
Delta R.T. -0.047 min
Lab File: BN022439.D
Acq: 01 Nov 2022 16:00

Instrument :
BNA_N
ClientSampleId :
EW4X7

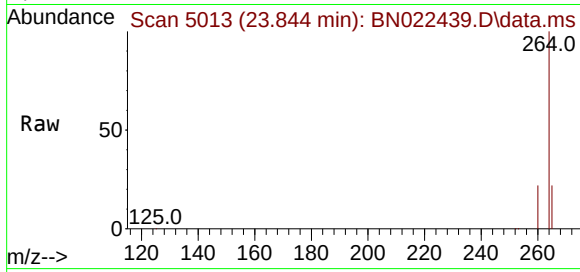

Tgt Ion:252 Resp: 3492
Ion Ratio Lower Upper
252 100
253 45.9 21.0 31.6#
125 47.3 17.9 26.9#

