




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
 Data File : BN022440.D
 Acq On : 01 Nov 2022 16:38
 Operator : CG/JU
 Sample : N5277-17
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4X8

Manual IntegrationsAPPROVED

Quant Time: Nov 02 00:54:41 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 01 01:09:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/02/2022
 Supervised By :mohammad ahmed 11/04/2022

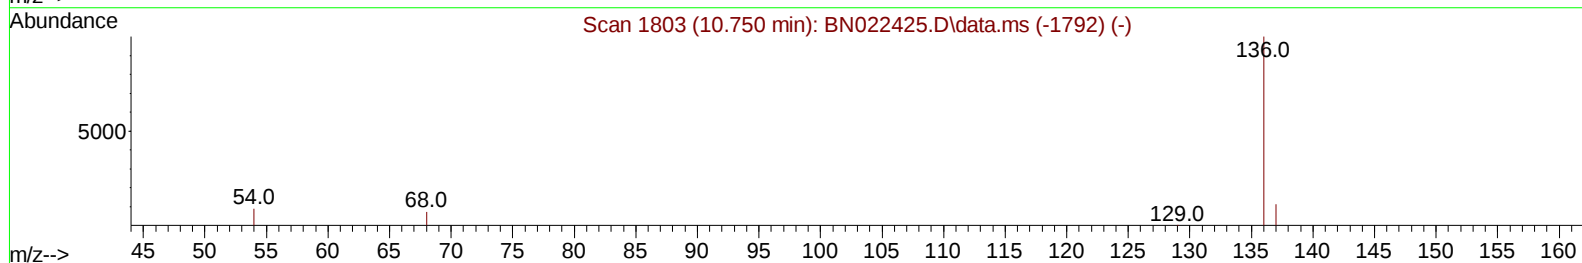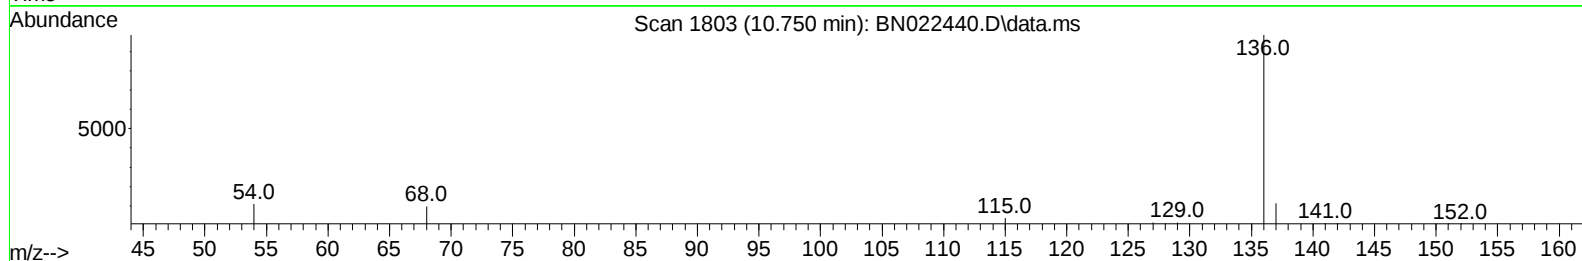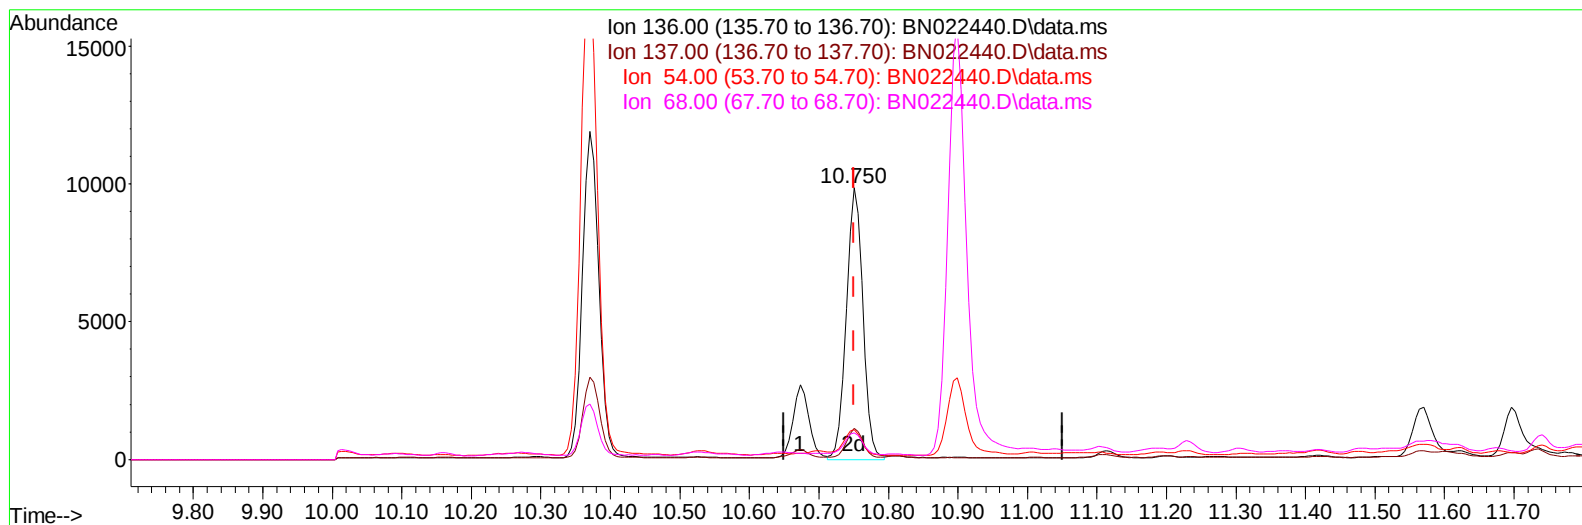

TIC: BN022440.D\data.ms

(4) Naphthalene-d8 (I)

10.750min (-0.000) 0.40 ng/ul m

response 16571

Ion	Exp%	Act%
136.00	100.00	100.00
137.00	11.50	11.38
54.00	9.30	10.93
68.00	7.70	9.90#




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
 Data File : BN022440.D
 Acq On : 01 Nov 2022 16:38
 Operator : CG/JU
 Sample : N5277-17
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4X8

Manual IntegrationsAPPROVED

Quant Time: Nov 02 00:54:41 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 01 01:09:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/02/2022
 Supervised By :mohammad ahmed 11/04/2022

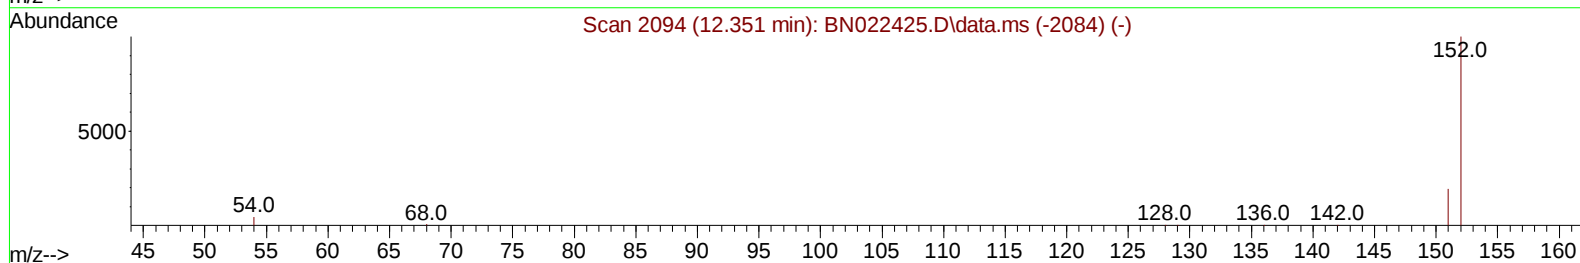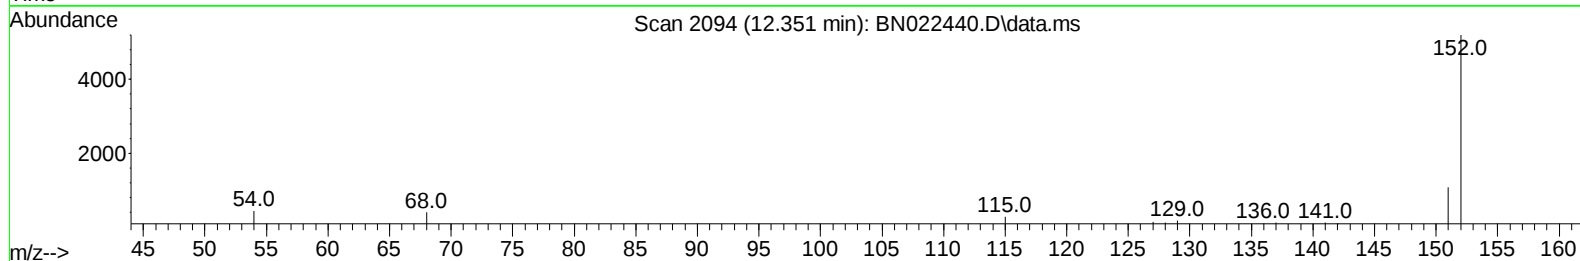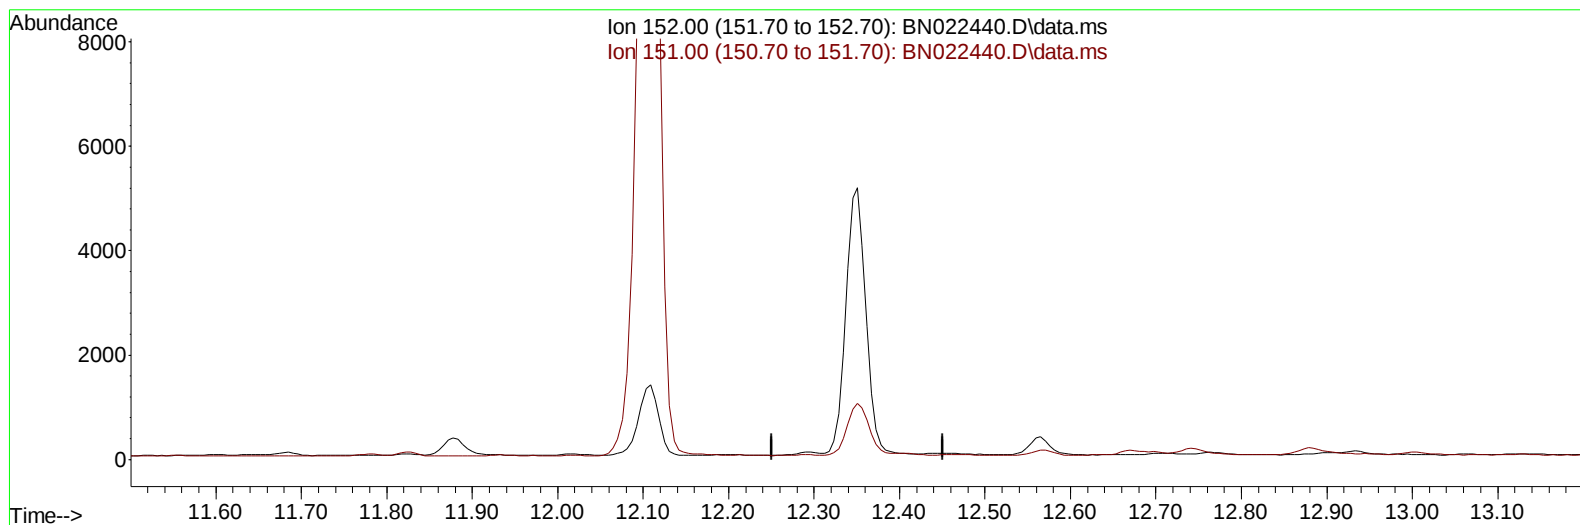

TIC: BN022440.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.351min (-12.351) 0.00 ng/u1

response 0

Ion	Exp%	Act%
152.00	100.00	0.00
151.00	20.80	0.00#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
 Data File : BN022440.D
 Acq On : 01 Nov 2022 16:38
 Operator : CG/JU
 Sample : N5277-17
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4X8

Manual IntegrationsAPPROVED

Quant Time: Nov 02 00:54:41 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 01 01:09:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/02/2022
 Supervised By :mohammad ahmed 11/04/2022

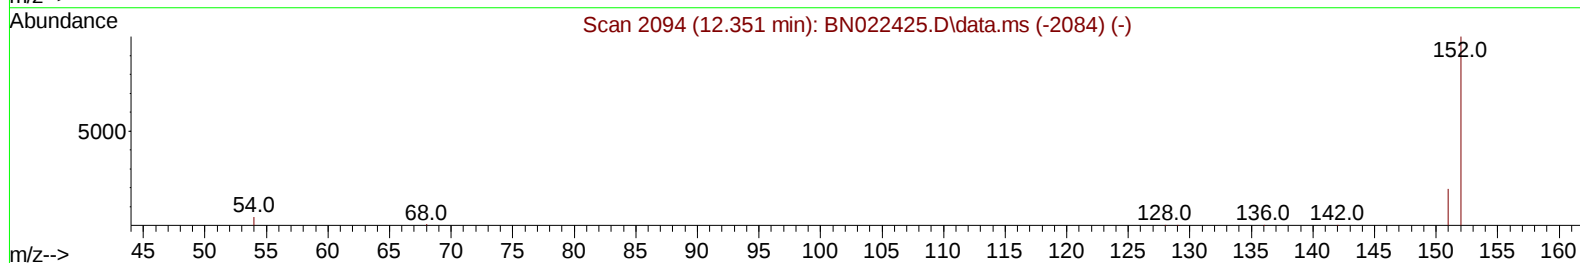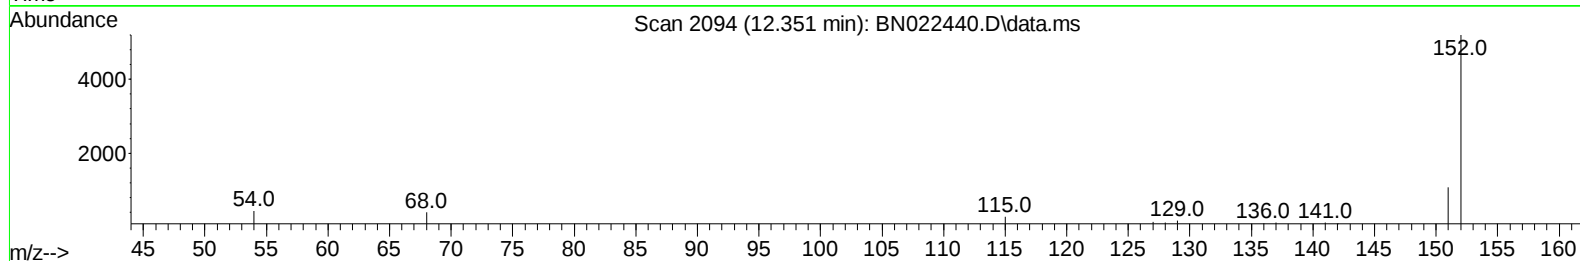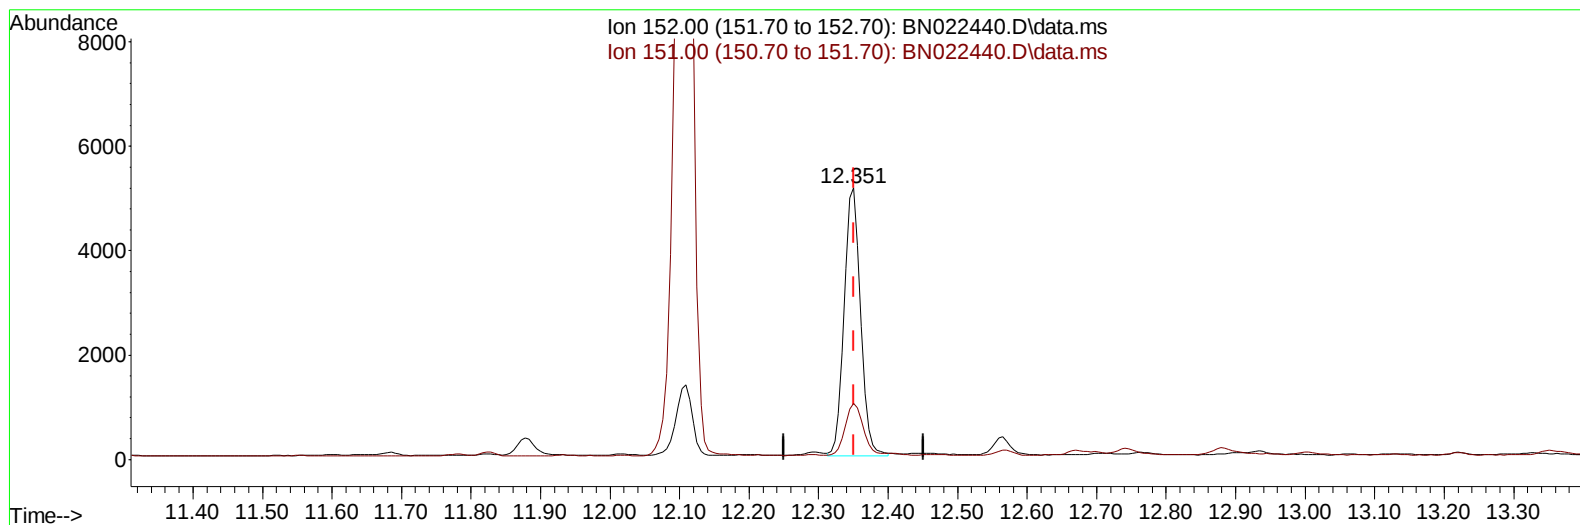

TIC: BN022440.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.351min (-0.000) 0.34 ng/ul m

response 8412

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.80	0.00#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
 Data File : BN022440.D
 Acq On : 01 Nov 2022 16:38
 Operator : CG/JU
 Sample : N5277-17
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4X8

Manual IntegrationsAPPROVED

Quant Time: Nov 02 00:54:41 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 01 01:09:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/02/2022
 Supervised By :mohammad ahmed 11/04/2022

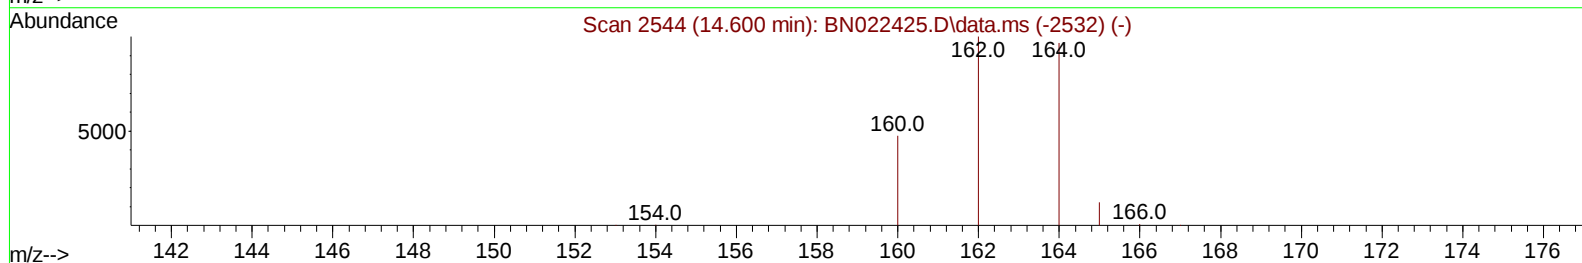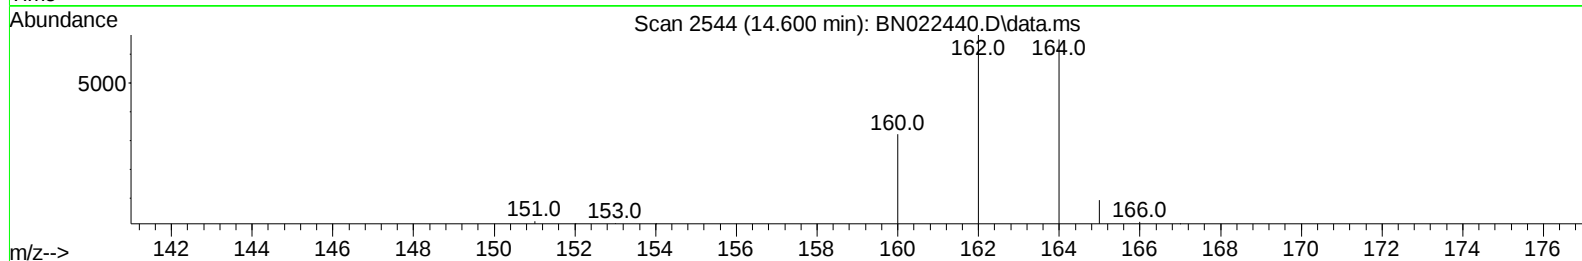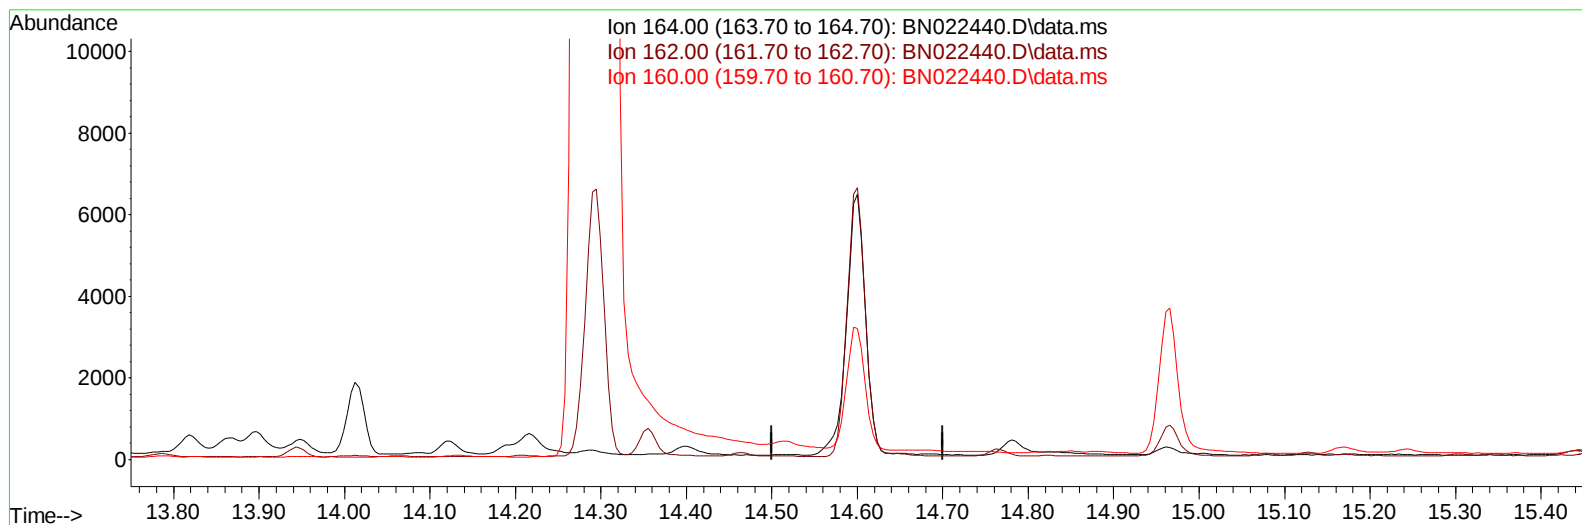

TIC: BN022440.D\data.ms

(9) Acenaphthene-d10 (I)

14.600min (-14.600) 0.00 ng/u1

response 0

Ion	Exp%	Act%
164.00	100.00	0.00
162.00	104.50	0.00#
160.00	50.40	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
Data File : BN022440.D
Acq On : 01 Nov 2022 16:38
Operator : CG/JU
Sample : N5277-17
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4X8

Manual IntegrationsAPPROVED

Quant Time: Nov 02 00:54:41 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 01 01:09:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/02/2022
Supervised By :mohammad ahmed 11/04/2022

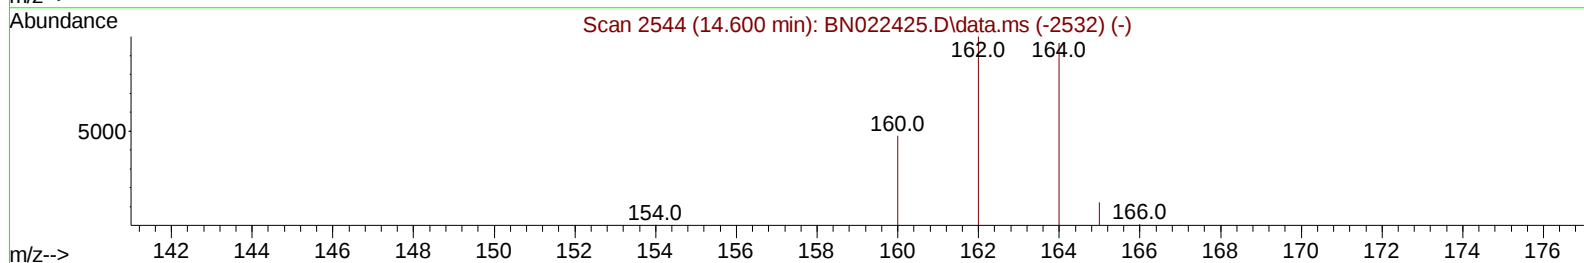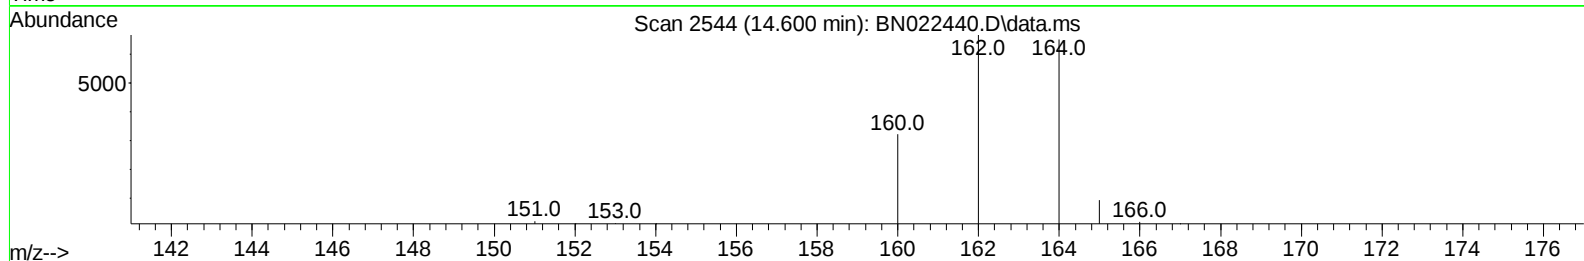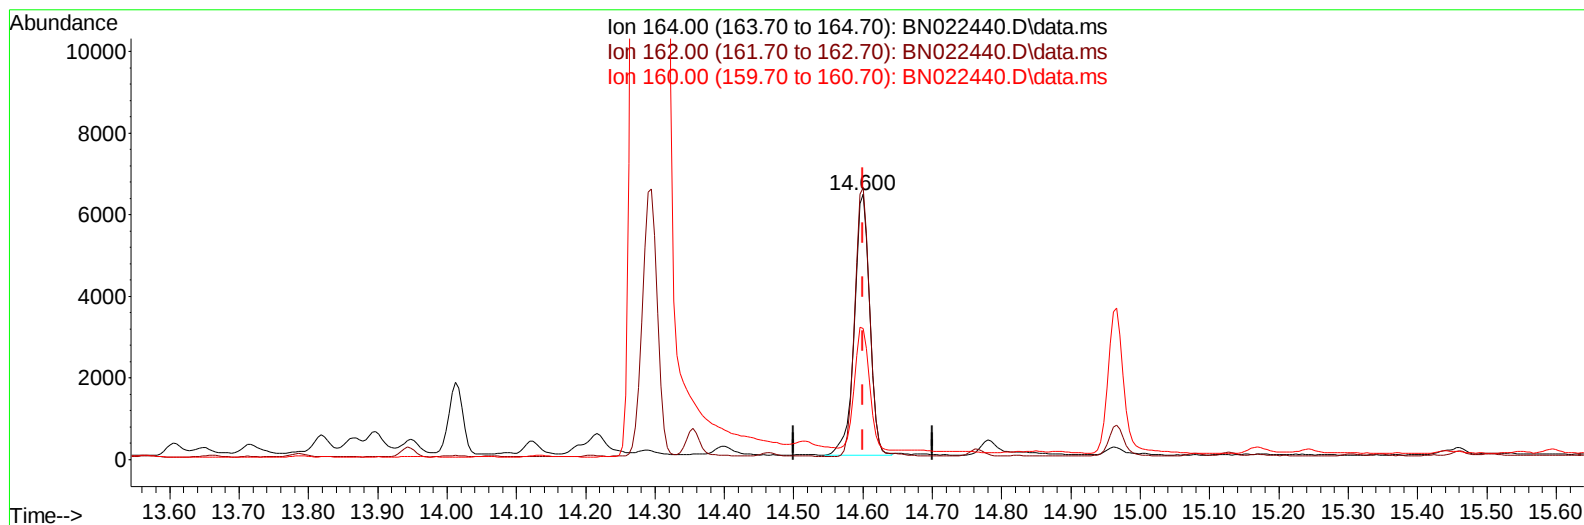

TIC: BN022440.D\data.ms

(9) Acenaphthene-d10 (I)

14.600min (-0.000) 0.40 ng/ul m

response 9899

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	104.50	102.35
160.00	50.40	49.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
 Data File : BN022440.D
 Acq On : 01 Nov 2022 16:38
 Operator : CG/JU
 Sample : N5277-17
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4X8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/02/2022
 Supervised By :mohammad ahmed 11/04/2022

Quant Time: Nov 02 00:54:41 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 01 01:09:32 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.928	152		4707	0.400	ng/ul	0.00
4) Naphthalene-d8	10.750	136		16571m	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.600	164		9899m	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.353	188		18007	0.400	ng/ul	0.00
17) Chrysene-d12	21.556	240		9054	0.400	ng/ul	0.00
23) Perylene-d12	23.999	264		7262	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.236	96		23385	3.823	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.351	152		8412m	0.336	ng/ul	0.00
18) Fluoranthene-d10	19.393	212		13870	0.456	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.278	88		1496	0.238	ng/ul#	25

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
Data File : BN022440.D
Acq On : 01 Nov 2022 16:38
Operator : CG/JU
Sample : N5277-17
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4X8

Manual IntegrationsAPPROVED

Quant Time: Nov 02 00:54:41 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 01 01:09:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/02/2022
Supervised By :mohammad ahmed 11/04/2022

