

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
 Data File : BN022407.D
 Acq On : 31 Oct 2022 18:44
 Operator : CG/JU
 Sample : N5277-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4W6

Quant Time: Nov 01 01:12:07 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 01 01:09:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	3993	0.400	ng/ul	0.00
4) Naphthalene-d8	10.750	136	13229	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.600	164	7273	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.357	188	14335	0.400	ng/ul	0.00
17) Chrysene-d12	21.559	240	7872	0.400	ng/ul	0.00
23) Perylene-d12	24.005	264	6205	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.236	96	21841	4.209	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.356	152	6373	0.318	ng/ul	0.00
18) Fluoranthene-d10	19.393	212	12639	0.478	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.278	88	1135	0.213	ng/ul#	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
Data File : BN022407.D
Acq On : 31 Oct 2022 18:44
Operator : CG/JU
Sample : N5277-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4W6

Quant Time: Nov 01 01:12:07 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 01 01:09:32 2022
Response via : Initial Calibration

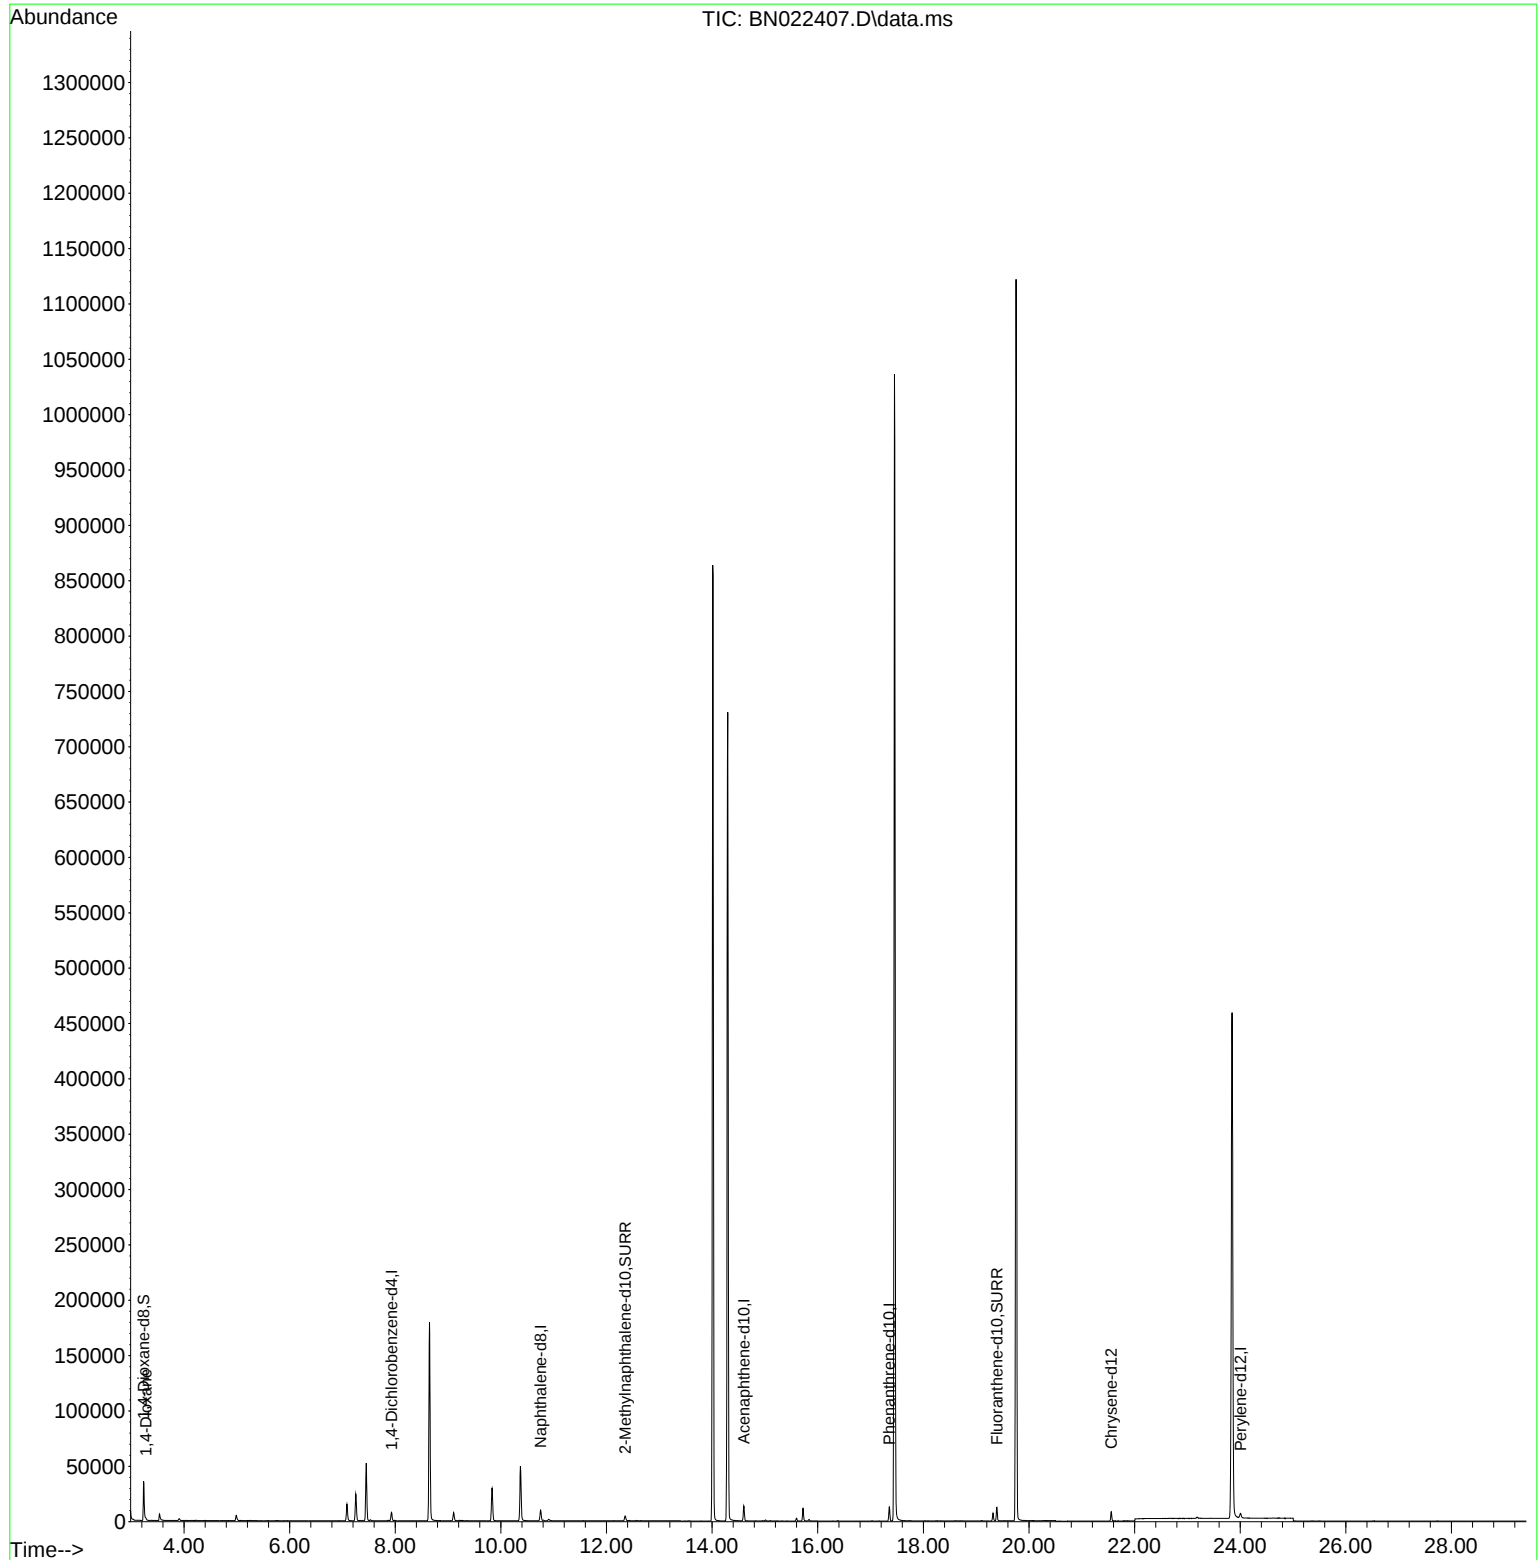

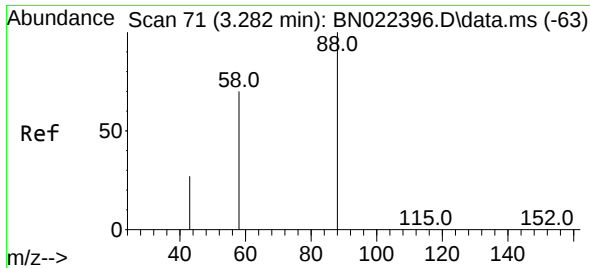

#2
 1,4-Dioxane
 Concen: 0.213 ng/ul
 RT: 3.278 min Scan# 70
 Delta R.T. -0.004 min
 Lab File: BN022407.D
 Acq: 31 Oct 2022 18:44

Instrument :
 BNA_N
 ClientSampleId :
 EW4W6

Tgt Ion: 88 Resp: 1135
 Ion Ratio Lower Upper
 88 100
 43 48.0 27.4 41.2#
 58 63.1 48.2 72.2

