

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
 Data File : BN022412.D
 Acq On : 31 Oct 2022 22:31
 Operator : CG/JU
 Sample : N5144-03DL 5X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BK9DL

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 11/01/2022
 Supervised By :mohammad ahmed 11/01/2022

Quant Time: Nov 01 01:12:42 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 01 01:09:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	4734	0.400	ng/ul	0.00
4) Naphthalene-d8	10.756	136	15509	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.600	164	8492	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.353	188	16244	0.400	ng/ul	0.00
17) Chrysene-d12	21.553	240	9395	0.400	ng/ul	0.00
23) Perylene-d12	24.002	264	6839	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.240	96	4837	0.786	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.351	152	1057	0.045	ng/ul	0.00
18) Fluoranthene-d10	19.389	212	1762	0.056	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.805	128	7323	0.160	ng/ul	98
7) 2-Methylnaphthalene	12.428	142	5549	0.192	ng/ul	99
8) 1-Methylnaphthalene	12.642	142	4414	0.149	ng/ul	100
10) Acenaphthylene	14.323	152	1388	0.036	ng/ul#	80
12) Fluorene	15.650	166	939	0.025	ng/ul#	93
15) Phenanthrene	17.395	178	18853	0.346	ng/ul	100
16) Anthracene	17.488	178	3062	0.067	ng/ul#	93
19) Fluoranthene	19.421	202	28407	0.660	ng/ul	97
20) Pyrene	19.784	202	23262m	0.538	ng/ul	
21) Benzo(a)anthracene	21.538	228	10186	0.289	ng/ul	96
22) Chrysene	21.591	228	10749	0.288	ng/ul	97
24) Benzo(b)fluoranthene	23.251	252	12190m	0.355	ng/ul	
25) Benzo(k)fluoranthene	23.295	252	3803m	0.114	ng/ul	
26) Benzo(a)pyrene	23.888	252	7039	0.257	ng/ul#	78
27) Indeno(1,2,3-cd)pyrene	26.565	276	4875	0.143	ng/ul#	96
28) Dibenzo(a,h)anthracene	26.578	278	1305	0.048	ng/ul#	47
29) Benzo(g,h,i)perylene	27.356	276	3806	0.137	ng/ul	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
Data File : BN022412.D
Acq On : 31 Oct 2022 22:31
Operator : CG/JU
Sample : N5144-03DL 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0BK9DL

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 11/01/2022
Supervised By :mohammad ahmed 11/01/2022


Quant Time: Nov 01 01:12:42 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 01 01:09:32 2022
Response via : Initial Calibration

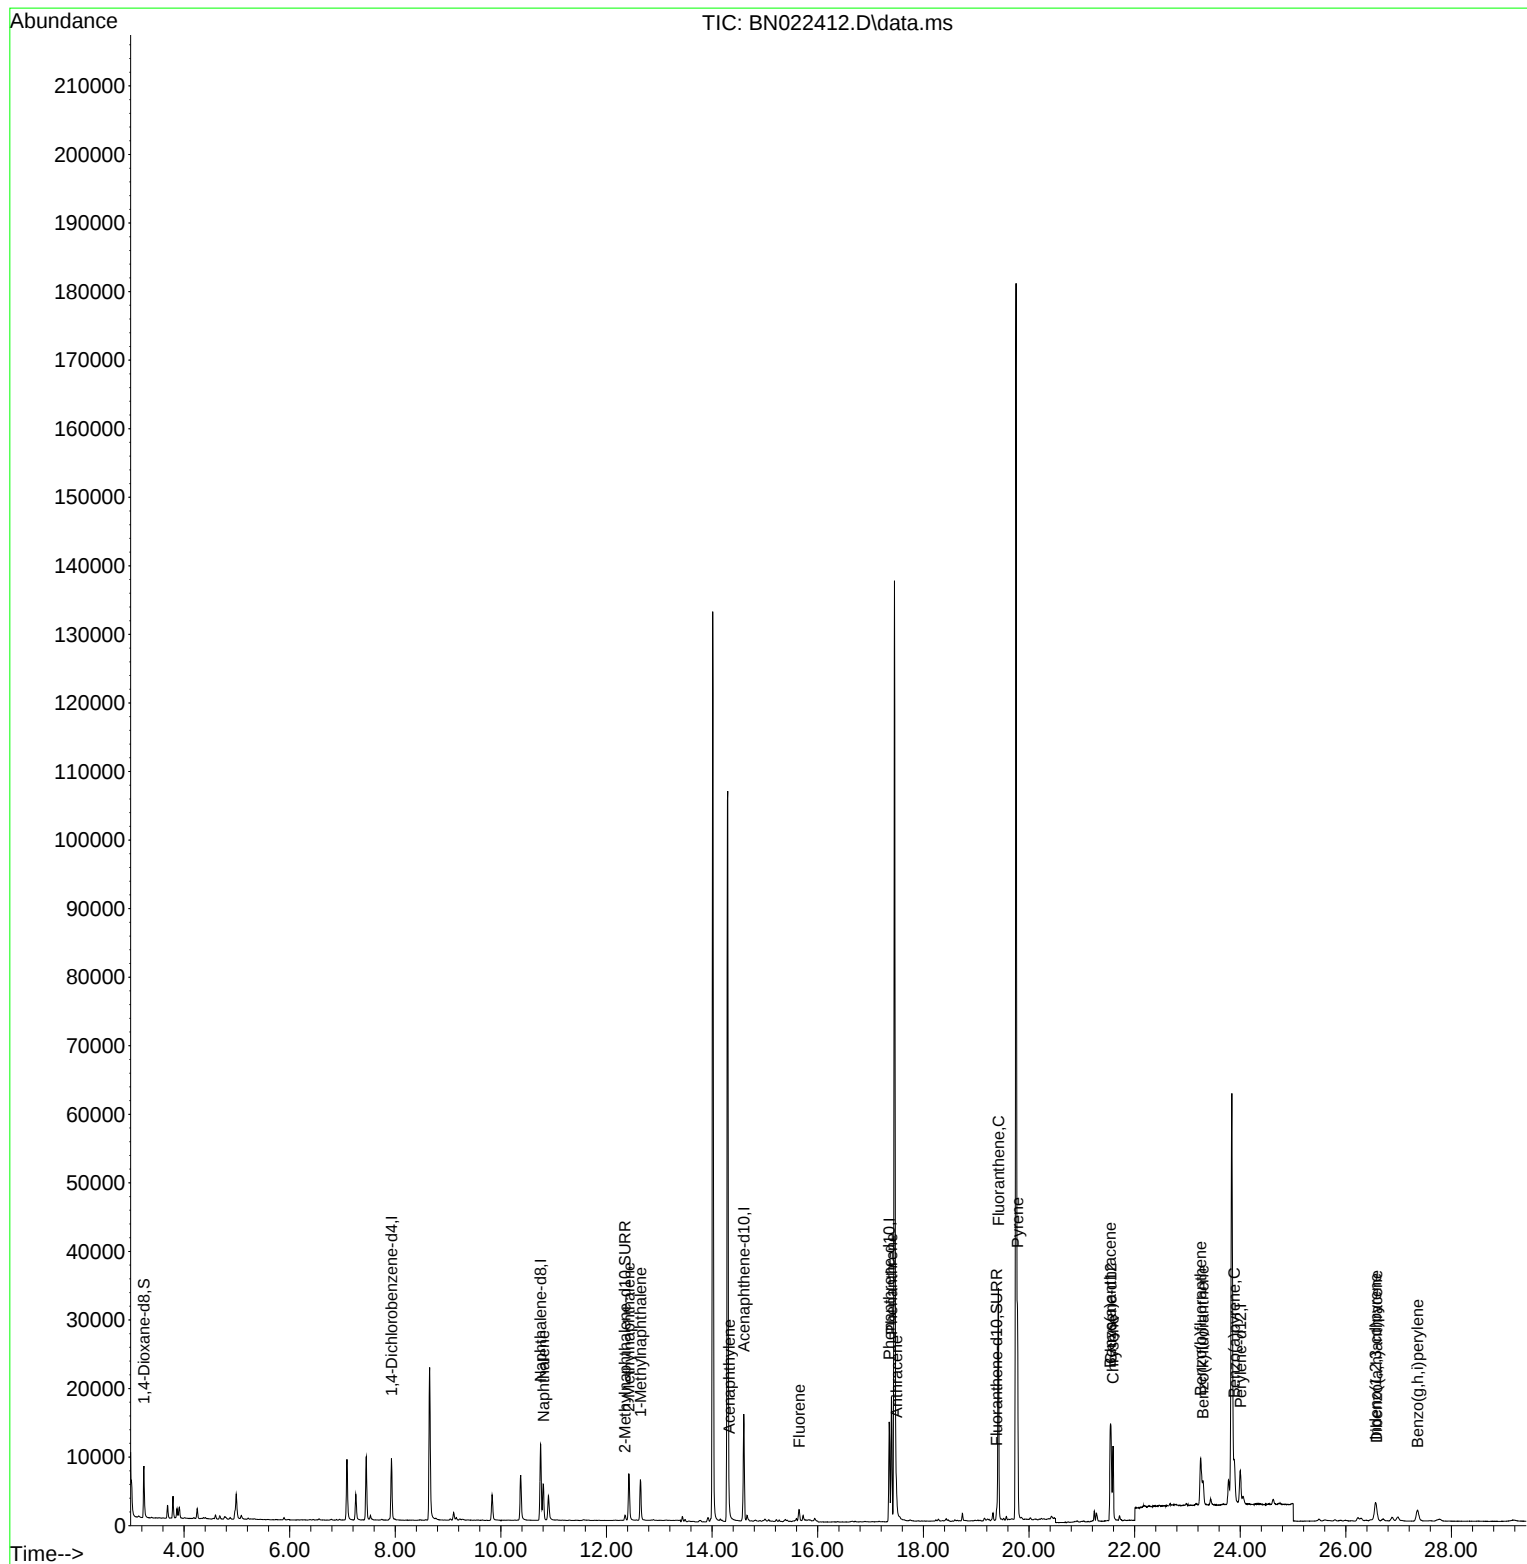

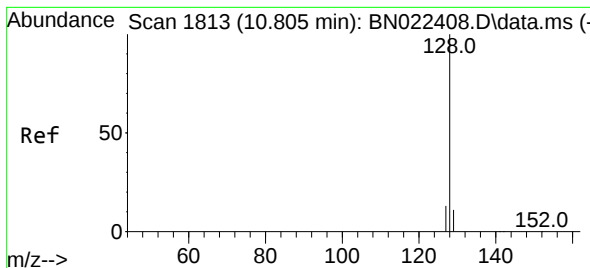

#5
Naphthalene
Concen: 0.160 ng/ul
RT: 10.805 min Scan# 1813
Delta R.T. 0.006 min
Lab File: BN022412.D
Acq: 31 Oct 2022 22:31




Instrument :
BNA_N
ClientSampleId :
C0BK9DL

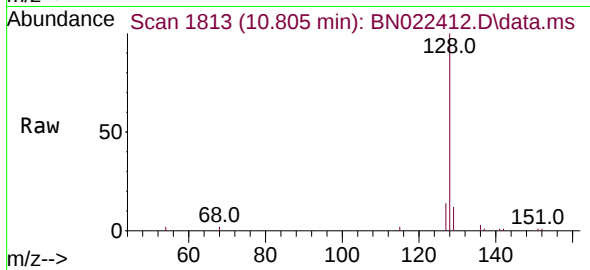


Tgt Ion:128 Resp: 7323
Ion Ratio Lower Upper
128 100
129 12.4 9.3 13.9
127 14.0 10.7 16.1

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 11/01/2022
Supervised By :mohammad ahmed 11/01/2022

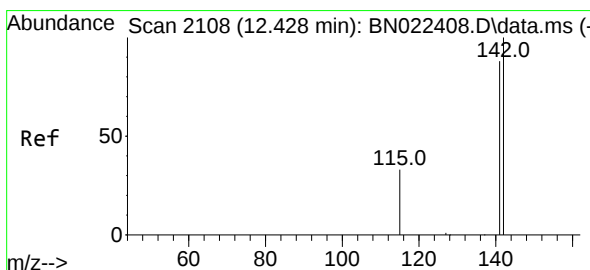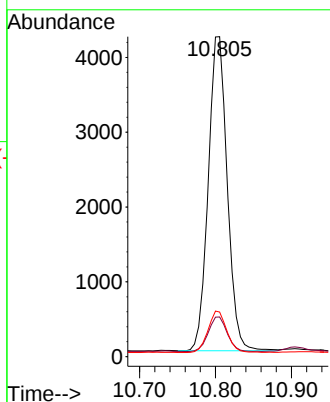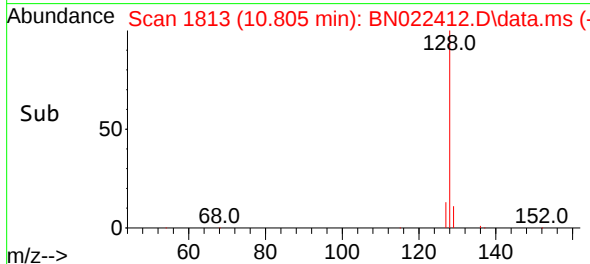


#7
2-Methylnaphthalene
Concen: 0.192 ng/ul
RT: 12.428 min Scan# 2108
Delta R.T. 0.006 min
Lab File: BN022412.D
Acq: 31 Oct 2022 22:31

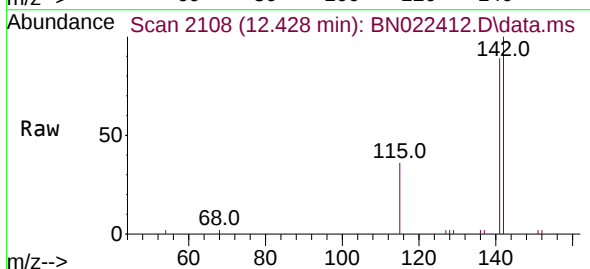


Tgt Ion:142 Resp: 5549
Ion Ratio Lower Upper
142 100
141 88.4 71.1 106.7

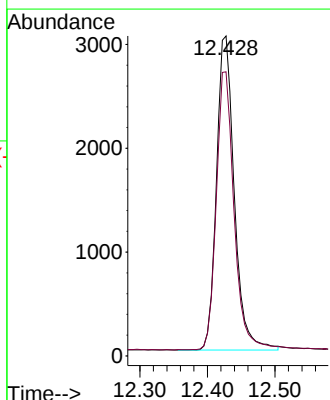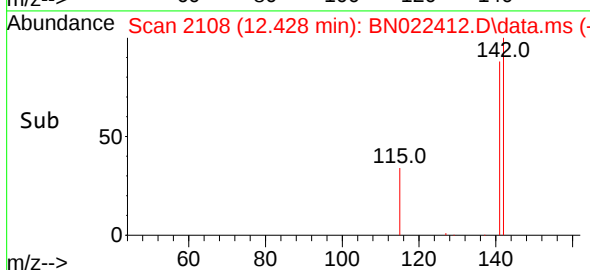



#8
1-Methylnaphthalene
Concen: 0.149 ng/ul
RT: 12.642 min Scan# 2148
Delta R.T. 0.000 min
Lab File: BN022412.D
Acq: 31 Oct 2022 22:31




Instrument :
BNA_N
ClientSampleId :
C0BK9DL

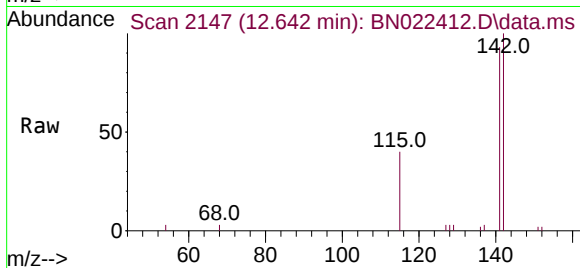

Tgt Ion:142 Resp: 4414
Ion Ratio Lower Upper
142 100
141 91.5 73.3 109.9




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 11/01/2022
Supervised By :mohammad ahmed 11/01/2022

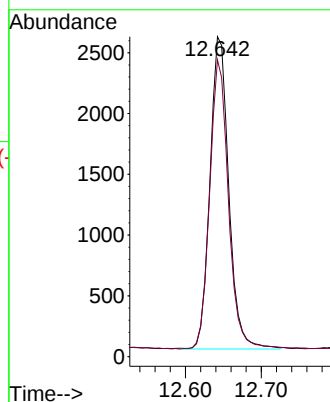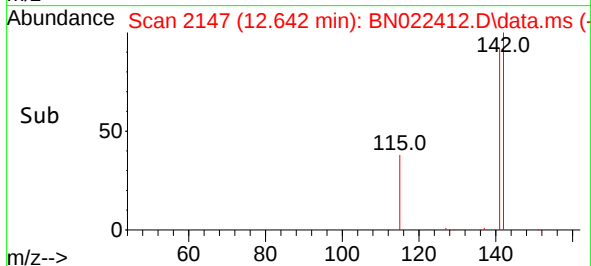

#10
Acenaphthylene
Concen: 0.036 ng/ul
RT: 14.323 min Scan# 2484
Delta R.T. 0.005 min
Lab File: BN022412.D
Acq: 31 Oct 2022 22:31

Tgt Ion:152 Resp: 1388
Ion Ratio Lower Upper
152 100
151 25.8 15.9 23.9#
153 26.2 10.8 16.2#

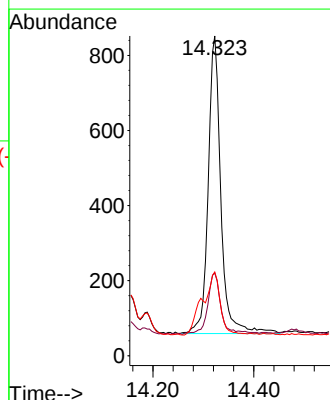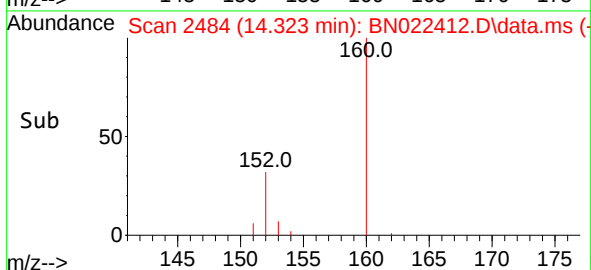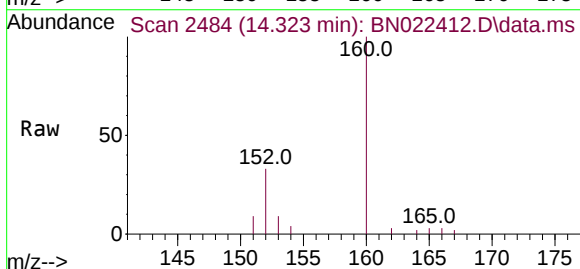



#12

Fluorene

Concen: 0.025 ng/ul

RT: 15.650 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN022412.D

Acq: 31 Oct 2022 22:31

Instrument :

BNA_N

ClientSampleId :





C0BK9DL

Tgt Ion:166	Resp:	939
Ion Ratio	Lower	Upper
166	100	
165	101.7	78.2 117.2
167	26.0	11.0 16.4

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 11/01/2022
Supervised By :mohammad ahmed 11/01/2022

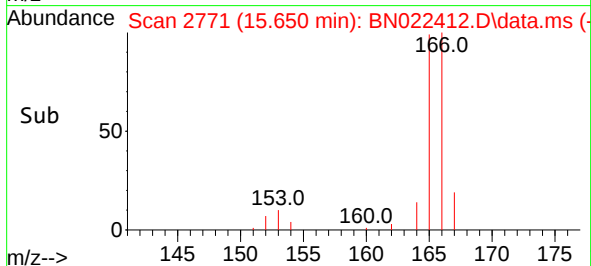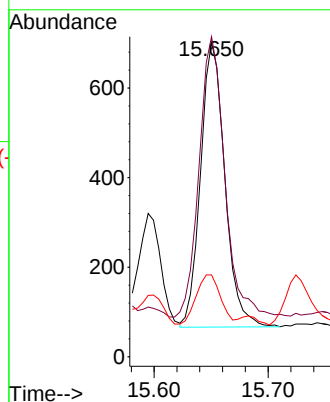

#15

Phenanthrene

Concen: 0.346 ng/ul




RT: 17.395 min Scan# 3177


Delta R.T. 0.000 min

Lab File: BN022412.D

Acq: 31 Oct 2022 22:31


Tgt Ion:178	Resp:	18853
Ion Ratio	Lower	Upper
178	100	
179	15.7	12.7 19.1
176	19.3	15.4 23.2

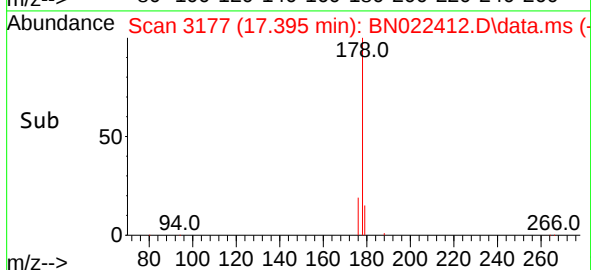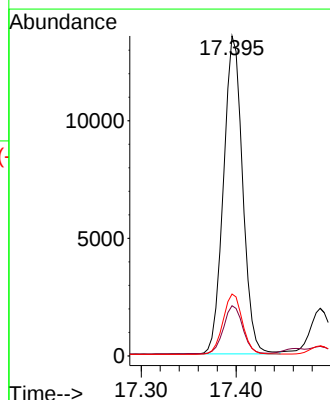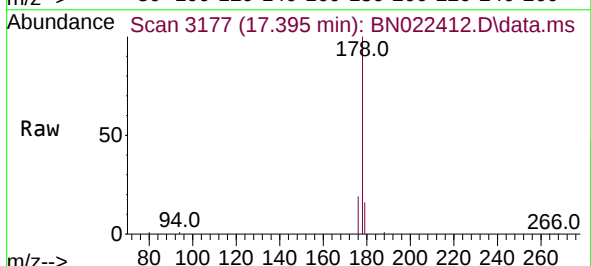

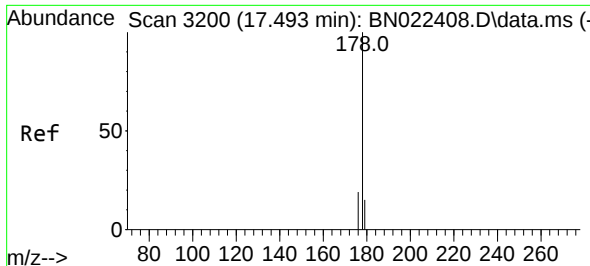

#16
 Anthracene
 Concen: 0.067 ng/ul
 RT: 17.488 min Scan# 3199
 Delta R.T. 0.000 min
 Lab File: BN022412.D
 Acq: 31 Oct 2022 22:31




Instrument :
 BNA_N
 ClientSampleId :
 C0BK9DL

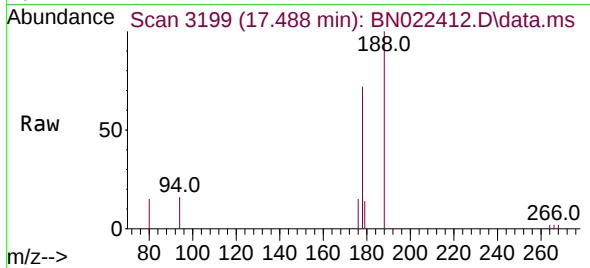

Tgt Ion:178 Resp: 3062
 Ion Ratio Lower Upper
 178 100
 179 20.0 12.6 18.8
 176 21.2 15.0 22.6




Manual Integrations
 APPROVED


Reviewed By :Jagrut Upadhyay 11/01/2022
 Supervised By :mohammad ahmed 11/01/2022

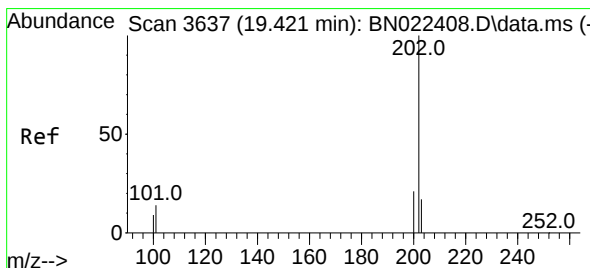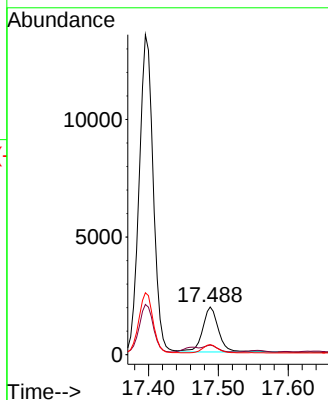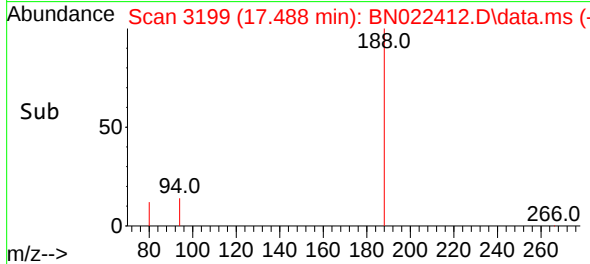

#19
 Fluoranthene
 Concen: 0.660 ng/ul
 RT: 19.421 min Scan# 3637
 Delta R.T. 0.000 min
 Lab File: BN022412.D
 Acq: 31 Oct 2022 22:31

Tgt Ion:202 Resp: 28407
 Ion Ratio Lower Upper
 202 100
 101 13.6 11.8 17.6
 100 9.8 8.7 13.1

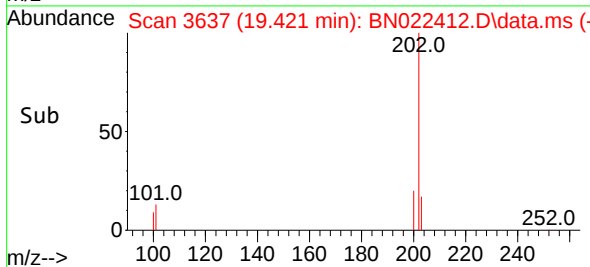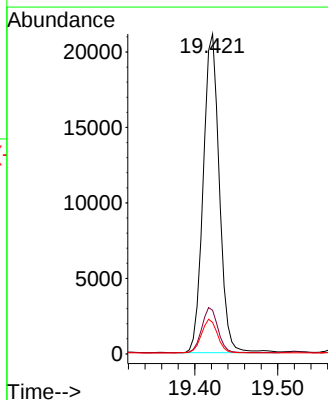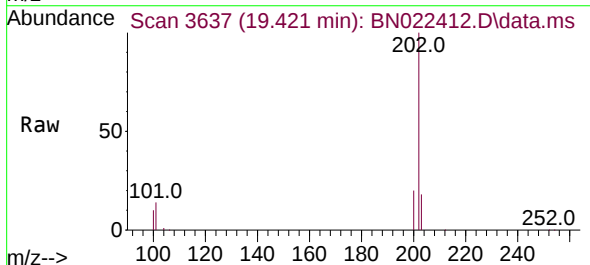

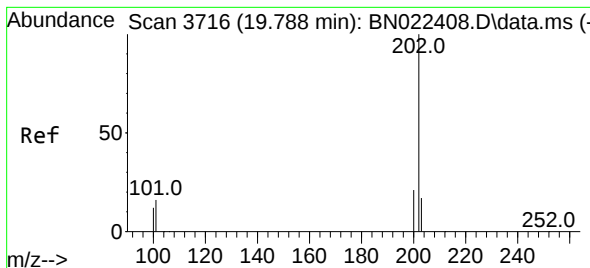

#20

Pyrene

Concen: 0.538 ng/ul m

RT: 19.784 min Scan# 3716

Delta R.T. 0.000 min

Lab File: BN022412.D

Acq: 31 Oct 2022 22:31

Instrument :

BNA_N

ClientSampleId :





C0BK9DL

Tgt Ion:	202	Resp:	2326
Ion Ratio	Lower	Upper	
202	100		
101	16.4	13.1	19.7
100	12.9	10.6	16.0

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 11/01/2022
Supervised By :mohammad ahmed 11/01/2022

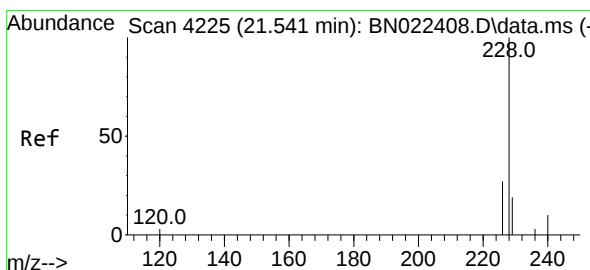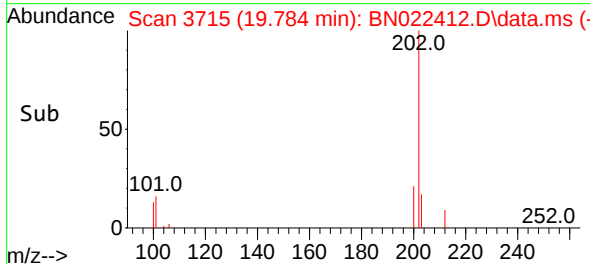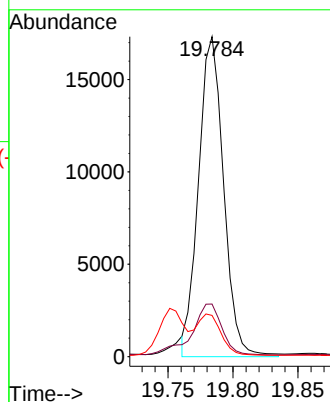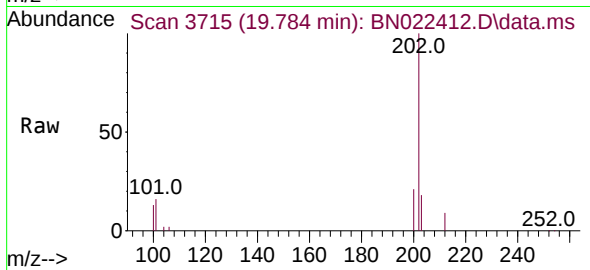

#21

Benzo(a)anthracene

Concen: 0.289 ng/ul




RT: 21.538 min Scan# 4224


Delta R.T. -0.003 min

Lab File: BN022412.D

Acq: 31 Oct 2022 22:31


Tgt Ion:	228	Resp:	10186
Ion Ratio	Lower	Upper	
228	100		
229	21.0	15.7	23.5
226	28.9	21.5	32.3

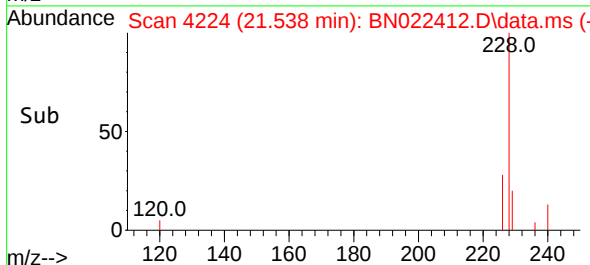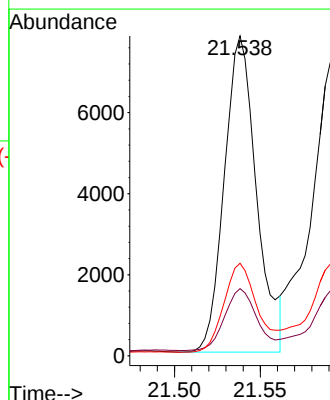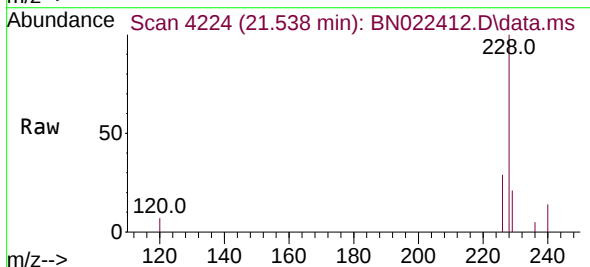

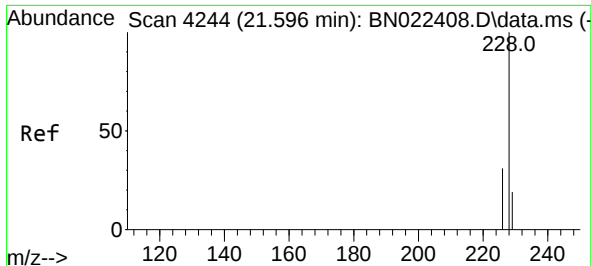

#22
Chrysene
Concen: 0.288 ng/ul
RT: 21.591 min Scan# 41
Delta R.T. -0.003 min
Lab File: BN022412.D
Acq: 31 Oct 2022 22:31




Instrument :
BNA_N
ClientSampleId :
C0BK9DL




Tgt Ion:228 Resp: 10749
Ion Ratio Lower Upper
228 100
226 31.2 23.9 35.9
229 22.2 15.9 23.9

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 11/01/2022
Supervised By :mohammad ahmed 11/01/2022

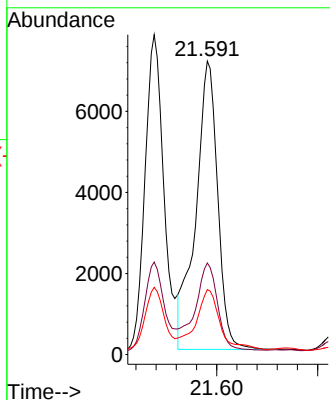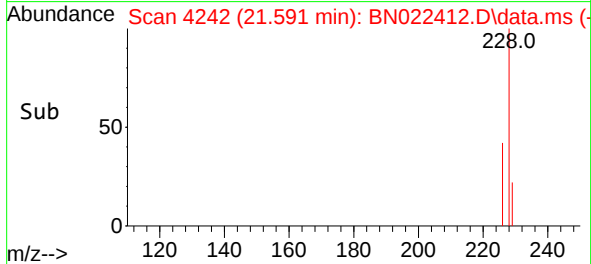


#24
Benzo(b)fluoranthene
Concen: 0.355 ng/ul m
RT: 23.251 min Scan# 4810
Delta R.T. 0.000 min
Lab File: BN022412.D
Acq: 31 Oct 2022 22:31

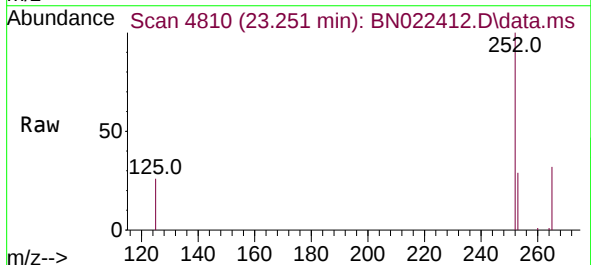


Tgt Ion:252 Resp: 12190
Ion Ratio Lower Upper
252 100
253 28.7 0.0 49.0
125 26.4 0.0 35.2

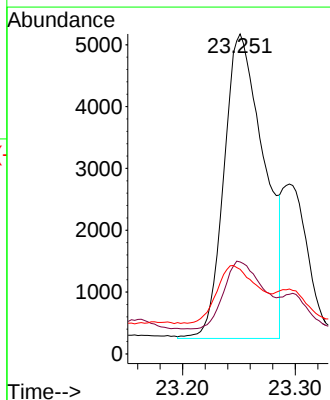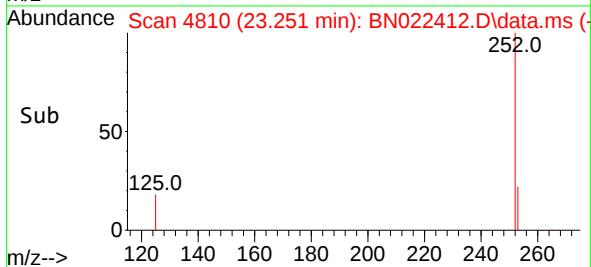

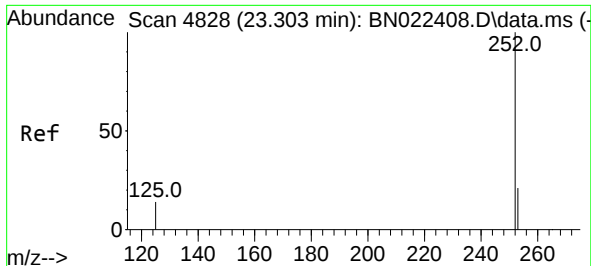

#25
Benzo(k)fluoranthene
Concen: 0.114 ng/ul m
RT: 23.295 min Scan# 4828
Delta R.T. -0.006 min
Lab File: BN022412.D
Acq: 31 Oct 2022 22:31




Instrument :
BNA_N
ClientSampleId :
C0BK9DL




Tgt Ion:252 Resp: 3803
Ion Ratio Lower Upper
252 100
253 35.1 19.7 29.5#
125 38.2 14.0 21.0#

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 11/01/2022
Supervised By :mohammad ahmed 11/01/2022

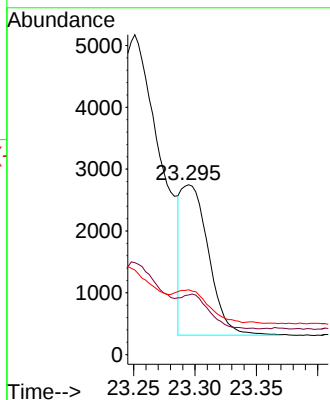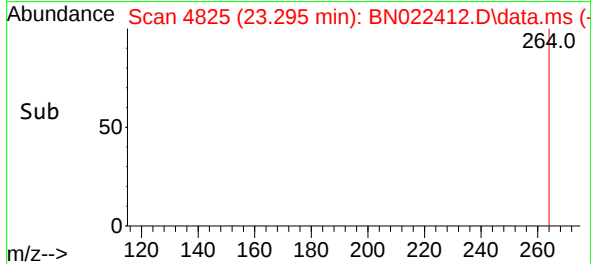


#26
Benzo(a)pyrene
Concen: 0.257 ng/ul
RT: 23.888 min Scan# 5028
Delta R.T. -0.003 min
Lab File: BN022412.D
Acq: 31 Oct 2022 22:31

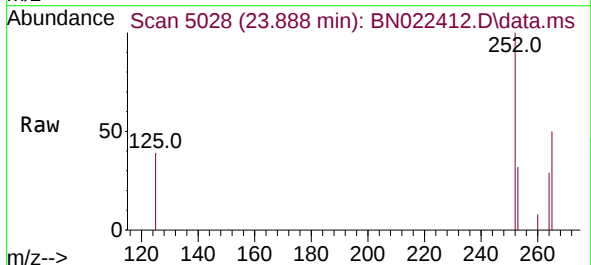

Tgt Ion:252 Resp: 7039
Ion Ratio Lower Upper
252 100
253 31.7 21.0 31.6#
125 38.9 17.9 26.9#

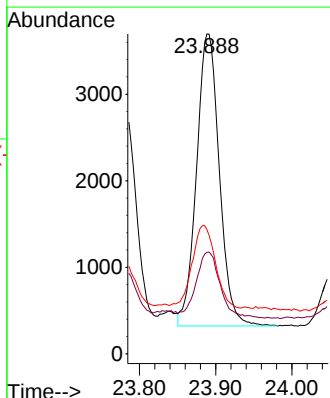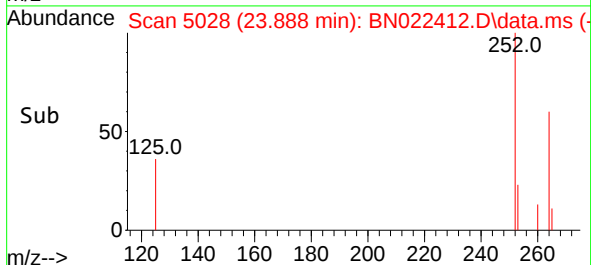




#27
Indeno(1,2,3-cd)pyrene
Concen: 0.143 ng/ul
RT: 26.565 min Scan# 5875
Delta R.T. -0.003 min
Lab File: BN022412.D
Acq: 31 Oct 2022 22:31

Instrument :

BNA_N

ClientSampleId :

C0BK9DL






Tgt Ion:276 Resp: 4875
Ion Ratio Lower Upper
276 100
138 32.5 27.7 41.5
227 0.0 0.2 0.2


Manual Integrations

APPROVED



Reviewed By :Jagrut Upadhyay 11/01/2022
Supervised By :mohammad ahmed 11/01/2022

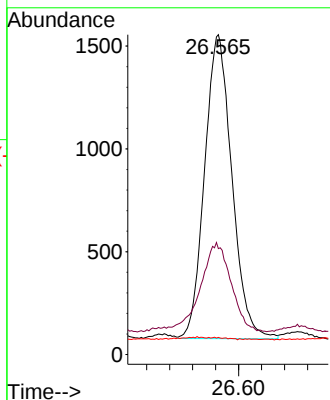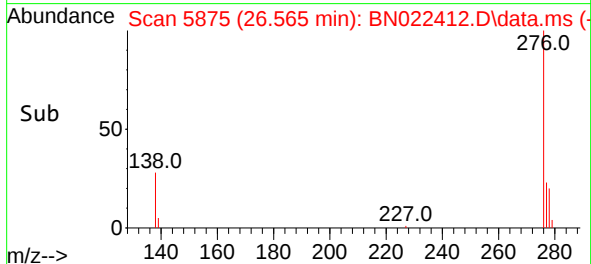


#28
Dibenzo(a,h)anthracene
Concen: 0.048 ng/ul
RT: 26.578 min Scan# 5879
Delta R.T. -0.010 min
Lab File: BN022412.D
Acq: 31 Oct 2022 22:31

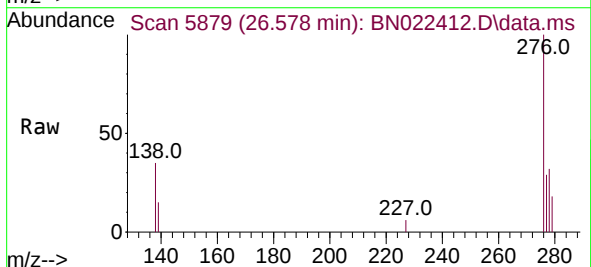

Tgt Ion:278 Resp: 1305
Ion Ratio Lower Upper
278 100
139 46.9 19.6 29.4#
279 56.3 20.6 30.8#

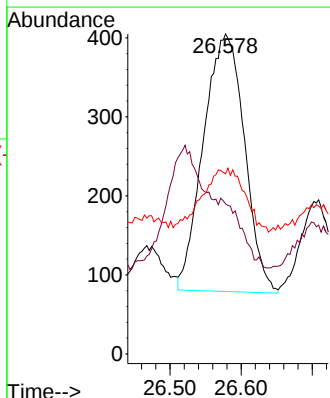



#29

Benzo(g,h,i)perylene

Concen: 0.137 ng/ul

RT: 27.356 min Scan# 61

Delta R.T. -0.003 min

Lab File: BN022412.D


Acq: 31 Oct 2022 22:31

Instrument :

BNA_N

ClientSampleId :

C0BK9DL

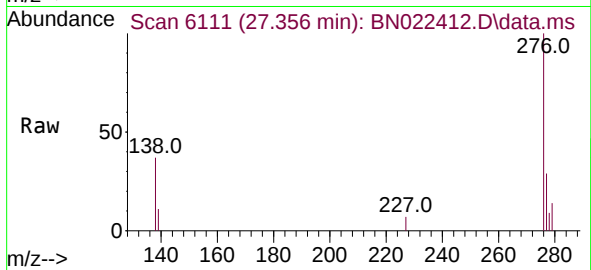

Tgt Ion:276 Resp: 3806

Ion Ratio Lower Upper

276 100

138 36.8 25.2 37.8

277 28.8 19.9 29.9

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 11/01/2022

Supervised By :mohammad ahmed 11/01/2022

