

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
 Data File : BN022414.D
 Acq On : 31 Oct 2022 23:46
 Operator : CG/JU
 Sample : N5277-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4W7

Quant Time: Nov 01 01:12:57 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 01 01:09:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.927	152	4006	0.400	ng/ul	0.00
4) Naphthalene-d8	10.750	136	12762	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.600	164	6543	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.353	188	11669	0.400	ng/ul	0.00
17) Chrysene-d12	21.553	240	7029	0.400	ng/ul	0.00
23) Perylene-d12	23.999	264	6409	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.236	96	21518	4.133	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.351	152	6521	0.338	ng/ul	0.00
18) Fluoranthene-d10	19.389	212	10167	0.431	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.278	88	928	0.174	ng/ul#	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
Data File : BN022414.D
Acq On : 31 Oct 2022 23:46
Operator : CG/JU
Sample : N5277-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4W7


Quant Time: Nov 01 01:12:57 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 01 01:09:32 2022
Response via : Initial Calibration

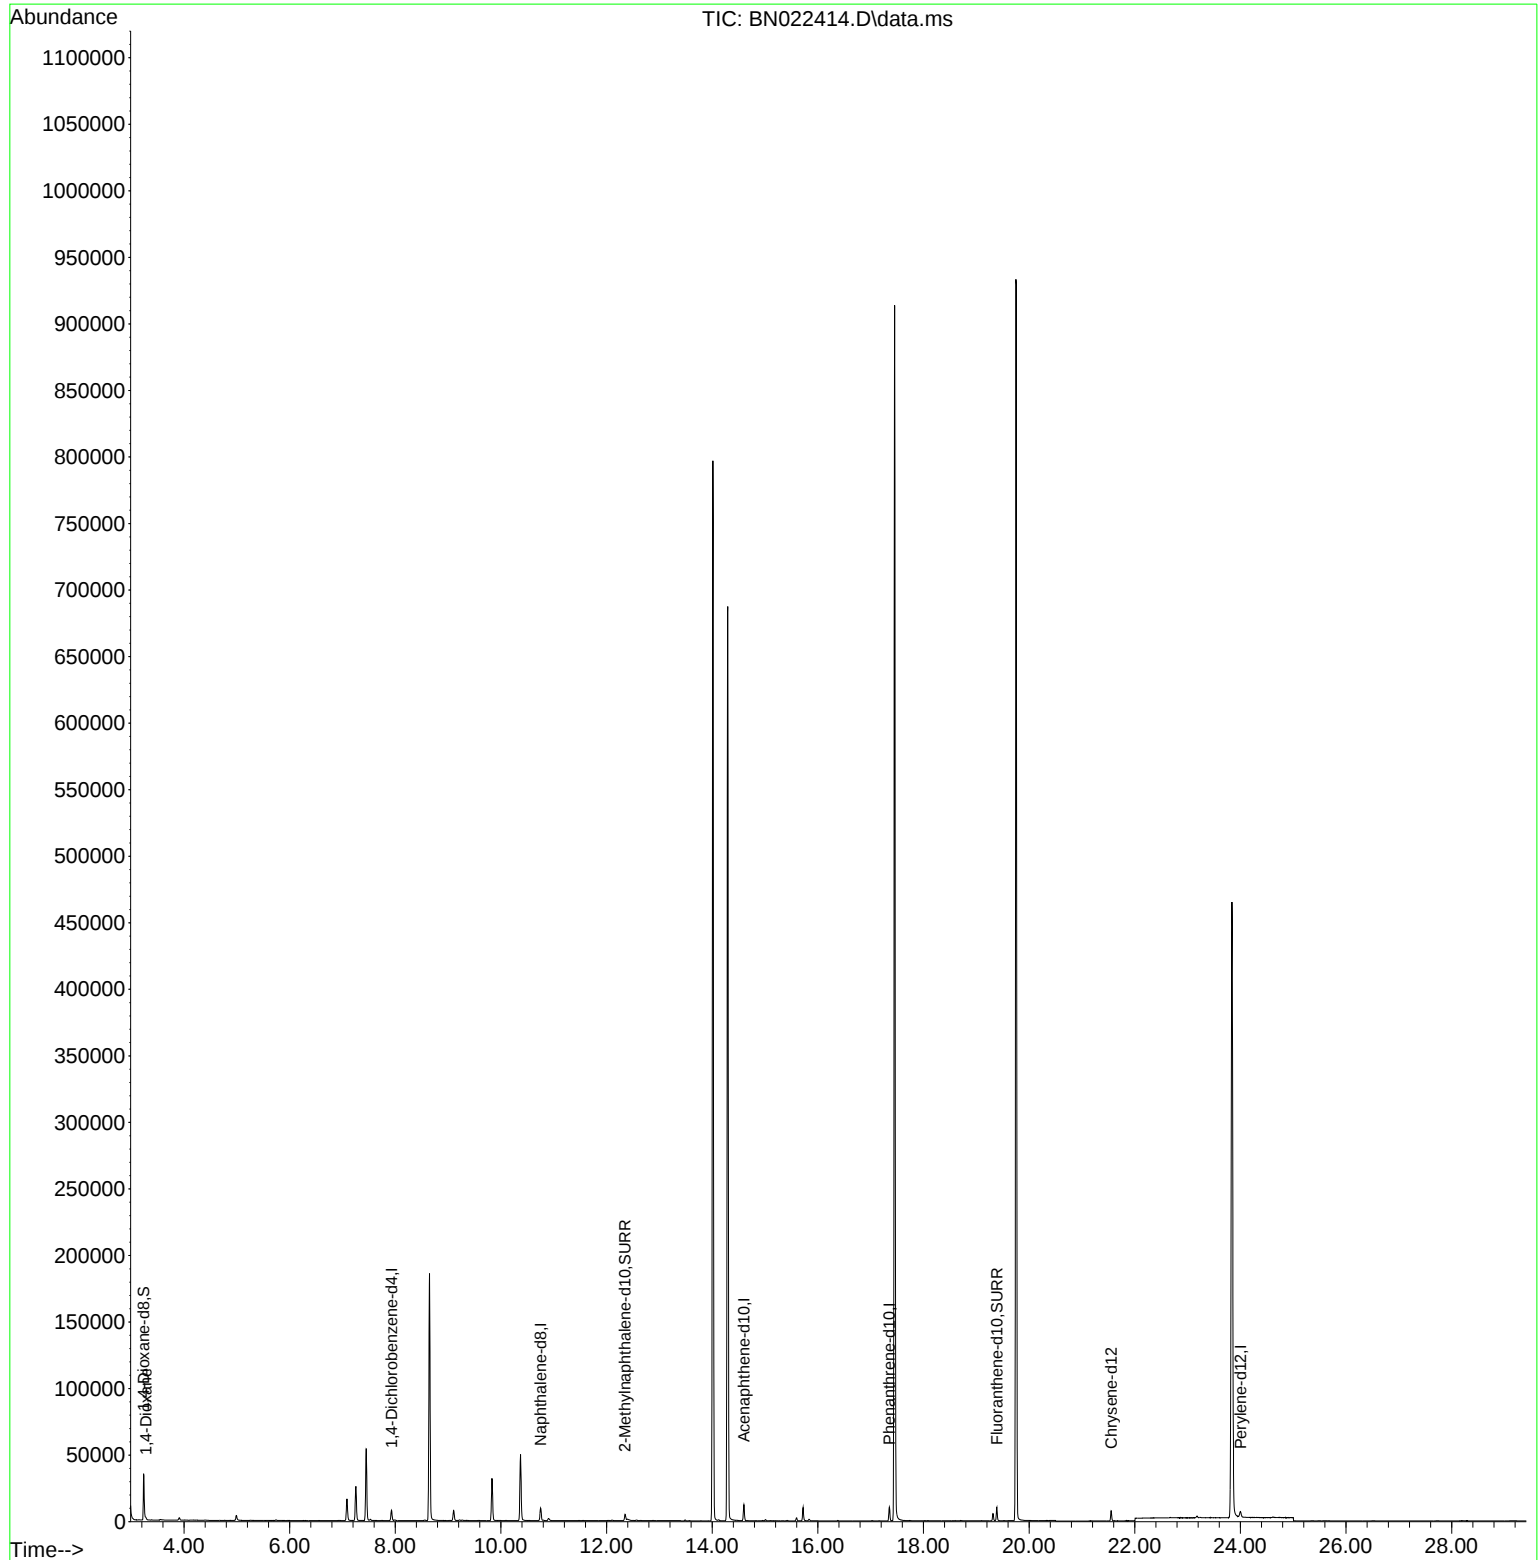

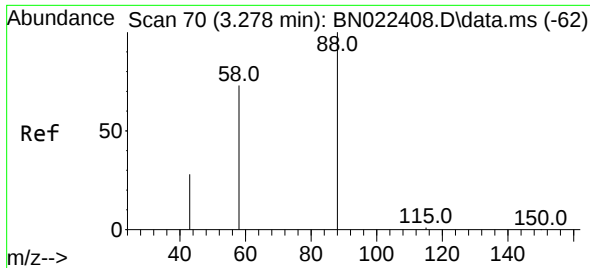

#2
 1,4-Dioxane
 Concen: 0.174 ng/ul
 RT: 3.278 min Scan# 70
 Delta R.T. -0.004 min
 Lab File: BN022414.D
 Acq: 31 Oct 2022 23:46

Instrument :
 BNA_N
 ClientSampleId :
 EW4W7

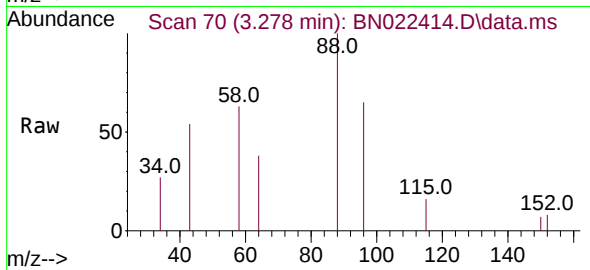

Tgt Ion:	88	Resp:	928
Ion	Ratio	Lower	Upper
88	100		
43	53.9	27.4	41.2#
58	63.1	48.2	72.2

