

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
 Data File : BN022418.D
 Acq On : 01 Nov 2022 02:15
 Operator : CG/JU
 Sample : N5276-13
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4X3

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 11/01/2022
 Supervised By :mohammad ahmed 11/01/2022

Quant Time: Nov 01 02:44:38 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 01 01:09:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	4657	0.400	ng/ul	0.00
4) Naphthalene-d8	10.750	136	16469m	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.600	164	11516m	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.353	188	15686	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.550	240	8242	0.400	ng/ul	# 0.00
23) Perylene-d12	23.996	264	7288	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.236	96	28193	4.658	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.351	152	9091m	0.365	ng/ul	0.00
18) Fluoranthene-d10	19.393	212	13408	0.485	ng/ul	0.00
Target Compounds						Qvalue
16) Anthracene	17.488	178	1377	0.031	ng/ul#	54

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
Data File : BN022418.D
Acq On : 01 Nov 2022 02:15
Operator : CG/JU
Sample : N5276-13
Misc :
ALS Vial : 24 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
EW4X3

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 11/01/2022
Supervised By :mohammad ahmed 11/01/2022


Quant Time: Nov 01 02:44:38 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 01 01:09:32 2022
Response via : Initial Calibration

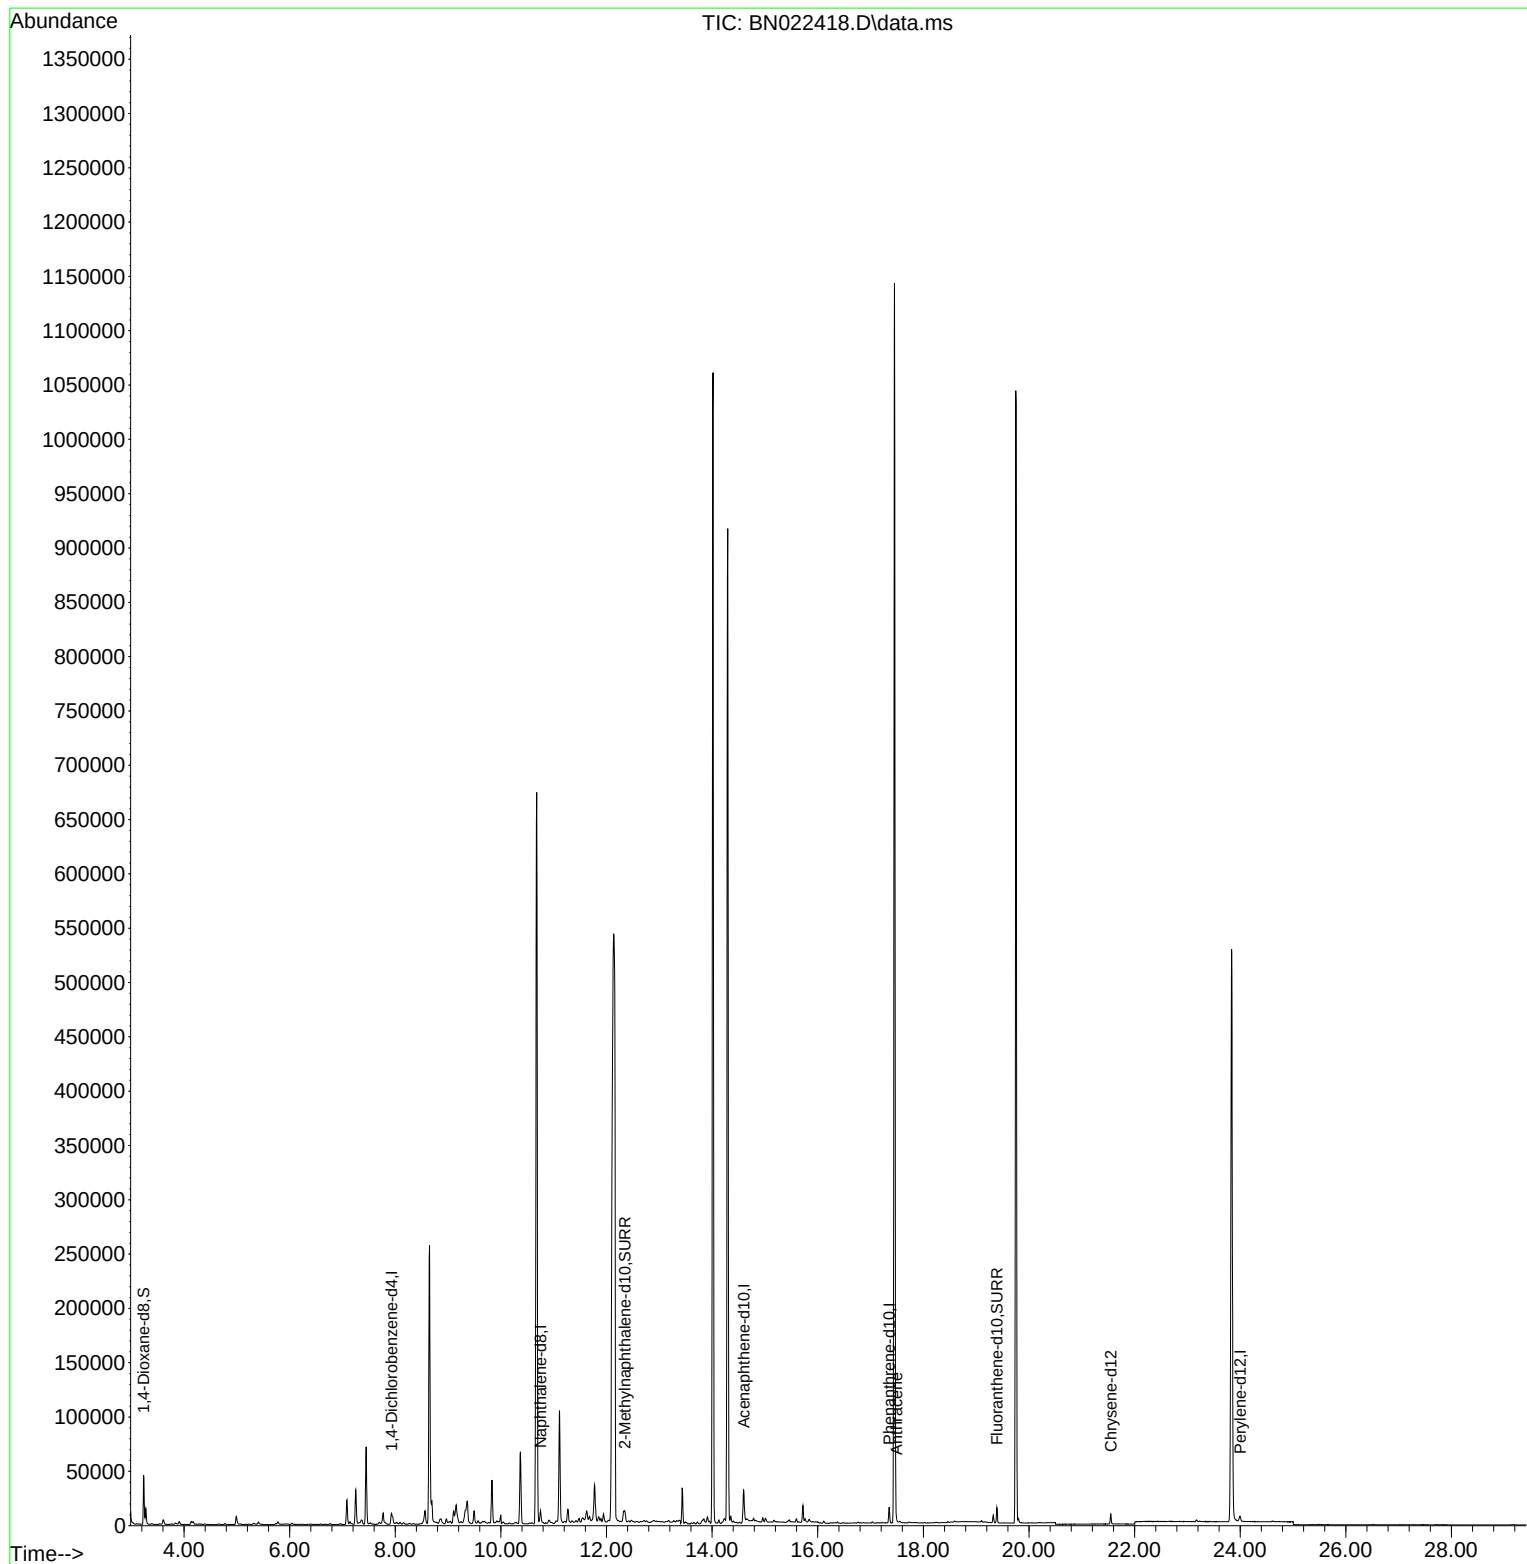

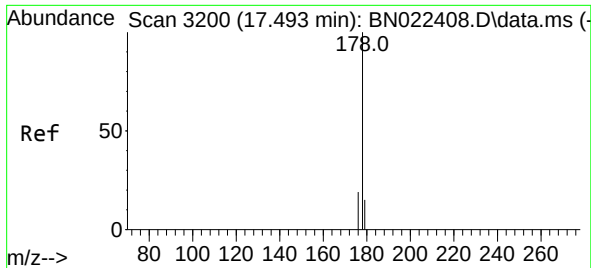

#16
 Anthracene
 Concen: 0.031 ng/ul
 RT: 17.488 min Scan# 3199
 Delta R.T. 0.000 min
 Lab File: BN022418.D
 Acq: 01 Nov 2022 02:15

Instrument :
 BNA_N
 ClientSampleId :
 EW4X3

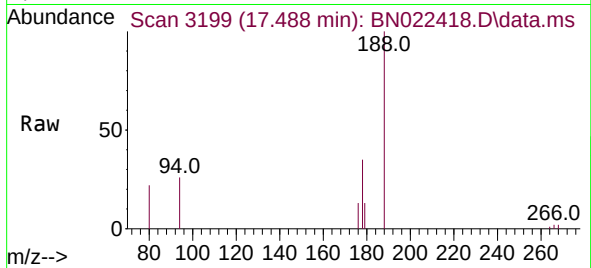

Tgt Ion:178 Resp: 1372
 Ion Ratio Lower Upper
 178 100
 179 38.7 12.6 18.8
 176 36.0 15.0 22.6

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 11/01/2022
 Supervised By :mohammad ahmed 11/01/2022

