

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
 Data File : BN022421.D
 Acq On : 01 Nov 2022 04:07
 Operator : CG/JU
 Sample : N5277-10
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4X1

Quant Time: Nov 01 04:41:55 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 01 01:09:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.927	152	4651	0.400	ng/u1	0.00
4) Naphthalene-d8	10.749	136	15739	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.599	164	8870	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.352	188	15450	0.400	ng/u1	0.00
17) Chrysene-d12	21.550	240	8952	0.400	ng/u1	0.00
23) Perylene-d12	23.994	264	7295	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.236	96	23811	3.939	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.349	152	7170	0.301	ng/u1	0.00
18) Fluoranthene-d10	19.387	212	12445	0.414	ng/u1	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.278	88	1192	0.192	ng/u1#	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
Data File : BN022421.D
Acq On : 01 Nov 2022 04:07
Operator : CG/JU
Sample : N5277-10
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4X1

Quant Time: Nov 01 04:41:55 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 01 01:09:32 2022
Response via : Initial Calibration

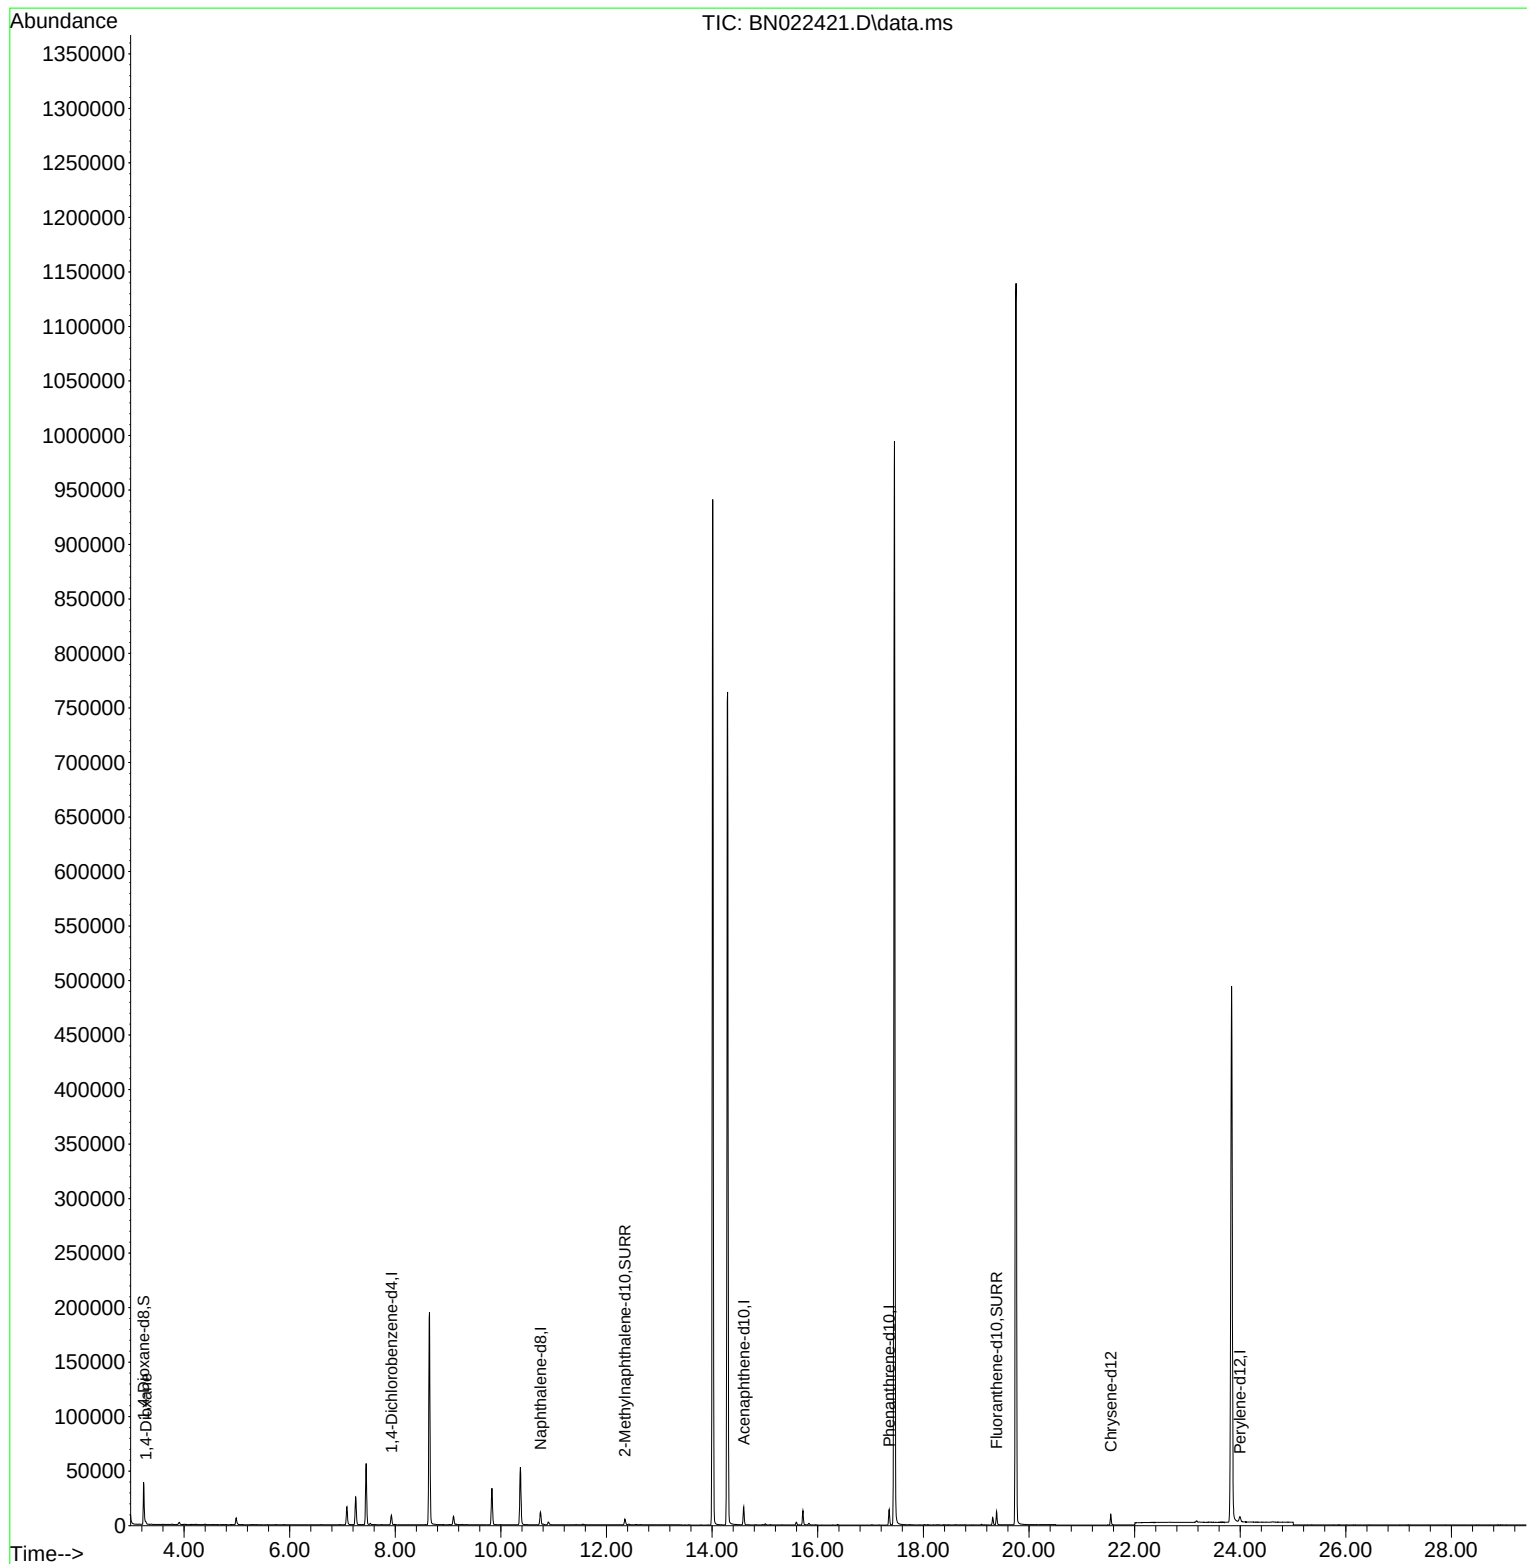

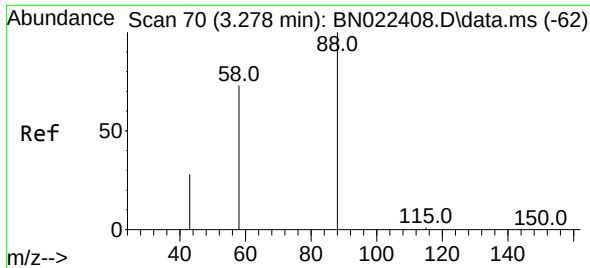

#2
 1,4-Dioxane
 Concen: 0.192 ng/ul
 RT: 3.278 min Scan# 70
 Delta R.T. -0.004 min
 Lab File: BN022421.D
 Acq: 01 Nov 2022 04:07

Instrument :
 BNA_N
 ClientSampleId :
 EW4X1

Tgt Ion: 88 Resp: 1192
 Ion Ratio Lower Upper
 88 100
 43 53.5 27.4 41.2#
 58 63.5 48.2 72.2

