

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
 Data File : BN022431.D
 Acq On : 01 Nov 2022 10:57
 Operator : CG/JU
 Sample : N5277-13
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4X4

Quant Time: Nov 02 00:52:49 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 01 01:09:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.927	152	4389	0.400	ng/ul	0.00
4) Naphthalene-d8	10.749	136	17625	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.598	164	10358	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.351	188	17669	0.400	ng/ul	0.00
17) Chrysene-d12	21.553	240	9216	0.400	ng/ul	0.00
23) Perylene-d12	23.993	264	7656	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.236	96	24552	4.304	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.349	152	7470	0.280	ng/ul	0.00
18) Fluoranthene-d10	19.387	212	13335	0.431	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.278	88	2016	0.344	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
Data File : BN022431.D
Acq On : 01 Nov 2022 10:57
Operator : CG/JU
Sample : N5277-13
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4X4

Quant Time: Nov 02 00:52:49 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 01 01:09:32 2022
Response via : Initial Calibration

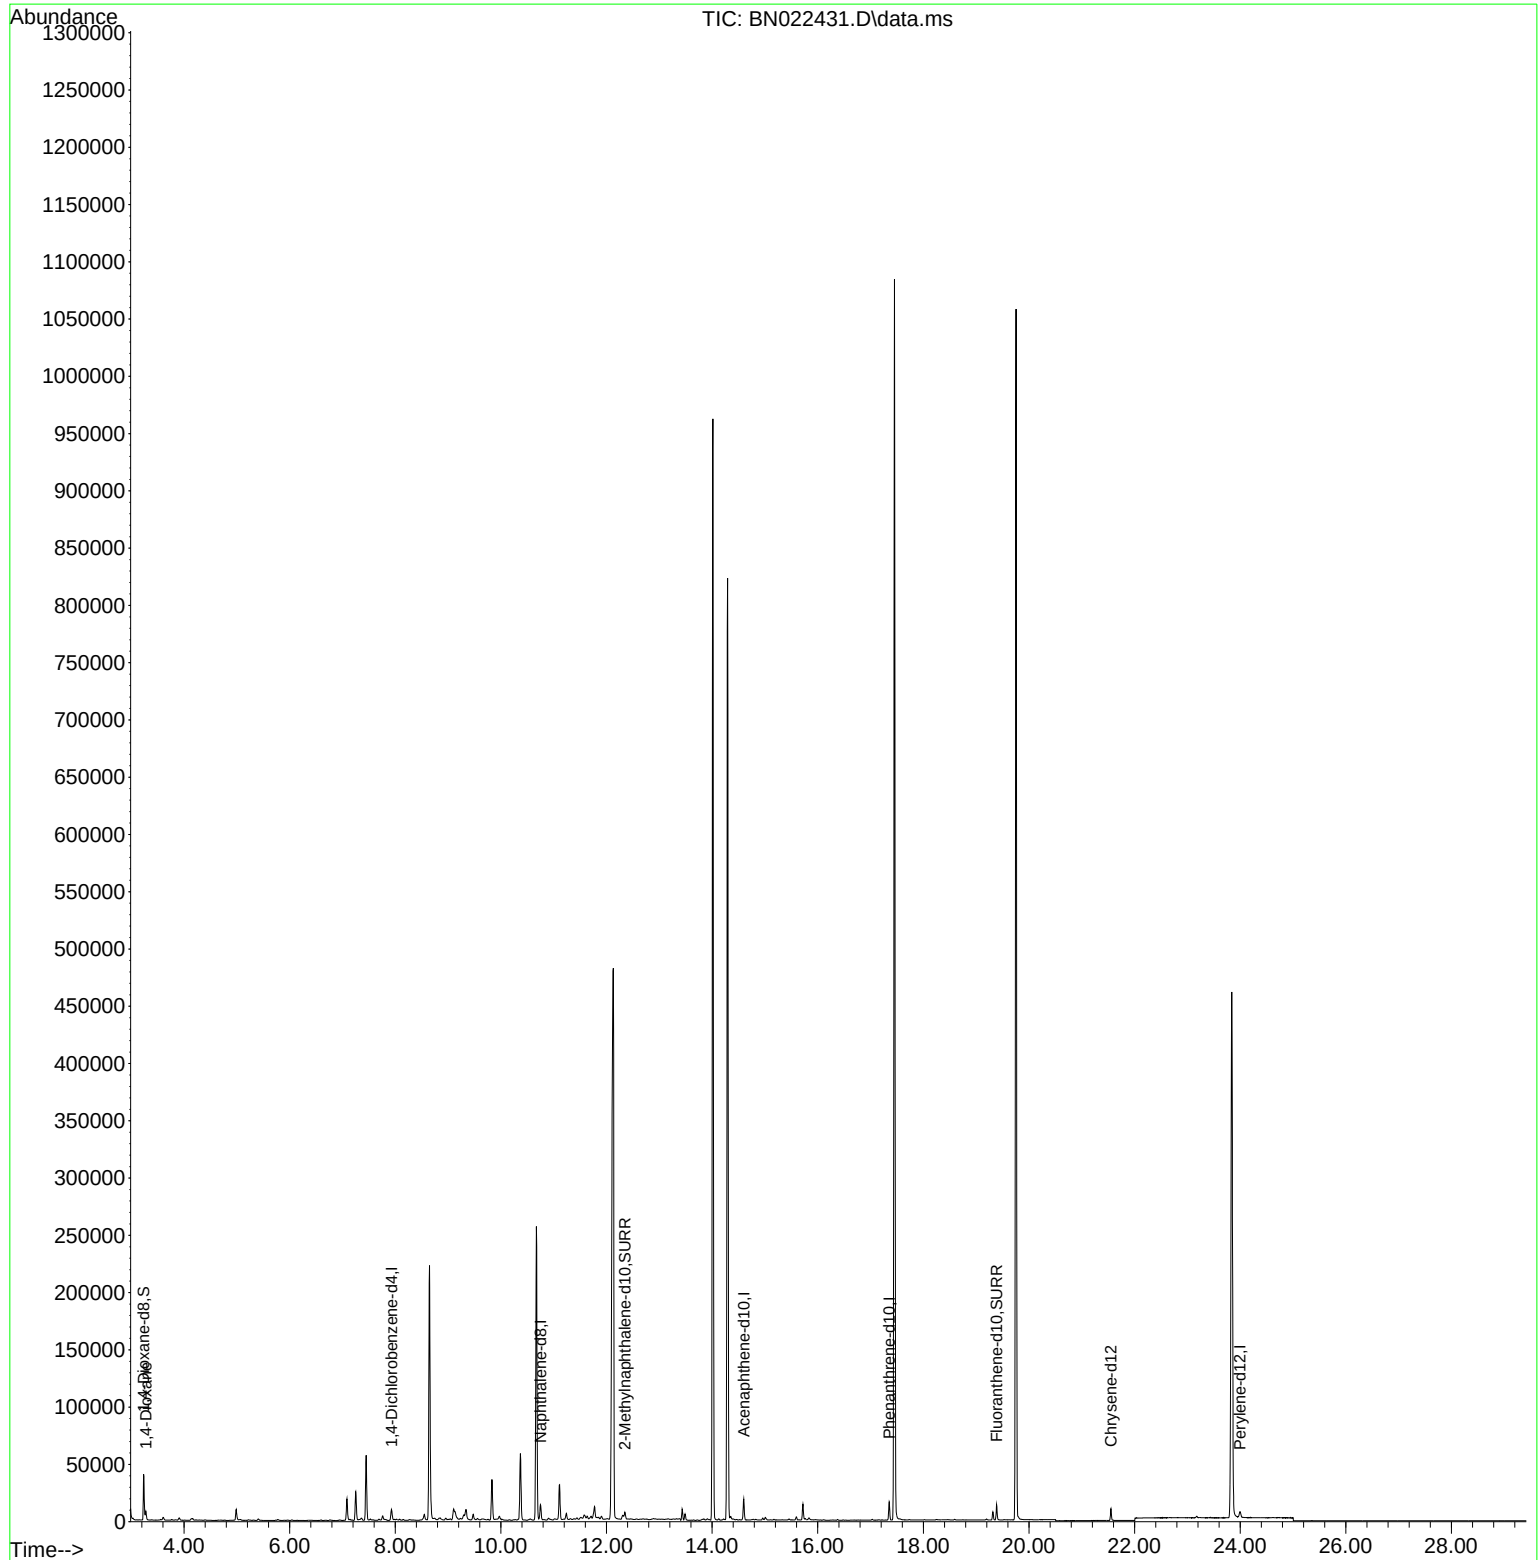

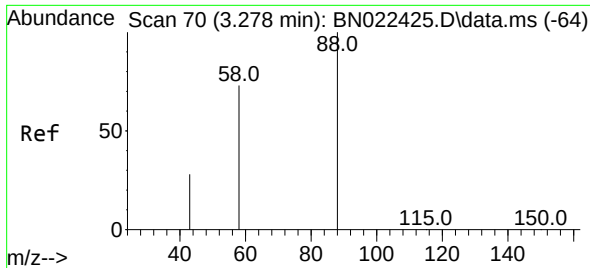

#2
 1,4-Dioxane
 Concen: 0.344 ng/ul
 RT: 3.278 min Scan# 70
 Delta R.T. -0.005 min
 Lab File: BN022431.D
 Acq: 01 Nov 2022 10:57

Instrument :
 BNA_N
 ClientSampleId :
 EW4X4

Tgt Ion: 88	Resp: 2016
Ion Ratio	Lower Upper
88	100
43	266.7 27.4 41.2#
58	92.7 48.2 72.2#

