

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\
 Data File : BN022441.D
 Acq On : 01 Nov 2022 17:17
 Operator : CG/JU
 Sample : N5277-18
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4X9

Quant Time: Nov 02 00:54:53 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 01 01:09:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	4159	0.400	ng/ul	0.00
4) Naphthalene-d8	10.750	136	16549	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.600	164	9085	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.353	188	17630	0.400	ng/ul	0.00
17) Chrysene-d12	21.556	240	9446	0.400	ng/ul	0.00
23) Perylene-d12	24.002	264	7322	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.236	96	25559	4.729	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.351	152	8416	0.336	ng/ul	0.00
18) Fluoranthene-d10	19.389	212	14665	0.462	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.278	88	1135	0.205	ng/ul#	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103122\  
Data File : BN022441.D  
Acq On    : 01 Nov 2022  17:17  
Operator  : CG/JU  
Sample    : N5277-18  
Misc      :  
ALS Vial  : 48    Sample Multiplier: 1
```

Instrument :
BNA_N
ClientSampleId :
EW4X9

Quant Time: Nov 02 00:54:53 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Qlast Update : Tue Nov 01 01:09:32 2022
Response via : Initial Calibration

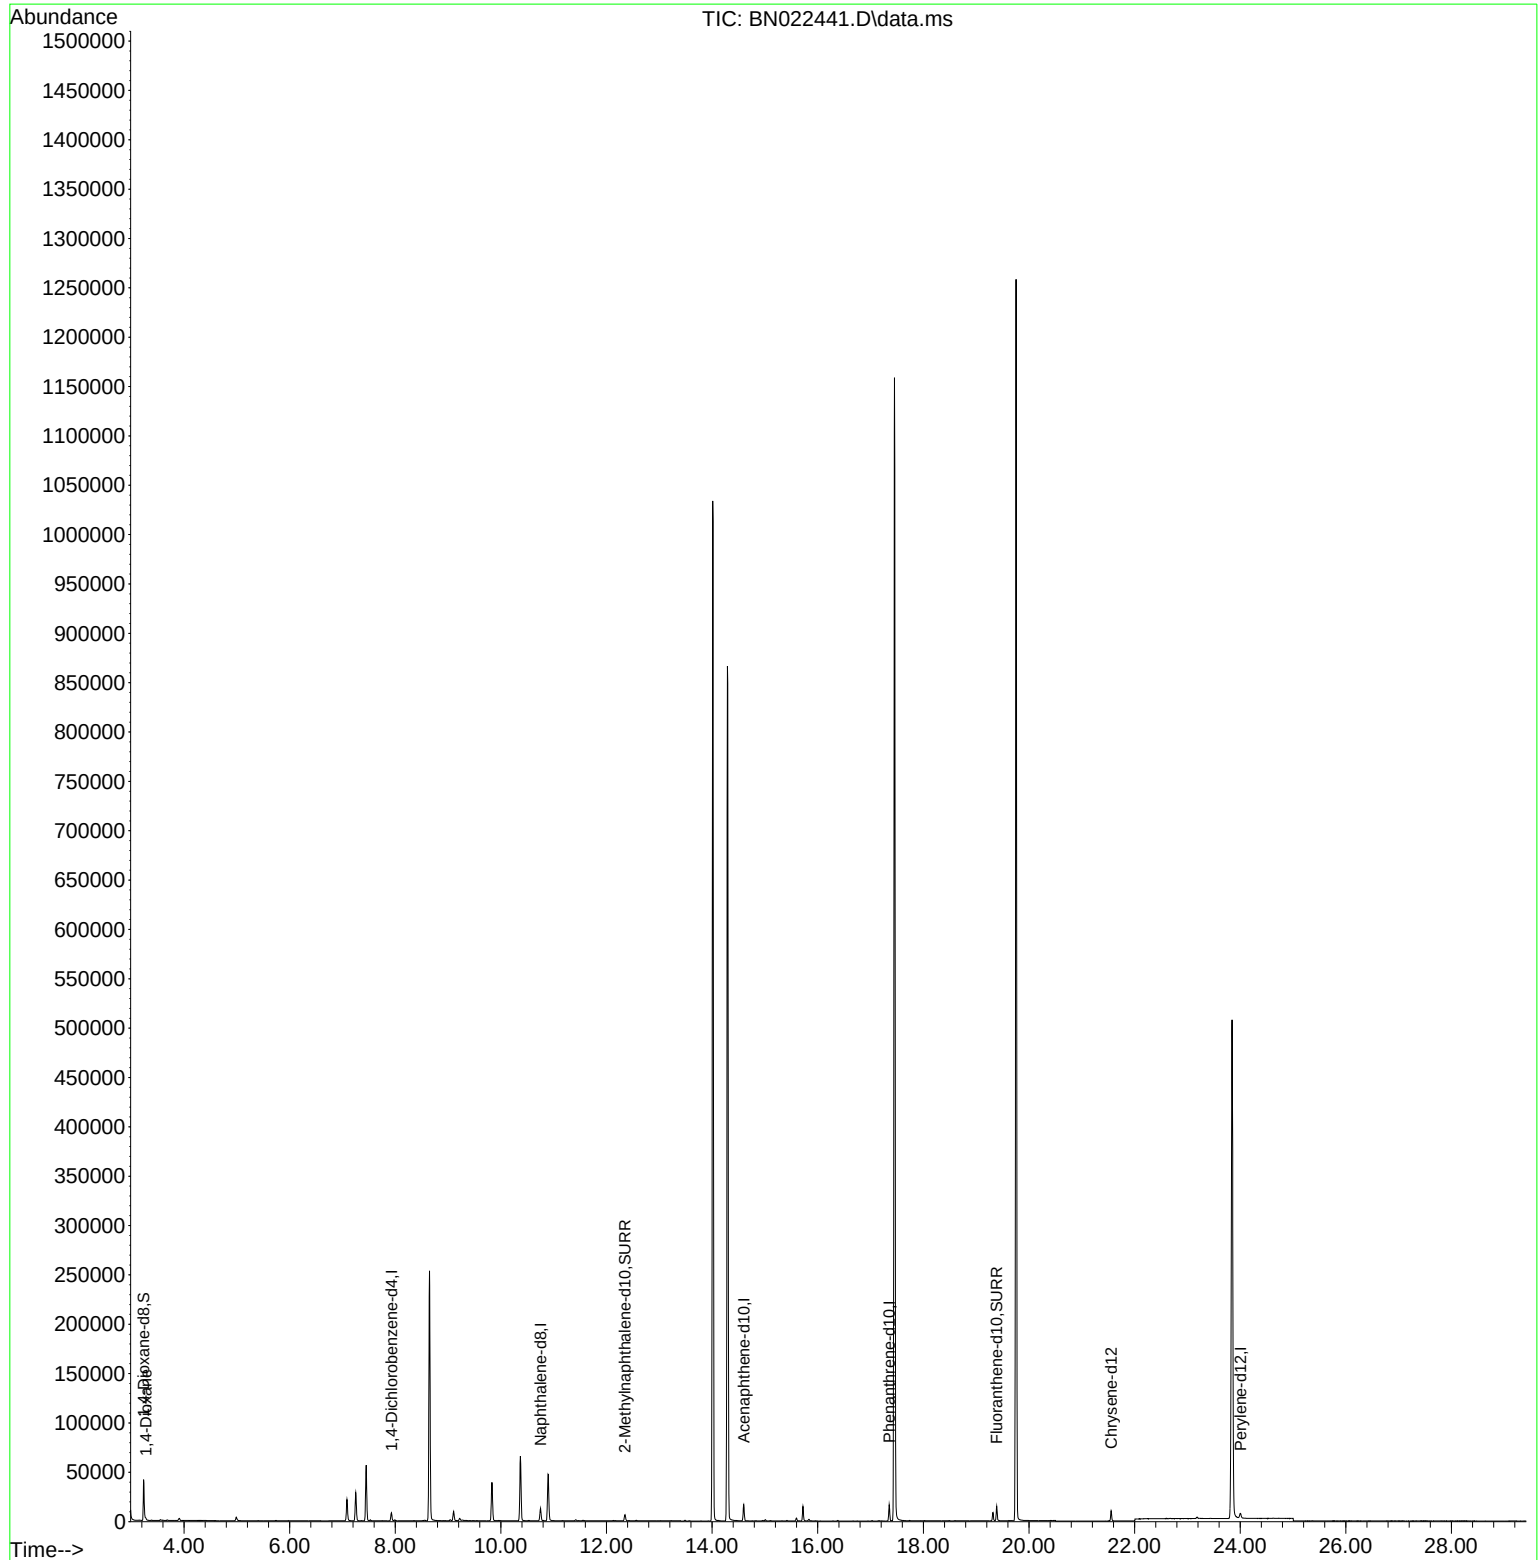

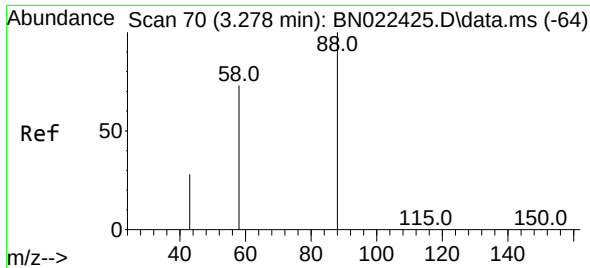

#2
 1,4-Dioxane
 Concen: 0.205 ng/ul
 RT: 3.278 min Scan# 70
 Delta R.T. -0.004 min
 Lab File: BN022441.D
 Acq: 01 Nov 2022 17:17

Instrument :
 BNA_N
 ClientSampleId :
 EW4X9

Tgt Ion: 88	Resp: 1135
Ion Ratio	Lower Upper
88	100
43	55.4 27.4 41.2#
58	65.4 48.2 72.2

