

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
 Data File : BN034776.D
 Acq On : 31 Oct 2024 21:18
 Operator : RC/JU
 Sample : P4529-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F7H13

Quant Time: Nov 03 23:23:07 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 11:13:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.600	152	8793	0.400	ng/ul	0.00
4) Naphthalene-d8	10.366	136	27899	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.236	164	15969	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-16.98
17) Chrysene-d12	21.172	240	21479	0.400	ng/ul	0.00
23) Perylene-d12	23.223	264	1239315	0.400	ng/ul	#-0.13
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.170	96	61639	6.772	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.961	152	15648	0.447	ng/ul	0.00
18) Fluoranthene-d10	19.014	212	30091	0.430	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.187	88	244	0.024	ng/ul#	4
20) Pyrene	19.381	202	3883	0.036	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034776.D
Acq On : 31 Oct 2024 21:18
Operator : RC/JU
Sample : P4529-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F7H13

Quant Time: Nov 03 23:23:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration




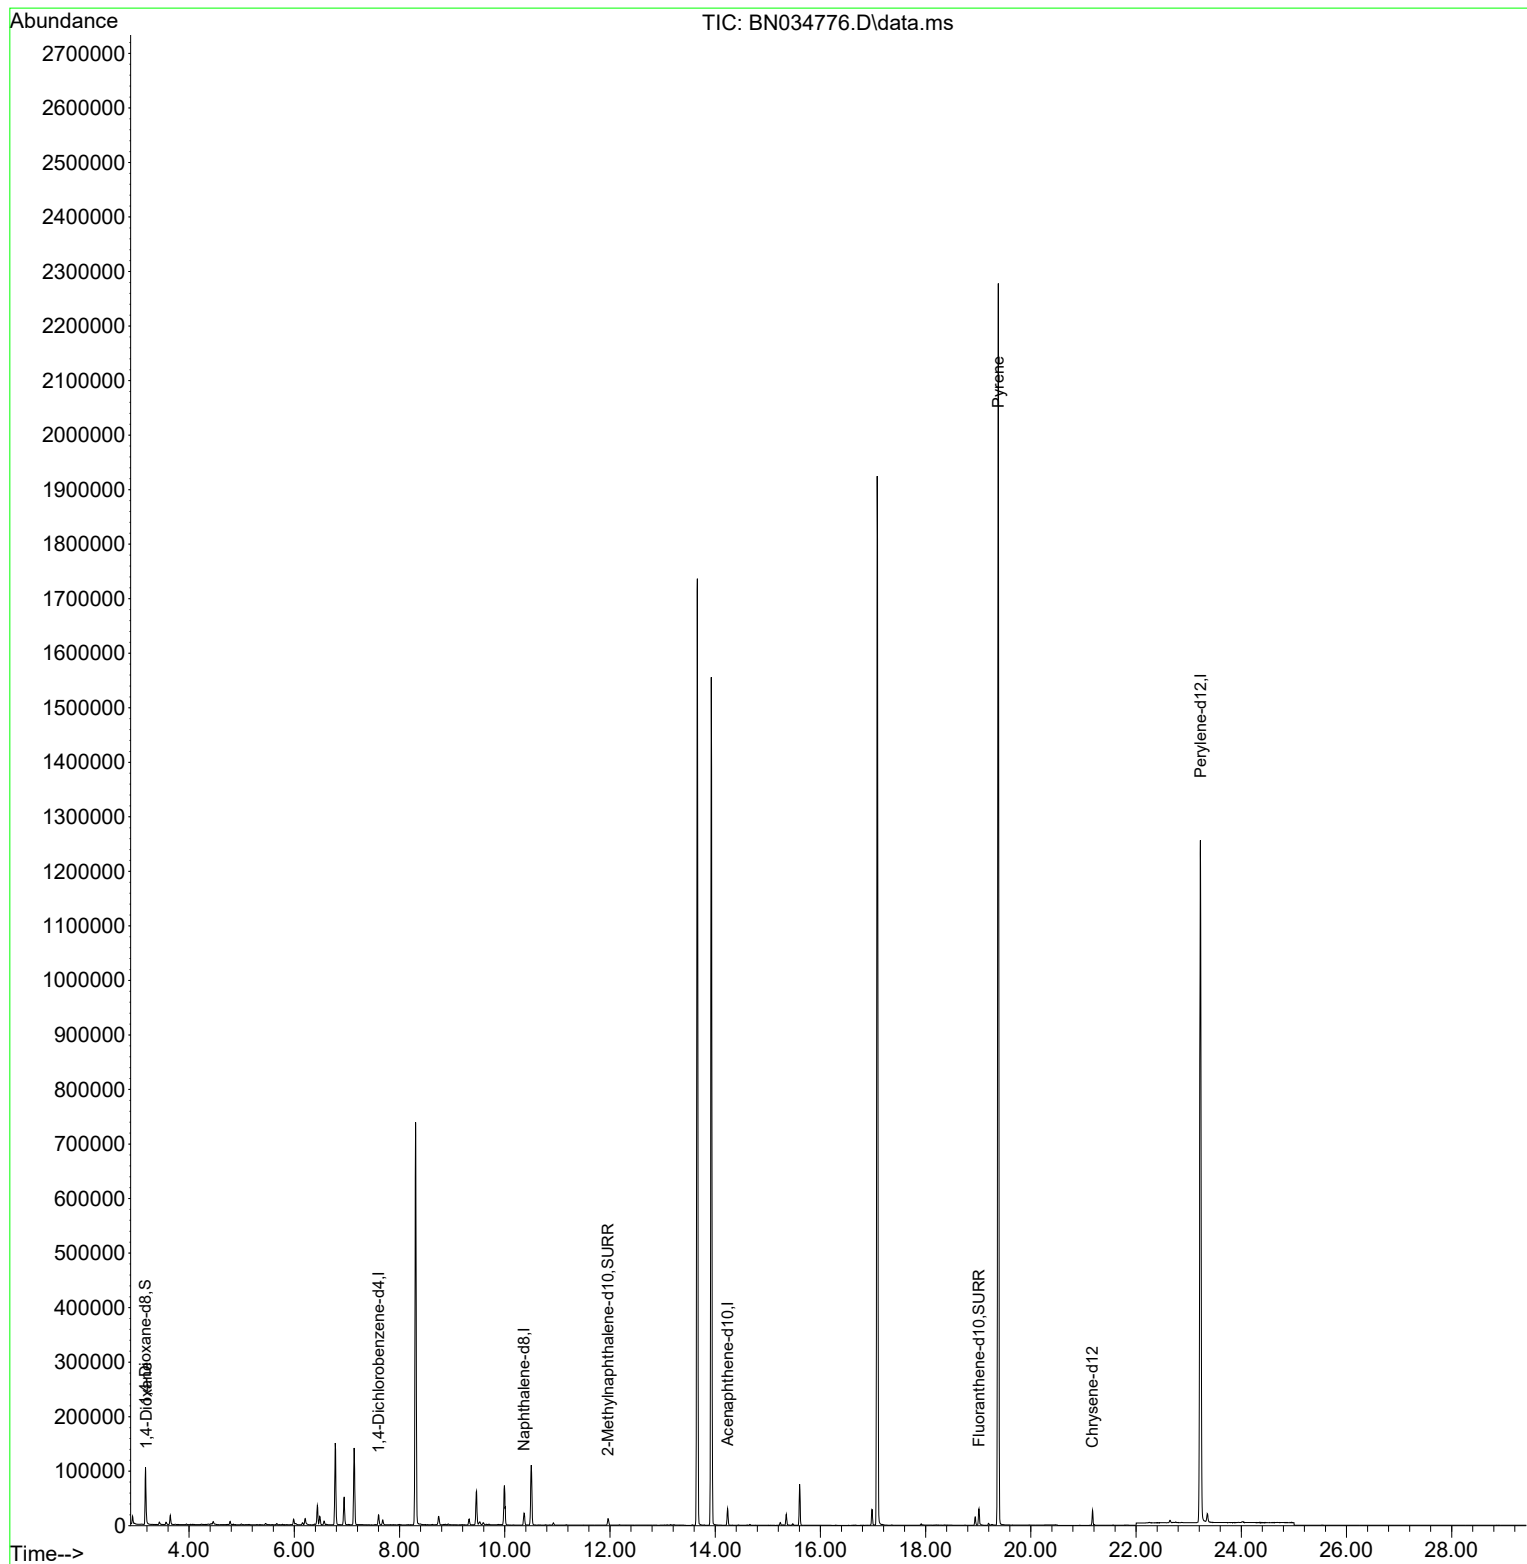


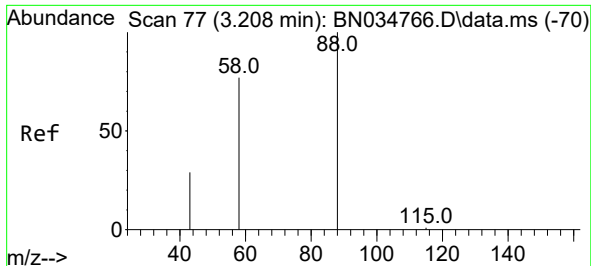

#2
1,4-Dioxane
Concen: 0.024 ng/ul
RT: 3.187 min Scan# 71
Delta R.T. -0.021 min
Lab File: BN034776.D
Acq: 31 Oct 2024 21:18

Instrument :
BNA_N
ClientSampleId :
F7H13

Tgt Ion: 88 Resp: 244
Ion Ratio Lower Upper
88 100
43 155.0 41.9 62.9#
58 21.8 57.5 86.3#

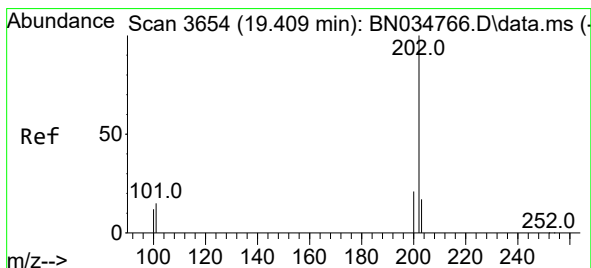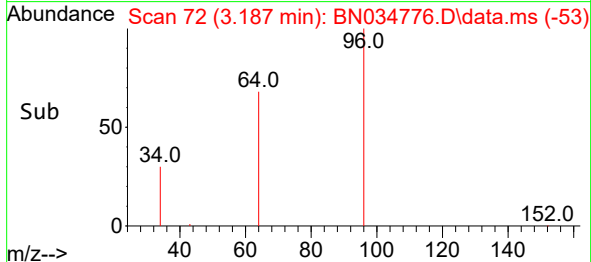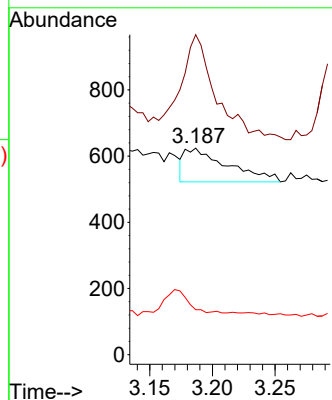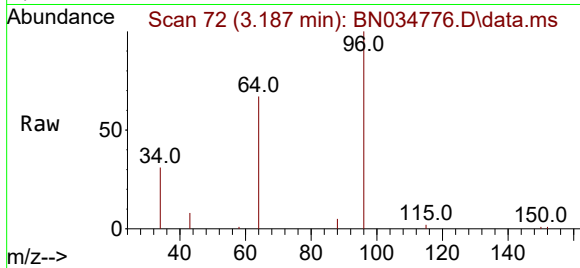

#20
Pyrene
Concen: 0.036 ng/ul
RT: 19.381 min Scan# 3648
Delta R.T. -0.028 min
Lab File: BN034776.D
Acq: 31 Oct 2024 21:18

Tgt Ion: 202 Resp: 3883
Ion Ratio Lower Upper
202 100
101 191.2 12.4 18.6#
100 1372.1 10.0 15.0#

