

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
 Data File : BN034777.D
 Acq On : 31 Oct 2024 21:54
 Operator : RC/JU
 Sample : PB164351BS
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SLCS351

Quant Time: Nov 03 23:23:13 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 11:13:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.600	152	7222	0.400	ng/ul	0.00
4) Naphthalene-d8	10.366	136	21776	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.236	164	11957	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.979	188	24536	0.400	ng/ul	0.00
17) Chrysene-d12	21.172	240	17199	0.400	ng/ul	0.00
23) Perylene-d12	23.355	264	14356	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.174	96	6570	0.879	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.967	152	13382	0.490	ng/ul	0.00
18) Fluoranthene-d10	19.014	212	26873	0.480	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.203	88	18605	2.267	ng/ul#	84
5) Naphthalene	10.416	128	27451	0.476	ng/ul	100
7) 2-Methylnaphthalene	12.038	142	17580	0.469	ng/ul	100
8) 1-Methylnaphthalene	12.258	142	17875	0.468	ng/ul	100
10) Acenaphthylene	13.953	152	25583	0.470	ng/ul	99
11) Acenaphthene	14.296	153	19604	0.471	ng/ul	99
12) Fluorene	15.290	166	21069	0.454	ng/ul	98
14) Pentachlorophenol	16.633	266	4661	0.963	ng/ul	99
15) Phenanthrene	17.021	178	34143	0.460	ng/ul	99
16) Anthracene	17.114	178	30952	0.451	ng/ul	100
19) Fluoranthene	19.042	202	38672	0.464	ng/ul	99
20) Pyrene	19.404	202	40401	0.465	ng/ul	97
21) Benzo(a)anthracene	21.157	228	33526	0.487	ng/ul	100
22) Chrysene	21.207	228	33591	0.487	ng/ul	100
24) Benzo(b)fluoranthene	22.706	252	29835	0.511	ng/ul	99
25) Benzo(k)fluoranthene	22.747	252	29550	0.501	ng/ul	98
26) Benzo(a)pyrene	23.258	252	25072	0.498	ng/ul	98
27) Indeno(1,2,3-cd)pyrene	25.530	276	26223	0.490	ng/ul	99
28) Dibenzo(a,h)anthracene	25.547	278	19836	0.490	ng/ul	98
29) Benzo(g,h,i)perylene	26.184	276	20694	0.492	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034777.D
Acq On : 31 Oct 2024 21:54
Operator : RC/JU
Sample : PB164351BS
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLCS351

Quant Time: Nov 03 23:23:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration




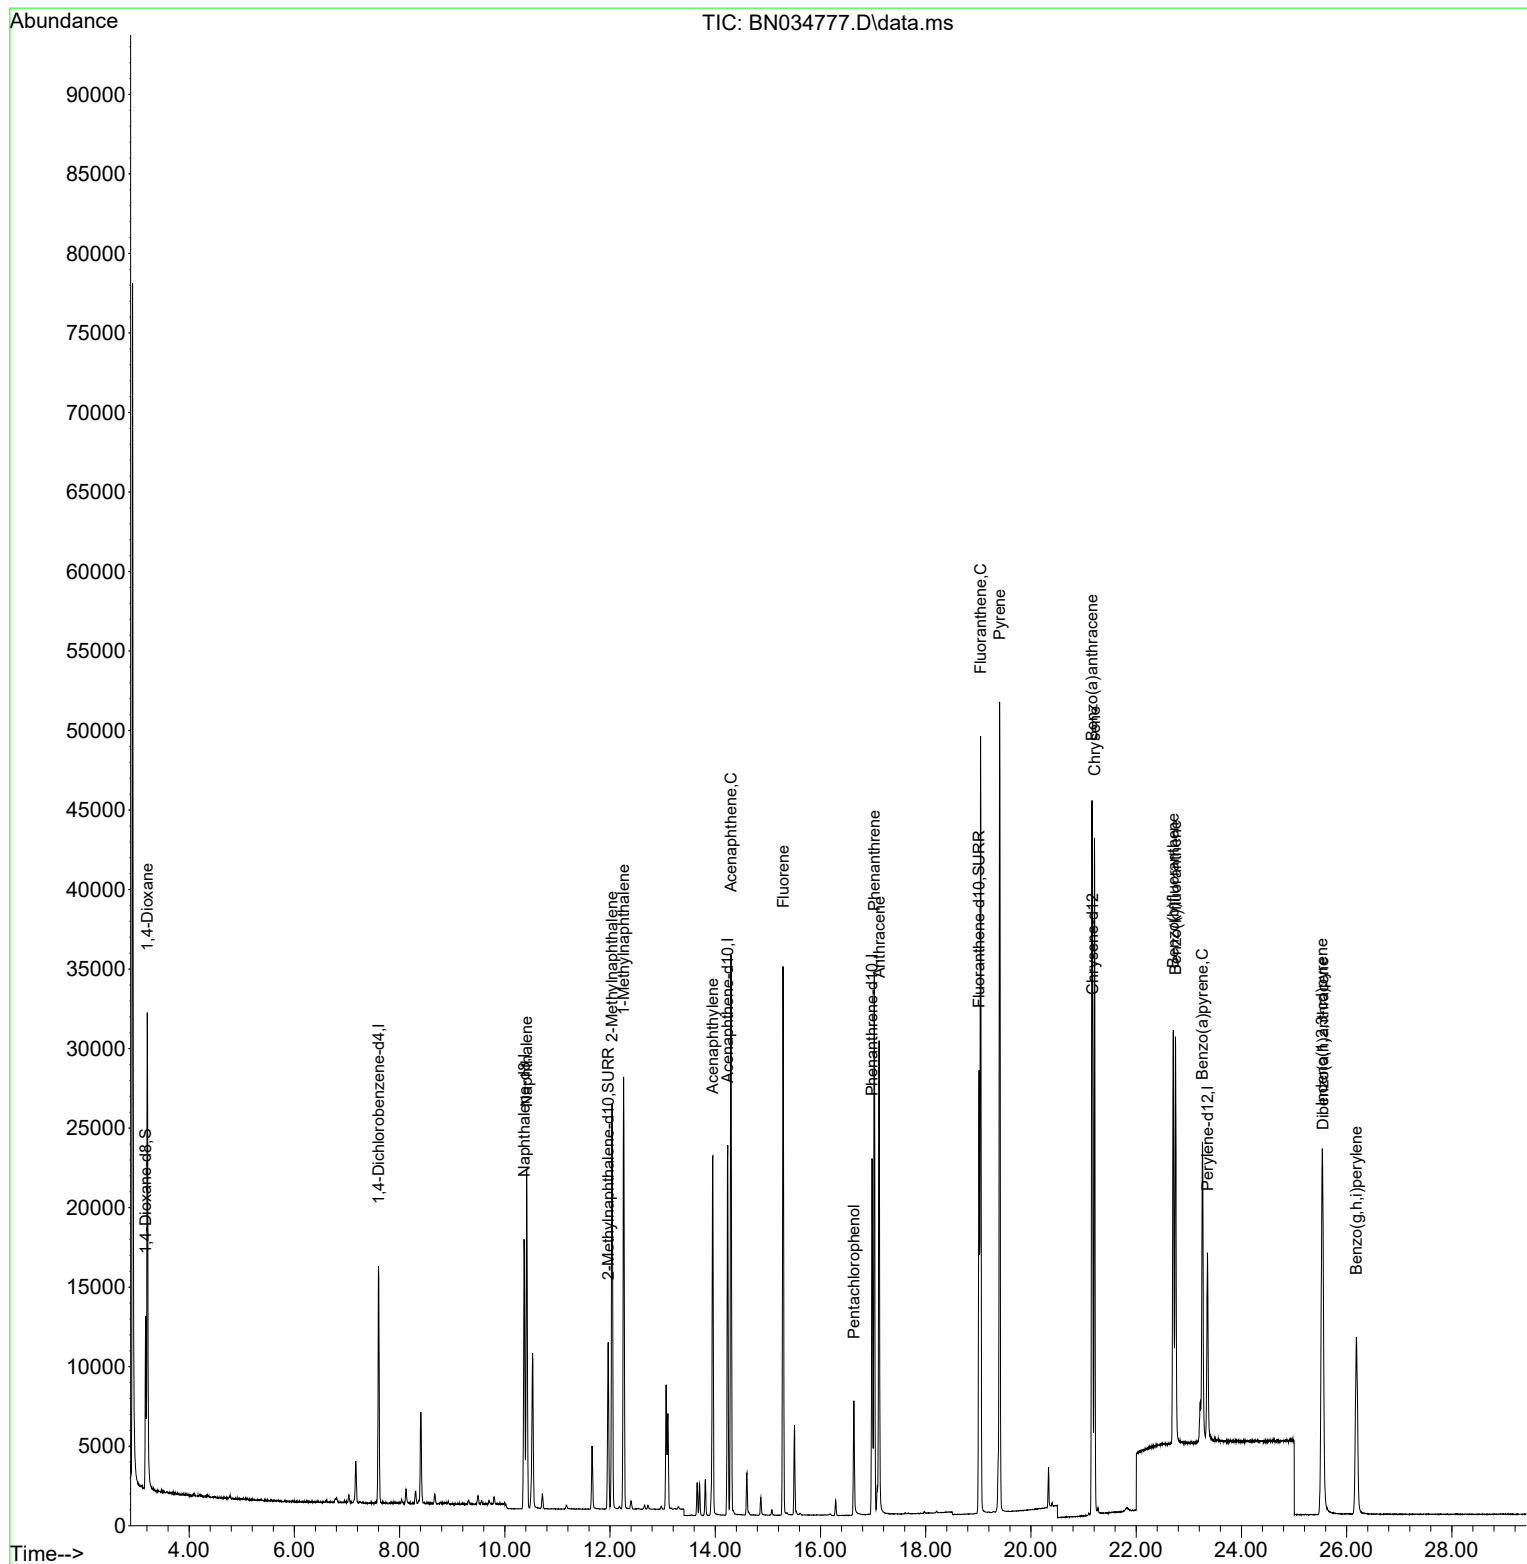


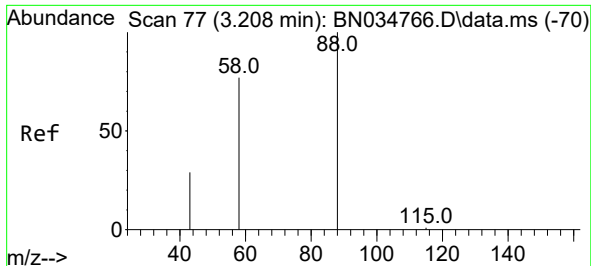

#2
1,4-Dioxane
Concen: 2.267 ng/ul
RT: 3.203 min Scan# 77
Delta R.T. -0.004 min
Lab File: BN034777.D
Acq: 31 Oct 2024 21:54




Instrument :
BNA_N
ClientSampleId :
SLCS351


Tgt Ion: 88 Resp: 18605
Ion Ratio Lower Upper
88 100
43 33.3 41.9 62.9#
58 78.8 57.5 86.3

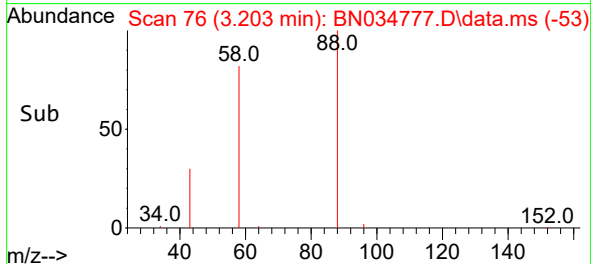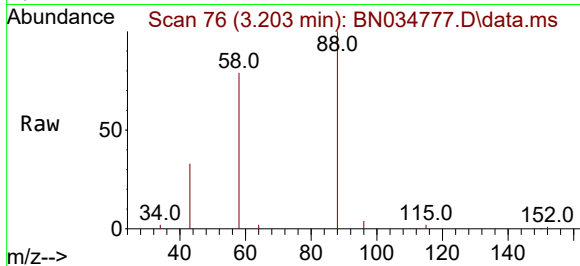

#5
Naphthalene
Concen: 0.476 ng/ul
RT: 10.416 min Scan# 1766
Delta R.T. -0.006 min
Lab File: BN034777.D
Acq: 31 Oct 2024 21:54

Tgt Ion:128 Resp: 27451
Ion Ratio Lower Upper
128 100
129 11.3 9.1 13.7
127 13.0 10.5 15.7


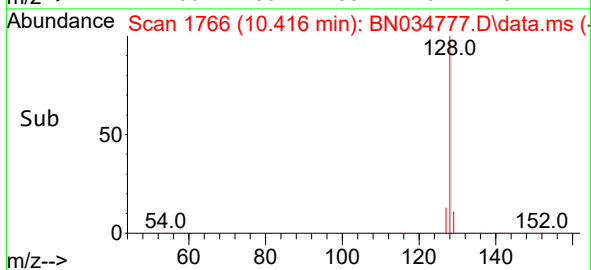

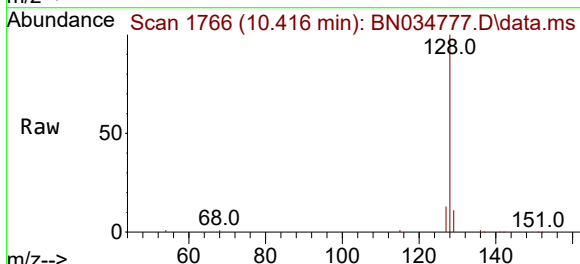




#7
2-Methylnaphthalene
Concen: 0.469 ng/ul
RT: 12.038 min Scan# 2061
Delta R.T. -0.006 min
Lab File: BN034777.D
Acq: 31 Oct 2024 21:54




Instrument :
BNA_N
ClientSampleId :
SLCS351


Tgt Ion:142 Resp: 17580
Ion Ratio Lower Upper
142 100
141 89.0 71.1 106.7

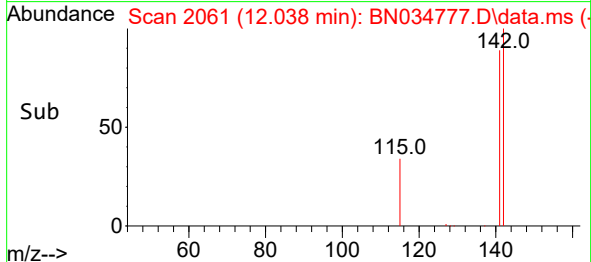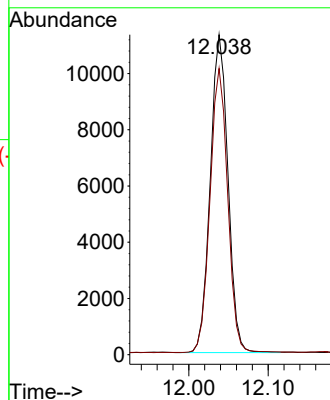

#8
1-Methylnaphthalene
Concen: 0.468 ng/ul
RT: 12.258 min Scan# 2101
Delta R.T. -0.006 min
Lab File: BN034777.D
Acq: 31 Oct 2024 21:54

Tgt Ion:142 Resp: 17875
Ion Ratio Lower Upper
142 100
141 92.2 73.6 110.4


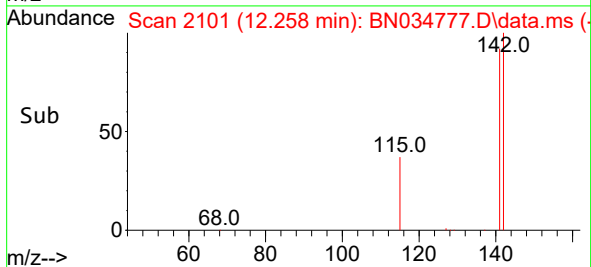
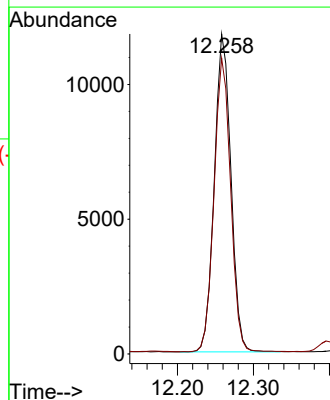
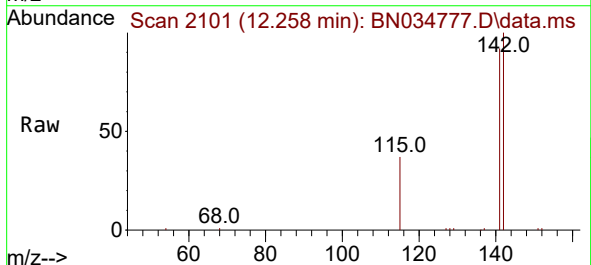




#10
Acenaphthylene
Concen: 0.470 ng/ul
RT: 13.953 min Scan# 2428
Delta R.T. -0.000 min
Lab File: BN034777.D
Acq: 31 Oct 2024 21:54




Instrument :
BNA_N
ClientSampleId :
SLCS351


Tgt Ion:152 Resp: 25583
Ion Ratio Lower Upper
152 100
151 19.6 16.0 24.0
153 13.1 10.7 16.1

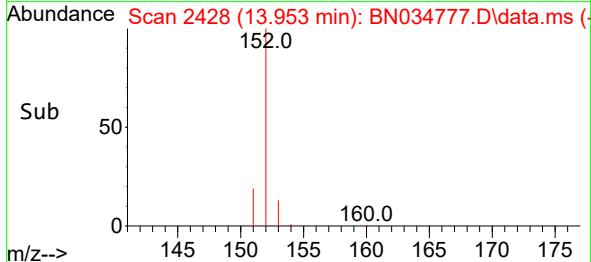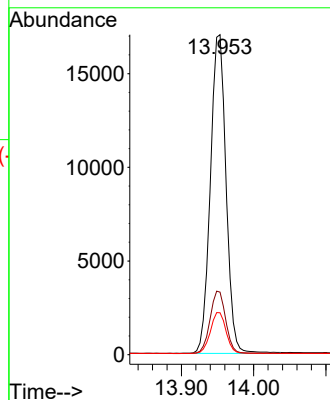

#11
Acenaphthene
Concen: 0.471 ng/ul
RT: 14.296 min Scan# 2502
Delta R.T. -0.005 min
Lab File: BN034777.D
Acq: 31 Oct 2024 21:54

Tgt Ion:153 Resp: 19604
Ion Ratio Lower Upper
153 100
152 51.6 40.3 60.5
154 87.4 69.9 104.9


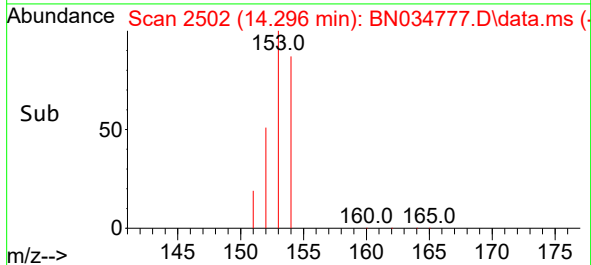
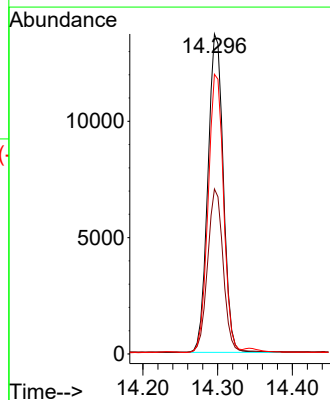
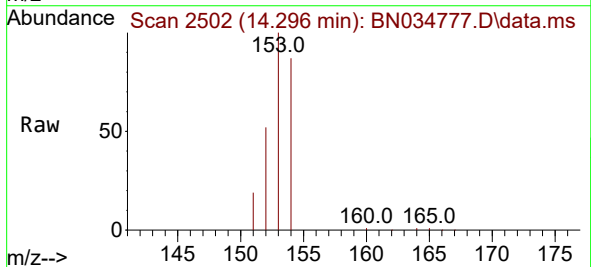




#12
Fluorene
Concen: 0.454 ng/ul
RT: 15.290 min Scan# 2717
Delta R.T. -0.000 min
Lab File: BN034777.D
Acq: 31 Oct 2024 21:54




Instrument :
BNA_N
ClientSampleId :
SLCS351


Tgt Ion:166 Resp: 21069
Ion Ratio Lower Upper
166 100
165 97.0 79.1 118.7
167 13.7 11.0 16.4

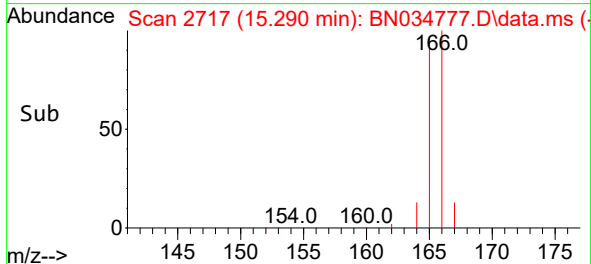

#14
Pentachlorophenol
Concen: 0.963 ng/ul
RT: 16.633 min Scan# 3016
Delta R.T. -0.004 min
Lab File: BN034777.D
Acq: 31 Oct 2024 21:54

Tgt Ion:266 Resp: 4661
Ion Ratio Lower Upper
266 100
264 62.5 50.1 75.1
268 64.0 52.0 78.0

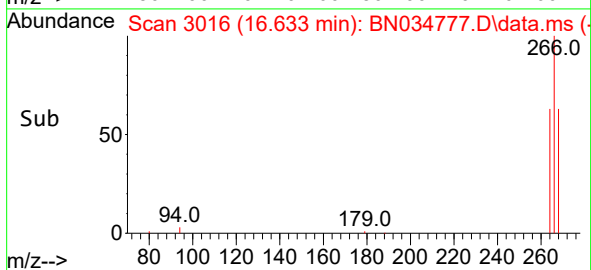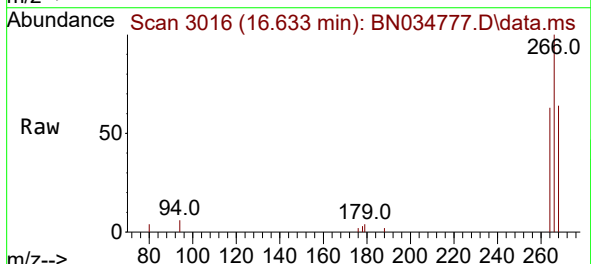



#15

Phenanthrene

Concen: 0.460 ng/ul

RT: 17.021 min Scan# 3108

Delta R.T. -0.004 min

Lab File: BN034777.D

Acq: 31 Oct 2024 21:54

Instrument :

BNA_N

ClientSampleId :

SLCS351





Tgt Ion:178 Resp: 34143

Ion Ratio Lower Upper

178 100

179 15.6 12.4 18.6

176 19.6 15.4 23.0

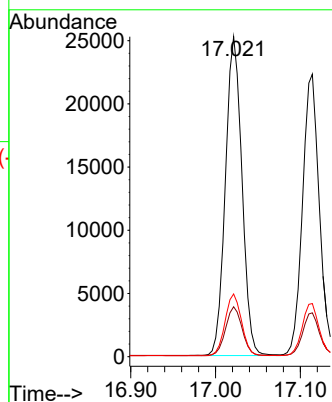

#16

Anthracene

Concen: 0.451 ng/ul

RT: 17.114 min Scan# 3130

Delta R.T. -0.000 min

Lab File: BN034777.D

Acq: 31 Oct 2024 21:54




Tgt Ion:178 Resp: 30952


Ion Ratio Lower Upper

178 100

179 15.5 12.3 18.5

176 18.8 15.1 22.7


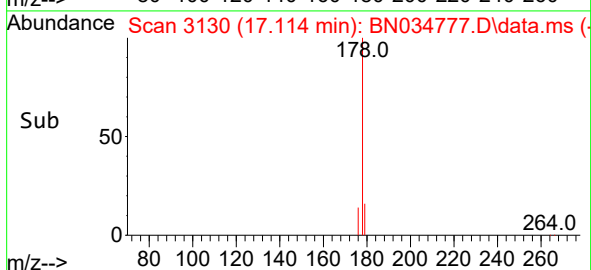






#19
Fluoranthene
Concen: 0.464 ng/ul
RT: 19.042 min Scan# 3575
Delta R.T. -0.005 min
Lab File: BN034777.D
Acq: 31 Oct 2024 21:54




Instrument :
BNA_N
ClientSampleId :
SLCS351


Tgt Ion:202 Resp: 38672
Ion Ratio Lower Upper
202 100
101 14.1 10.8 16.2
100 10.6 8.2 12.2

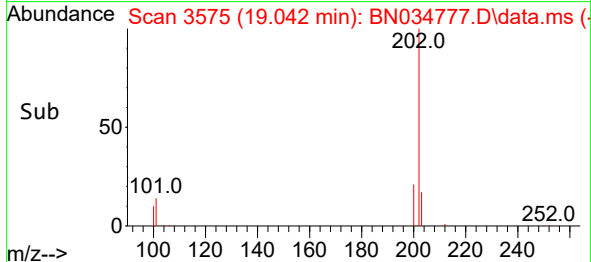

#20
Pyrene
Concen: 0.465 ng/ul
RT: 19.404 min Scan# 3653
Delta R.T. -0.005 min
Lab File: BN034777.D
Acq: 31 Oct 2024 21:54


Tgt Ion:202 Resp: 40401
Ion Ratio Lower Upper
202 100
101 16.7 12.4 18.6
100 13.7 10.0 15.0

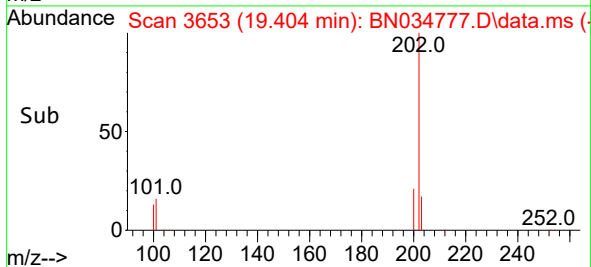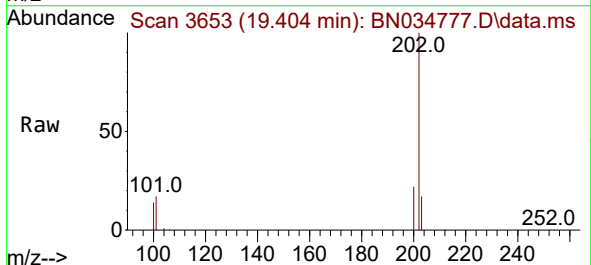






#21
Benzo(a)anthracene
Concen: 0.487 ng/ul
RT: 21.157 min Scan# 4113
Delta R.T. -0.003 min
Lab File: BN034777.D
Acq: 31 Oct 2024 21:54

Instrument :
BNA_N
ClientSampleId :
SLCS351







Tgt Ion:228 Resp: 33526
Ion Ratio Lower Upper
228 100
229 19.4 15.5 23.3
226 27.6 22.1 33.1

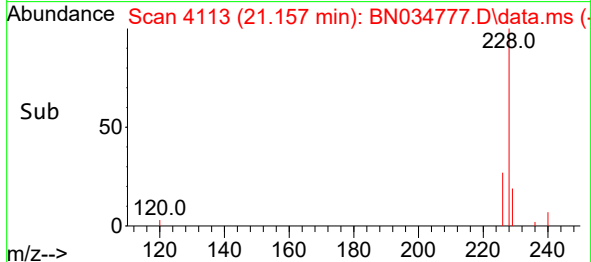

#22
Chrysene
Concen: 0.487 ng/ul
RT: 21.207 min Scan# 4130
Delta R.T. -0.006 min
Lab File: BN034777.D
Acq: 31 Oct 2024 21:54


Tgt Ion:228 Resp: 33591
Ion Ratio Lower Upper
228 100
226 30.8 24.3 36.5
229 19.4 15.6 23.4

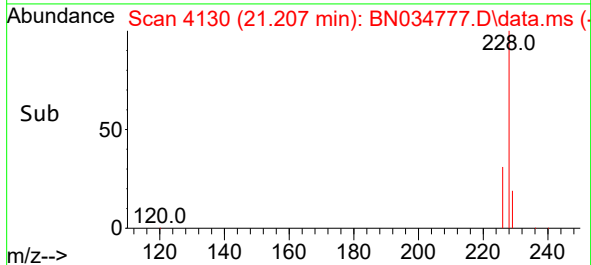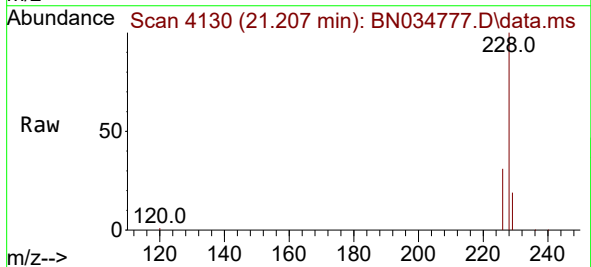





#24
Benzo(b)fluoranthene
Concen: 0.511 ng/ul
RT: 22.706 min Scan# 4643
Delta R.T. -0.003 min
Lab File: BN034777.D
Acq: 31 Oct 2024 21:54

Instrument :
BNA_N
ClientSampleId :
SLCS351







Tgt Ion:252 Resp: 29835
Ion Ratio Lower Upper
252 100
253 23.6 0.0 47.6
125 19.8 0.0 41.4



#25
Benzo(k)fluoranthene
Concen: 0.501 ng/ul
RT: 22.747 min Scan# 4657
Delta R.T. -0.003 min
Lab File: BN034777.D
Acq: 31 Oct 2024 21:54

Tgt Ion:252 Resp: 29550
Ion Ratio Lower Upper
252 100
253 23.5 19.1 28.7
125 19.9 17.0 25.4


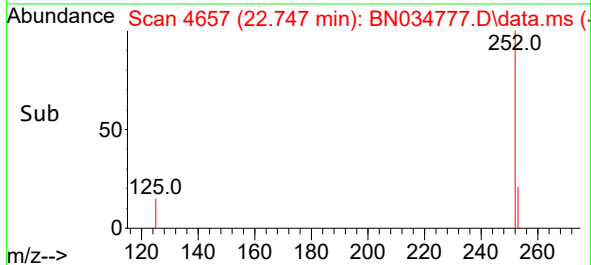

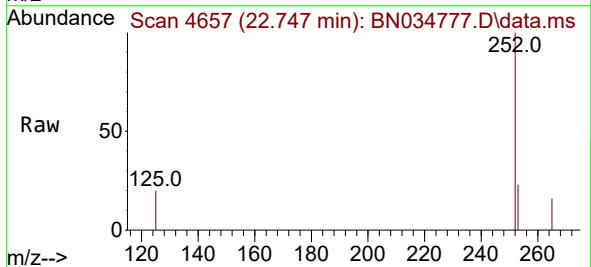




#26
Benzo(a)pyrene
Concen: 0.498 ng/ul
RT: 23.258 min Scan# 4832
Delta R.T. -0.006 min
Lab File: BN034777.D
Acq: 31 Oct 2024 21:54




Instrument :
BNA_N
ClientSampleId :
SLCS351


Tgt Ion:252 Resp: 25072
Ion Ratio Lower Upper
252 100
253 24.4 20.0 30.0
125 23.2 19.8 29.6

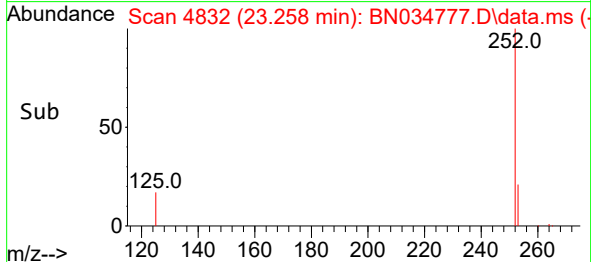

#27
Indeno(1,2,3-cd)pyrene
Concen: 0.490 ng/ul
RT: 25.530 min Scan# 5586
Delta R.T. -0.007 min
Lab File: BN034777.D
Acq: 31 Oct 2024 21:54

Tgt Ion:276 Resp: 26223
Ion Ratio Lower Upper
276 100
138 39.3 31.8 47.6
227 0.2 0.2 0.4


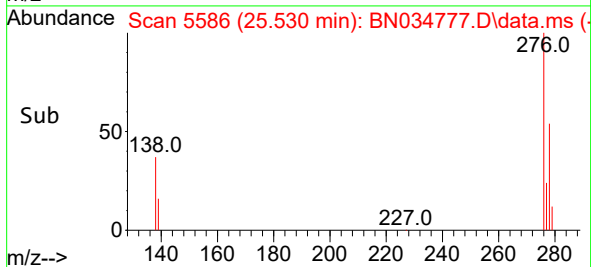

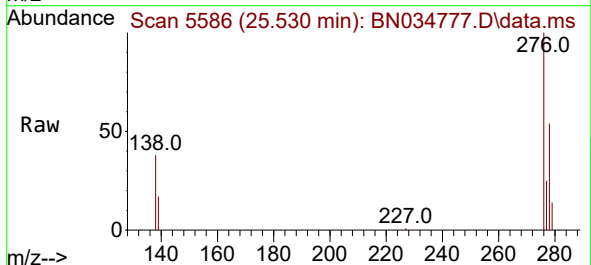




#28
Dibenzo(a,h)anthracene
Concen: 0.490 ng/ul
RT: 25.547 min Scan# 51
Delta R.T. -0.007 min
Lab File: BN034777.D
Acq: 31 Oct 2024 21:54

Instrument :
BNA_N
ClientSampleId :
SLCS351

Tgt Ion:278 Resp: 19836
Ion Ratio Lower Upper
278 100
139 27.7 23.4 35.2
279 25.5 20.6 31.0

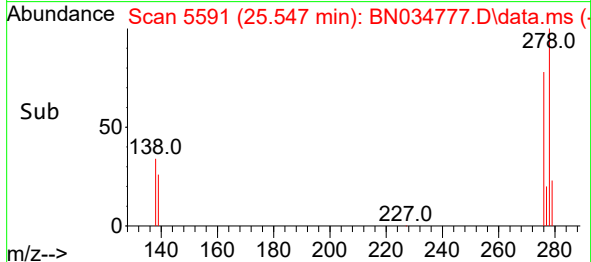

#29
Benzo(g,h,i)perylene
Concen: 0.492 ng/ul
RT: 26.184 min Scan# 5781
Delta R.T. -0.010 min
Lab File: BN034777.D
Acq: 31 Oct 2024 21:54

Tgt Ion:276 Resp: 20694
Ion Ratio Lower Upper
276 100
138 35.0 28.8 43.2
277 24.7 20.2 30.2

