

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
 Data File : BN034784.D
 Acq On : 01 Nov 2024 02:42
 Operator : RC/JU
 Sample : PB164351BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK351

Quant Time: Nov 03 23:24:26 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 11:13:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.600	152	7612	0.400	ng/ul	0.00
4) Naphthalene-d8	10.366	136	24584	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.236	164	13812	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-16.98
17) Chrysene-d12	21.172	240	17916	0.400	ng/ul	0.00
23) Perylene-d12	23.220	264	850920	0.400	ng/ul	#-0.14
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.170	96	41667	5.288	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.961	152	9603	0.312	ng/ul	0.00
18) Fluoranthene-d10	19.009	212	18288	0.314	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.376	202	2503	0.028	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034784.D
Acq On : 01 Nov 2024 02:42
Operator : RC/JU
Sample : PB164351BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK351


Quant Time: Nov 03 23:24:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

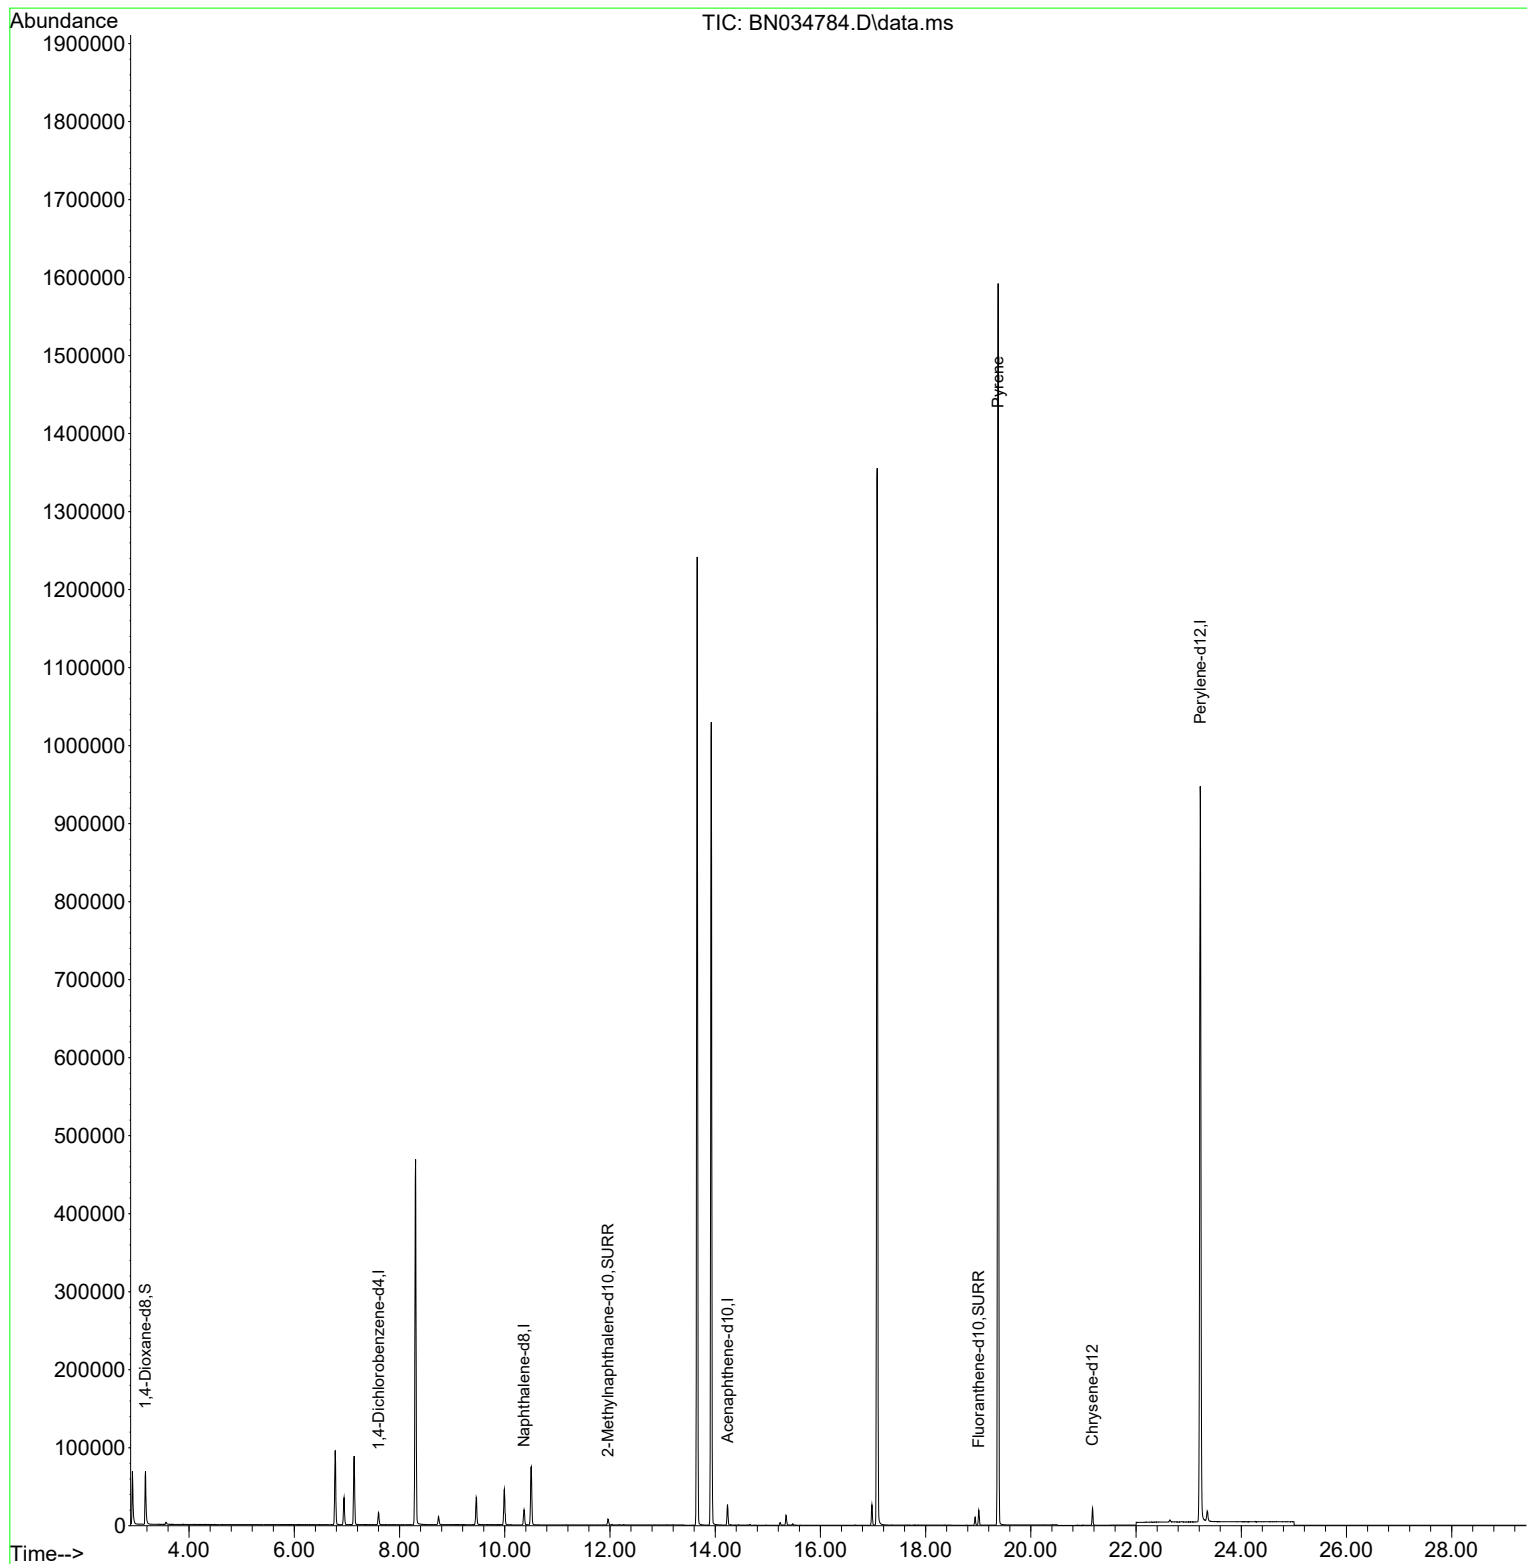

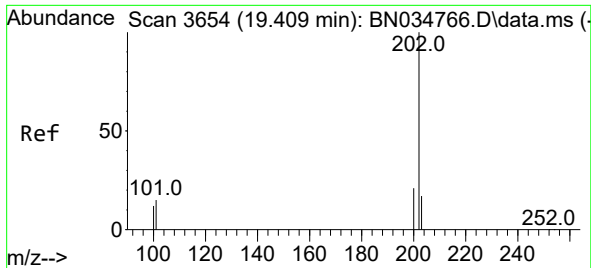

#20
 Pyrene
 Concen: 0.028 ng/ul
 RT: 19.376 min Scan# 30
 Delta R.T. -0.033 min
 Lab File: BN034784.D
 Acq: 01 Nov 2024 02:42

Instrument :
 BNA_N
 ClientSampleId :
 SBLK351

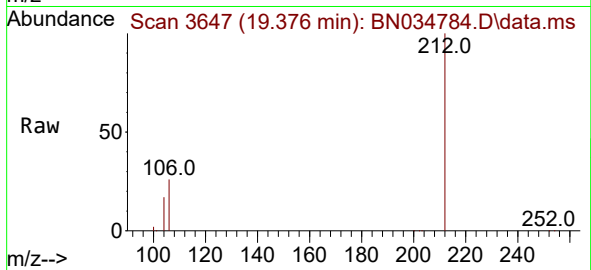

Tgt Ion:202 Resp: 2503
 Ion Ratio Lower Upper
 202 100
 101 190.2 12.4 18.6#
 100 1402.1 10.0 15.0#

