

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
 Data File : BN034790.D
 Acq On : 01 Nov 2024 06:19
 Operator : RC/JU
 Sample : P4529-12
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F7H22

Quant Time: Nov 03 23:25:11 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 11:13:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.600	152	7847	0.400	ng/ul	0.00
4) Naphthalene-d8	10.366	136	25146	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.235	164	14390	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.979	188	29038	0.400	ng/ul	0.00
17) Chrysene-d12	21.174	240	20095	0.400	ng/ul	0.00
23) Perylene-d12	23.220	264	658698	0.400	ng/ul	#-0.14
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.169	96	33029	4.066	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.961	152	8635	0.274	ng/ul	0.00
18) Fluoranthene-d10	19.009	212	17848	0.273	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.235	166	2642	0.047	ng/ul#	13
20) Pyrene	19.376	202	2392	0.024	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034790.D
Acq On : 01 Nov 2024 06:19
Operator : RC/JU
Sample : P4529-12
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F7H22

Quant Time: Nov 03 23:25:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

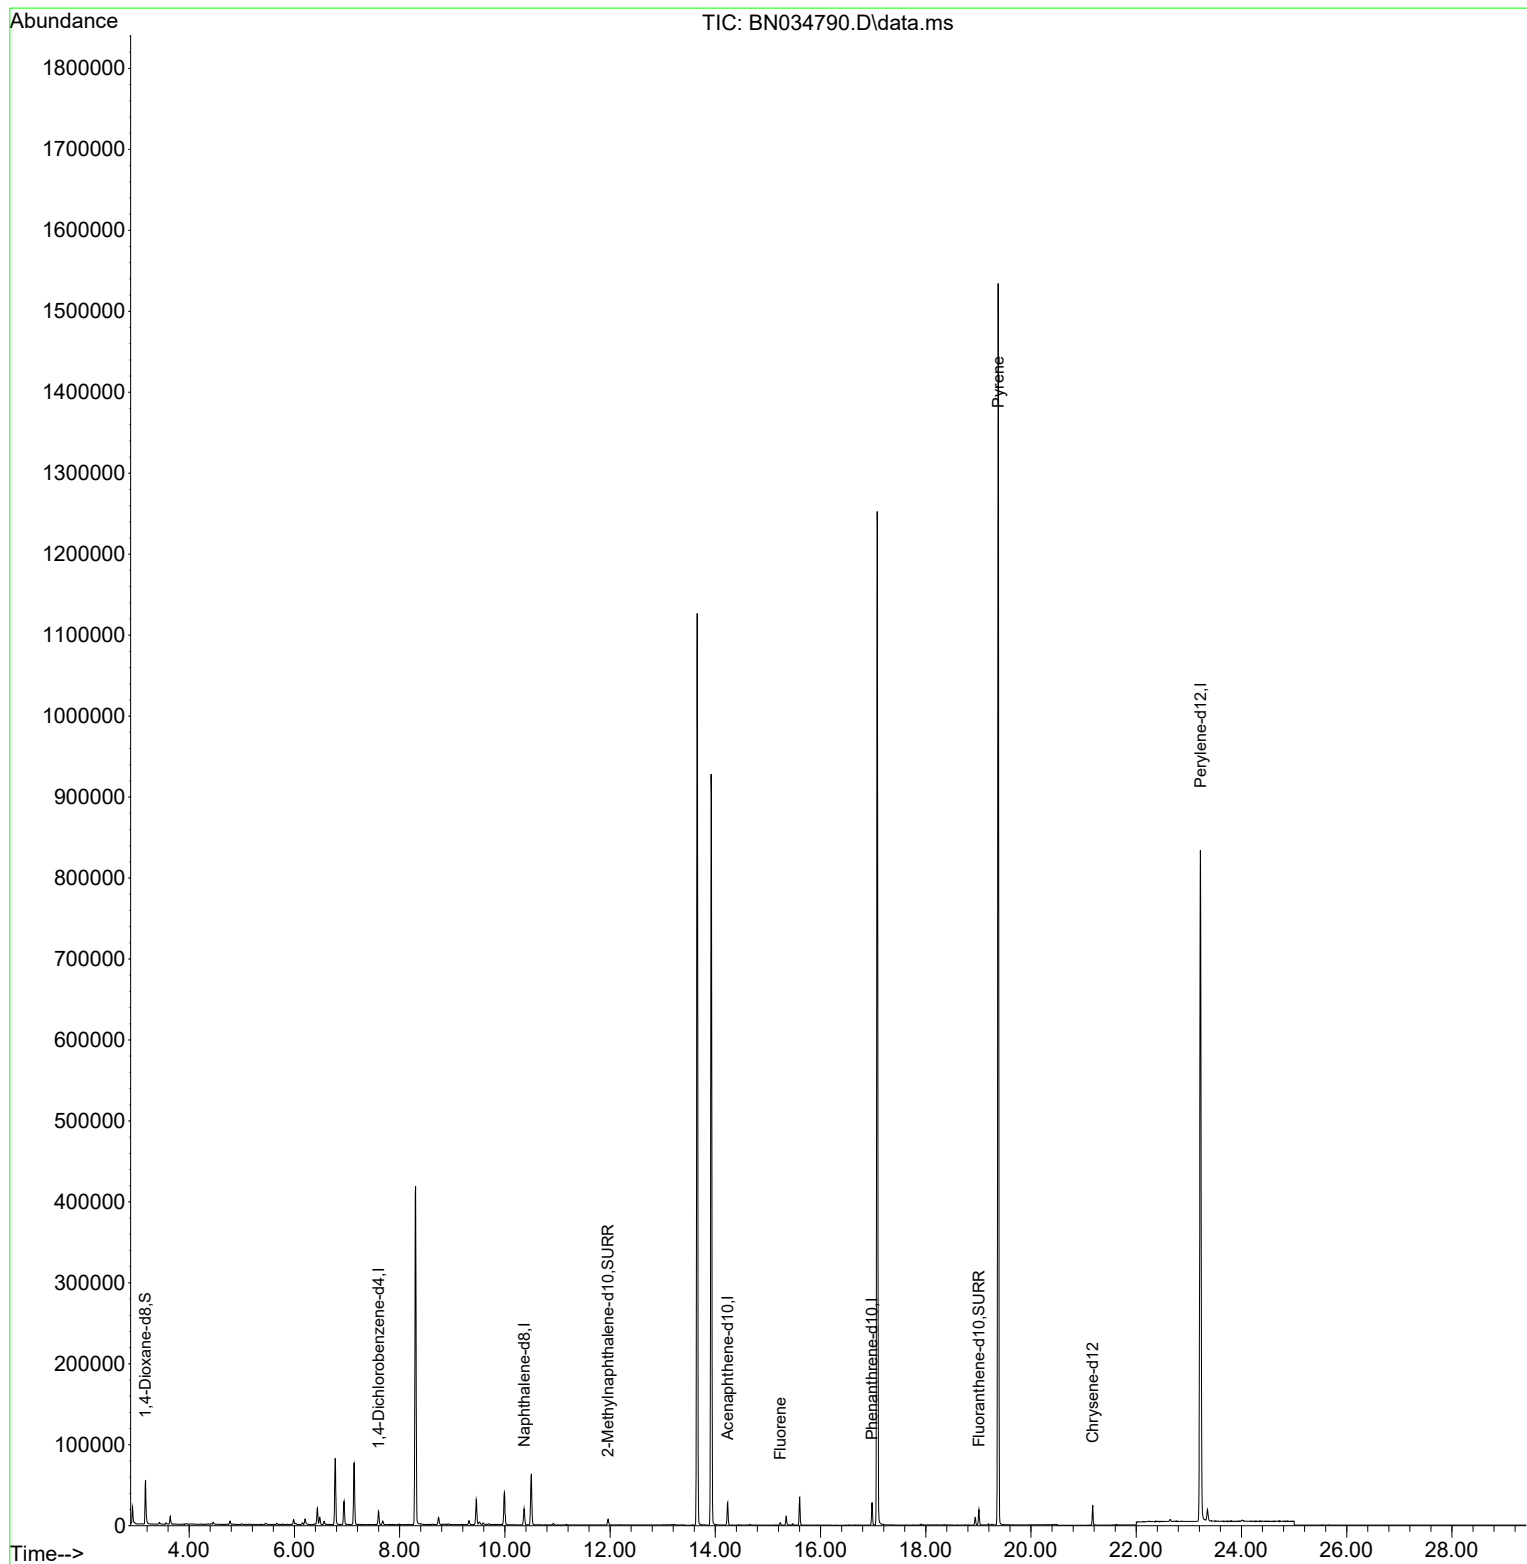

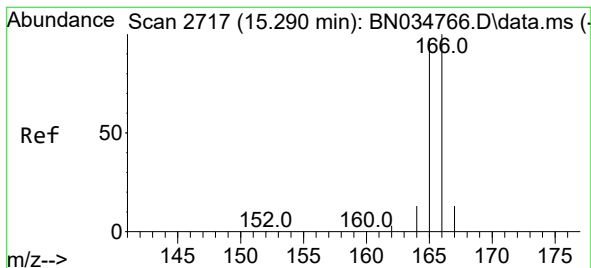

#12

Fluorene

Concen: 0.047 ng/ul

RT: 15.235 min Scan# 21

Delta R.T. -0.056 min

Lab File: BN034790.D

Acq: 01 Nov 2024 06:19

Instrument :

BNA_N

ClientSampleId :

F7H22





Tgt Ion:166 Resp: 2642

Ion Ratio Lower Upper

166 100

165 8.2 79.1 118.7#

167 35.3 11.0 16.4#

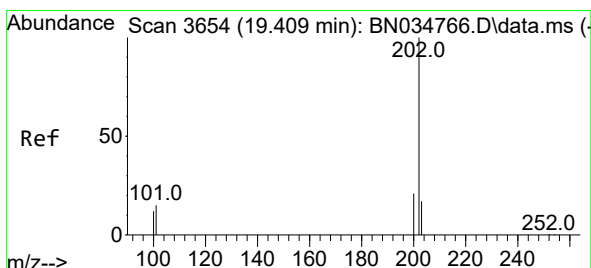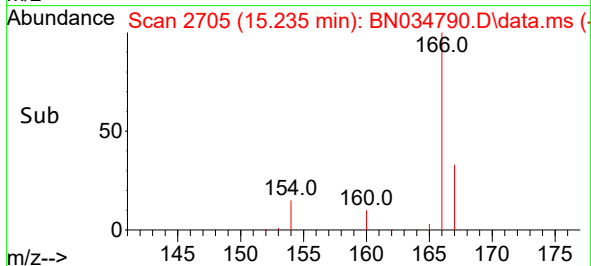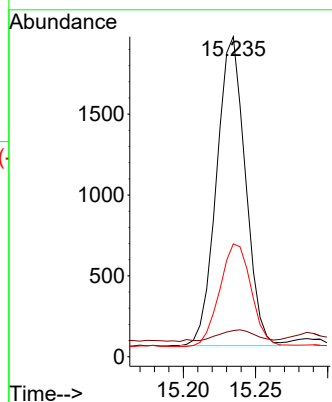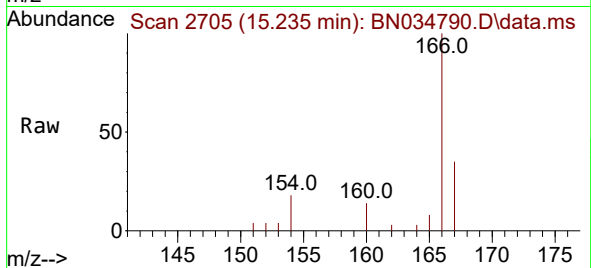

#20

Pyrene

Concen: 0.024 ng/ul

RT: 19.376 min Scan# 3647

Delta R.T. -0.033 min

Lab File: BN034790.D

Acq: 01 Nov 2024 06:19

Tgt Ion:202 Resp: 2392

Ion Ratio Lower Upper

202 100

101 189.6 12.4 18.6#

100 1402.0 10.0 15.0#

