

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
 Data File : BN034802.D
 Acq On : 01 Nov 2024 13:33
 Operator : RC/JU
 Sample : PB164483BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK483

Quant Time: Nov 03 23:26:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 11:13:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.600	152	6475	0.400	ng/ul	0.00
4) Naphthalene-d8	10.367	136	20403	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.231	164	11288	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-16.98
17) Chrysene-d12	21.169	240	14676	0.400	ng/ul	0.00
23) Perylene-d12	23.215	264	881617	0.400	ng/ul	#-0.14
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.170	96	47049	7.019	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.961	152	10500	0.410	ng/ul	0.00
18) Fluoranthene-d10	19.009	212	20427	0.428	ng/ul	0.00
Target Compounds						
						Qvalue
12) Fluorene	15.230	166	3060	0.070	ng/ul#	13
20) Pyrene	19.377	202	2914	0.039	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
 Data File : BN034802.D
 Acq On : 01 Nov 2024 13:33
 Operator : RC/JU
 Sample : PB164483BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK483

Quant Time: Nov 03 23:26:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 11:13:08 2024
 Response via : Initial Calibration

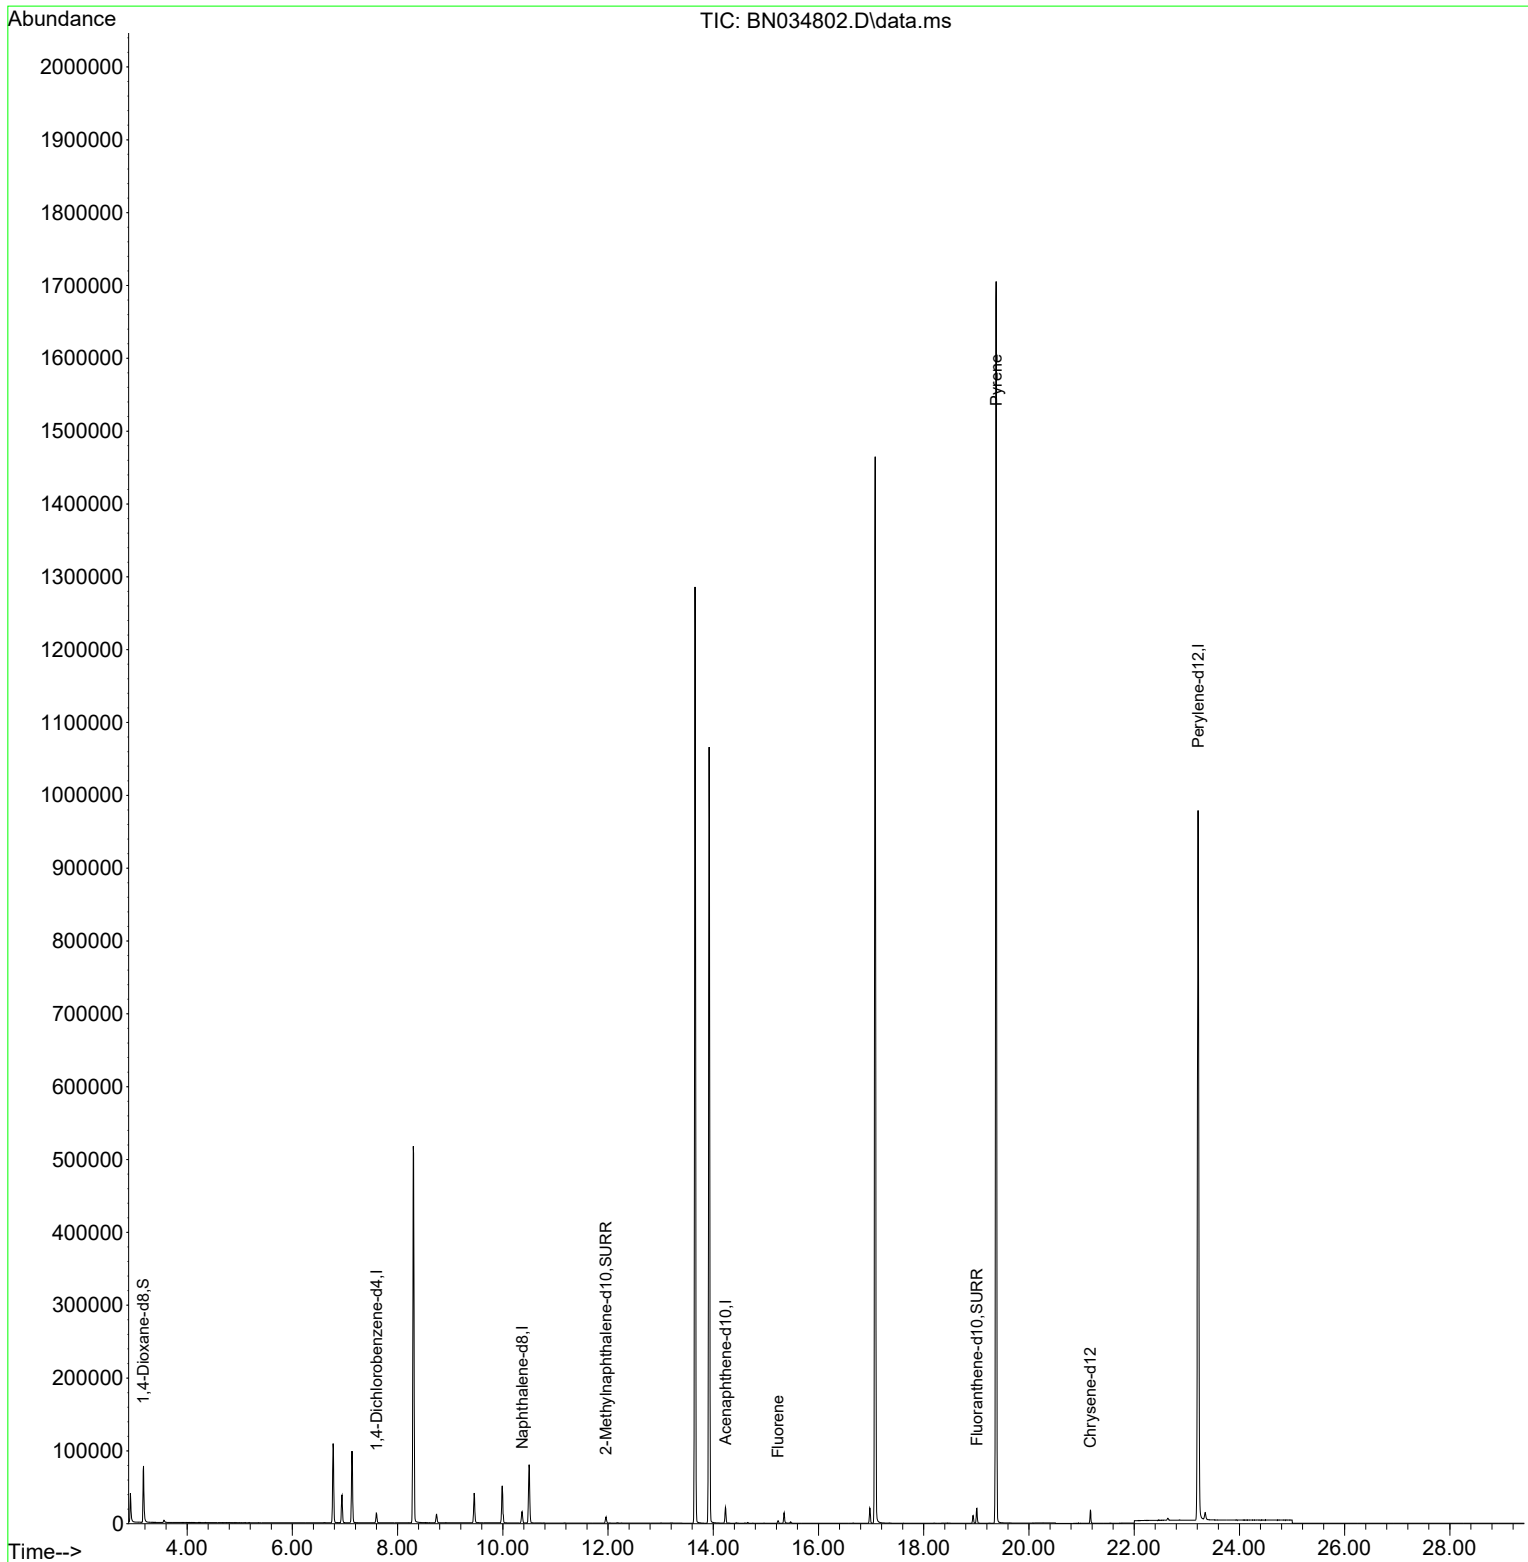




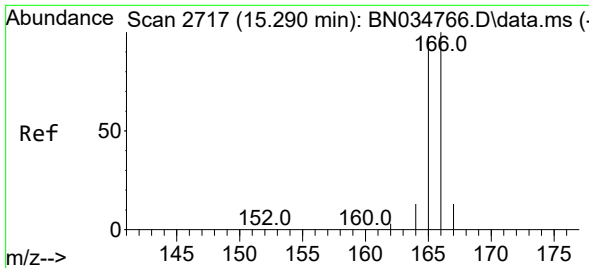


#12
 Fluorene
 Concen: 0.070 ng/u1
 RT: 15.230 min Scan# 21
 Delta R.T. -0.060 min
 Lab File: BN034802.D
 Acq: 01 Nov 2024 13:33

Instrument :
 BNA_N
 ClientSampleId :
 SBLK483

Tgt Ion:166 Resp: 3060

Ion	Ratio	Lower	Upper
166	100		
165	7.2	79.1	118.7#
167	33.5	11.0	16.4#

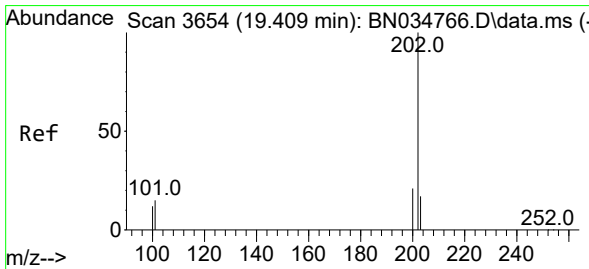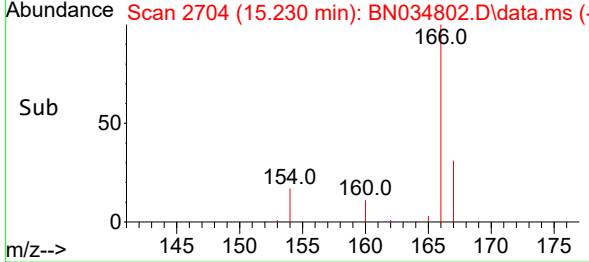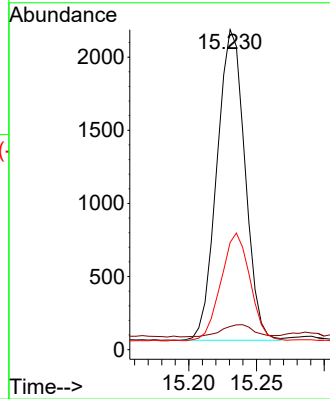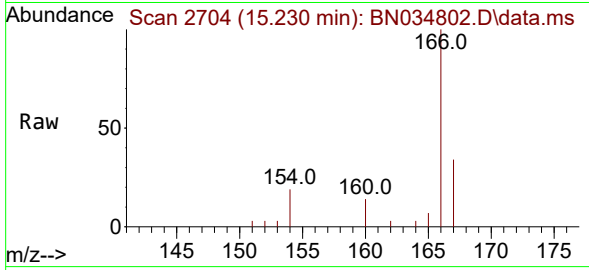

#20
 Pyrene
 Concen: 0.039 ng/u1
 RT: 19.377 min Scan# 3647
 Delta R.T. -0.032 min
 Lab File: BN034802.D
 Acq: 01 Nov 2024 13:33

Tgt Ion:202 Resp: 2914

Ion	Ratio	Lower	Upper
202	100		
101	186.5	12.4	18.6#
100	1333.3	10.0	15.0#

