

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
 Data File : BN034803.D
 Acq On : 01 Nov 2024 14:10
 Operator : RC/JU
 Sample : P4530-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F7H49

Quant Time: Nov 03 23:26:47 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 11:13:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.600	152	6293	0.400	ng/ul	0.00
4) Naphthalene-d8	10.366	136	19648	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.231	164	11003	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-16.98
17) Chrysene-d12	21.169	240	14808	0.400	ng/ul	0.00
23) Perylene-d12	23.217	264	1007279	0.400	ng/ul	#-0.14
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.170	96	34490	5.295	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.961	152	10006	0.406	ng/ul	0.00
18) Fluoranthene-d10	19.009	212	24153	0.501	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.416	128	1980	0.038	ng/ul#	88
20) Pyrene	19.376	202	3818	0.051	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034803.D
Acq On : 01 Nov 2024 14:10
Operator : RC/JU
Sample : P4530-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F7H49

Quant Time: Nov 03 23:26:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration




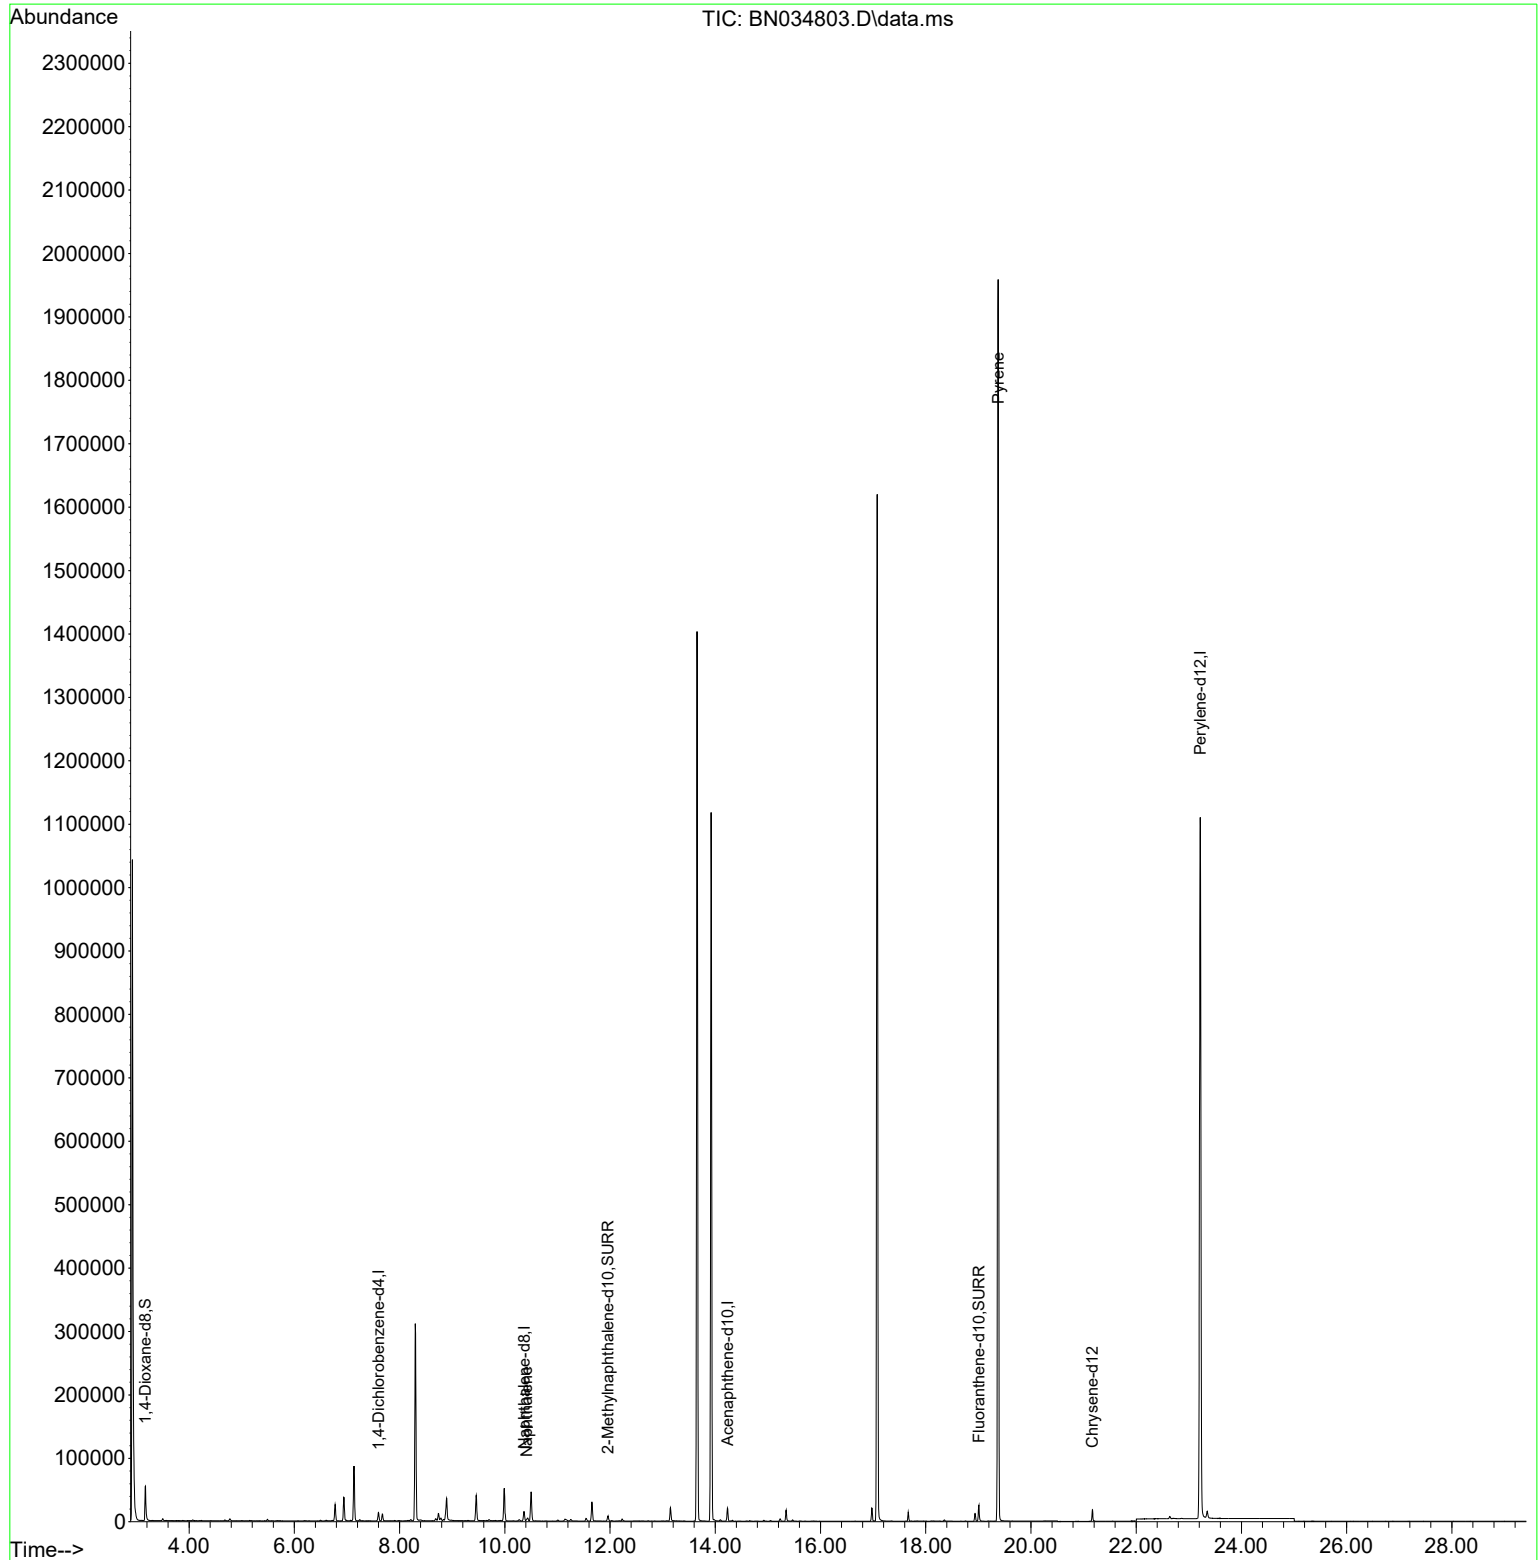


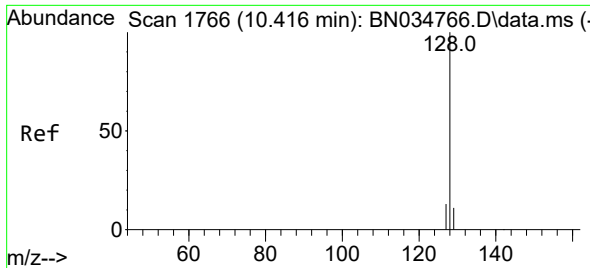

#5
Naphthalene
Concen: 0.038 ng/ul
RT: 10.416 min Scan# 1766
Delta R.T. -0.006 min
Lab File: BN034803.D
Acq: 01 Nov 2024 14:10

Instrument :
BNA_N
ClientSampleId :
F7H49

Tgt Ion:128 Resp: 1980
Ion Ratio Lower Upper
128 100
129 17.5 9.1 13.7#
127 16.3 10.5 15.7#

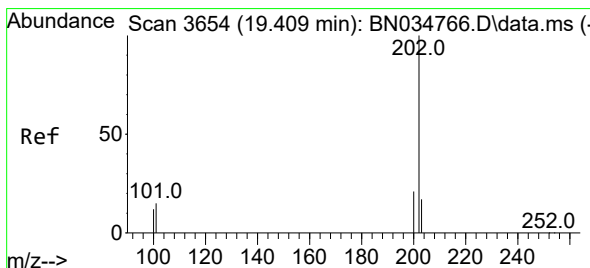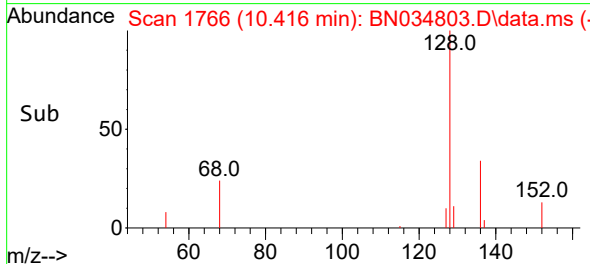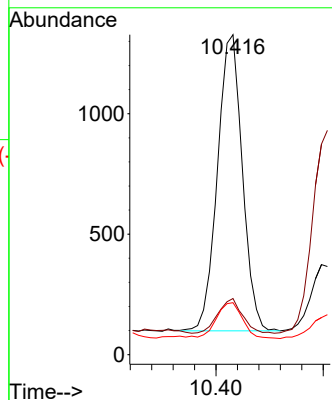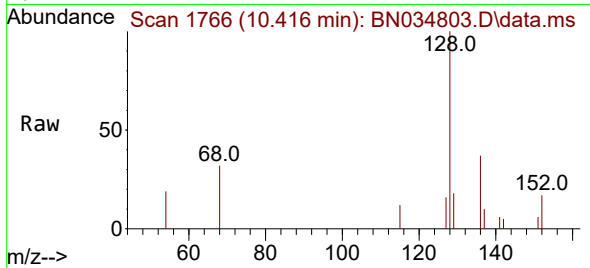

#20
Pyrene
Concen: 0.051 ng/ul
RT: 19.376 min Scan# 3647
Delta R.T. -0.033 min
Lab File: BN034803.D
Acq: 01 Nov 2024 14:10

Tgt Ion:202 Resp: 3818
Ion Ratio Lower Upper
202 100
101 186.7 12.4 18.6#
100 1331.4 10.0 15.0#

