

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
 Data File : BN034807.D
 Acq On : 01 Nov 2024 16:35
 Operator : RC/JU
 Sample : P4534-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1LB3

Quant Time: Nov 03 23:27:11 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 11:13:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.596	152	6169	0.400	ng/ul	0.00
4) Naphthalene-d8	10.361	136	19065	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.231	164	10602	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-16.98
17) Chrysene-d12	21.169	240	15563	0.400	ng/ul	0.00
23) Perylene-d12	23.220	264	1081838	0.400	ng/ul	#-0.14
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.170	96	30391	4.759	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.961	152	8767	0.367	ng/ul	0.00
18) Fluoranthene-d10	19.009	212	23225	0.459	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.376	202	3652	0.046	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034807.D
Acq On : 01 Nov 2024 16:35
Operator : RC/JU
Sample : P4534-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1LB3


Quant Time: Nov 03 23:27:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

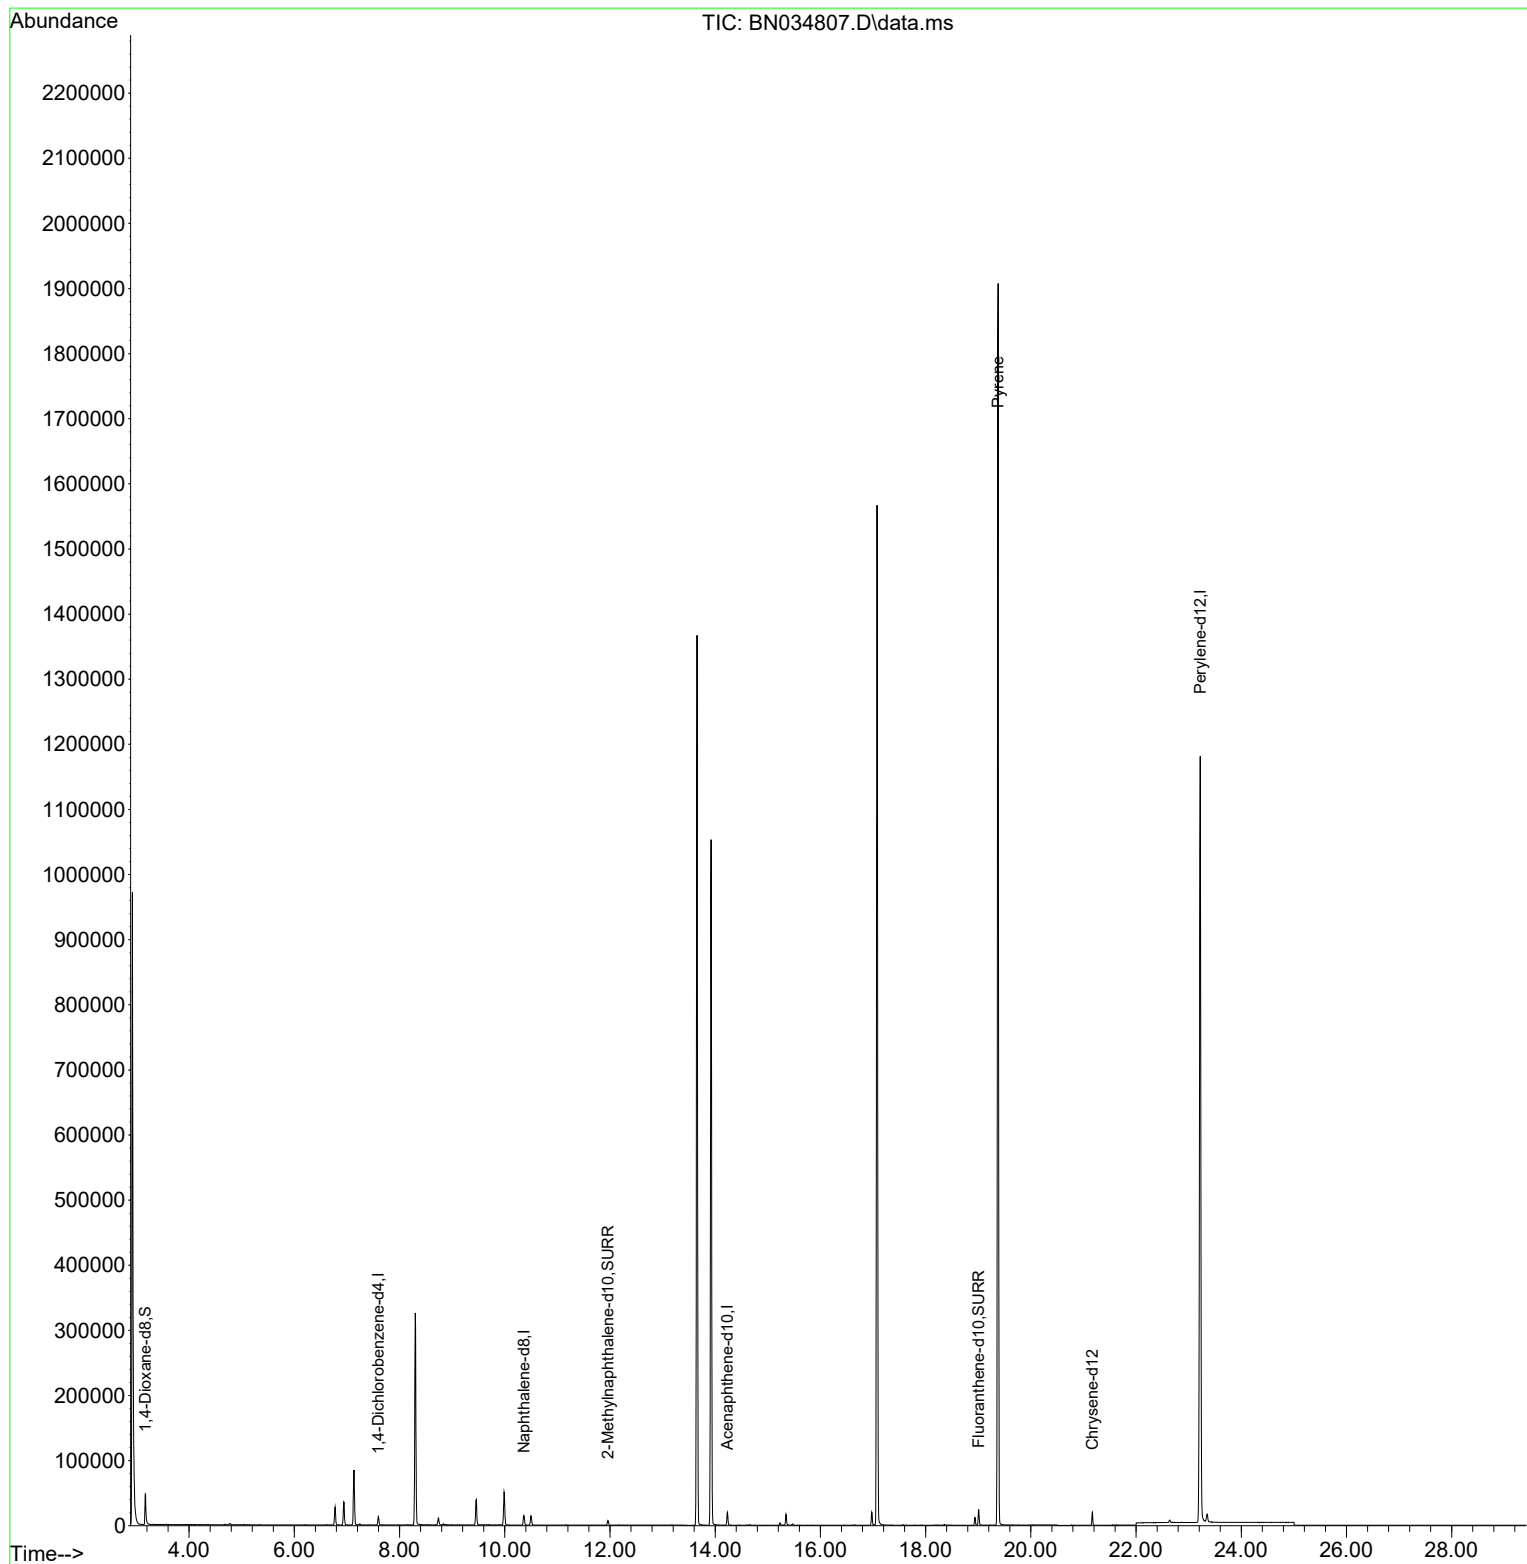

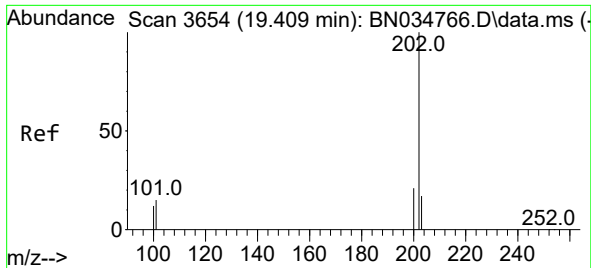

#20
 Pyrene
 Concen: 0.046 ng/ul
 RT: 19.376 min Scan# 30
 Delta R.T. -0.033 min
 Lab File: BN034807.D
 Acq: 01 Nov 2024 16:35

Instrument :
 BNA_N
 ClientSampleId :
 E1LB3

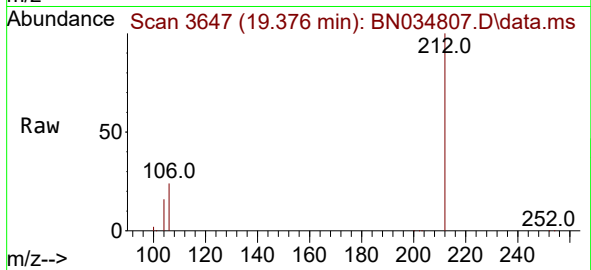

Tgt Ion:202 Resp: 3652
 Ion Ratio Lower Upper
 202 100
 101 185.3 12.4 18.6#
 100 1320.1 10.0 15.0#

