

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
 Data File : BN034809.D
 Acq On : 01 Nov 2024 17:48
 Operator : RC/JU
 Sample : P4534-17
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1L64

Quant Time: Nov 03 23:27:23 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 11:13:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.596	152	7481	0.400	ng/ul	0.00
4) Naphthalene-d8	10.361	136	22989	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.231	164	12870	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-16.98
17) Chrysene-d12	21.172	240	19471	0.400	ng/ul	0.00
23) Perylene-d12	23.223	264	1036091	0.400	ng/ul	#-0.13
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.170	96	32760	4.230	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.961	152	9886	0.343	ng/ul	0.00
18) Fluoranthene-d10	19.009	212	22937	0.362	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.203	88	469	0.055	ng/ul#	68
20) Pyrene	19.376	202	3030	0.031	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034809.D
Acq On : 01 Nov 2024 17:48
Operator : RC/JU
Sample : P4534-17
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1L64

Quant Time: Nov 03 23:27:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

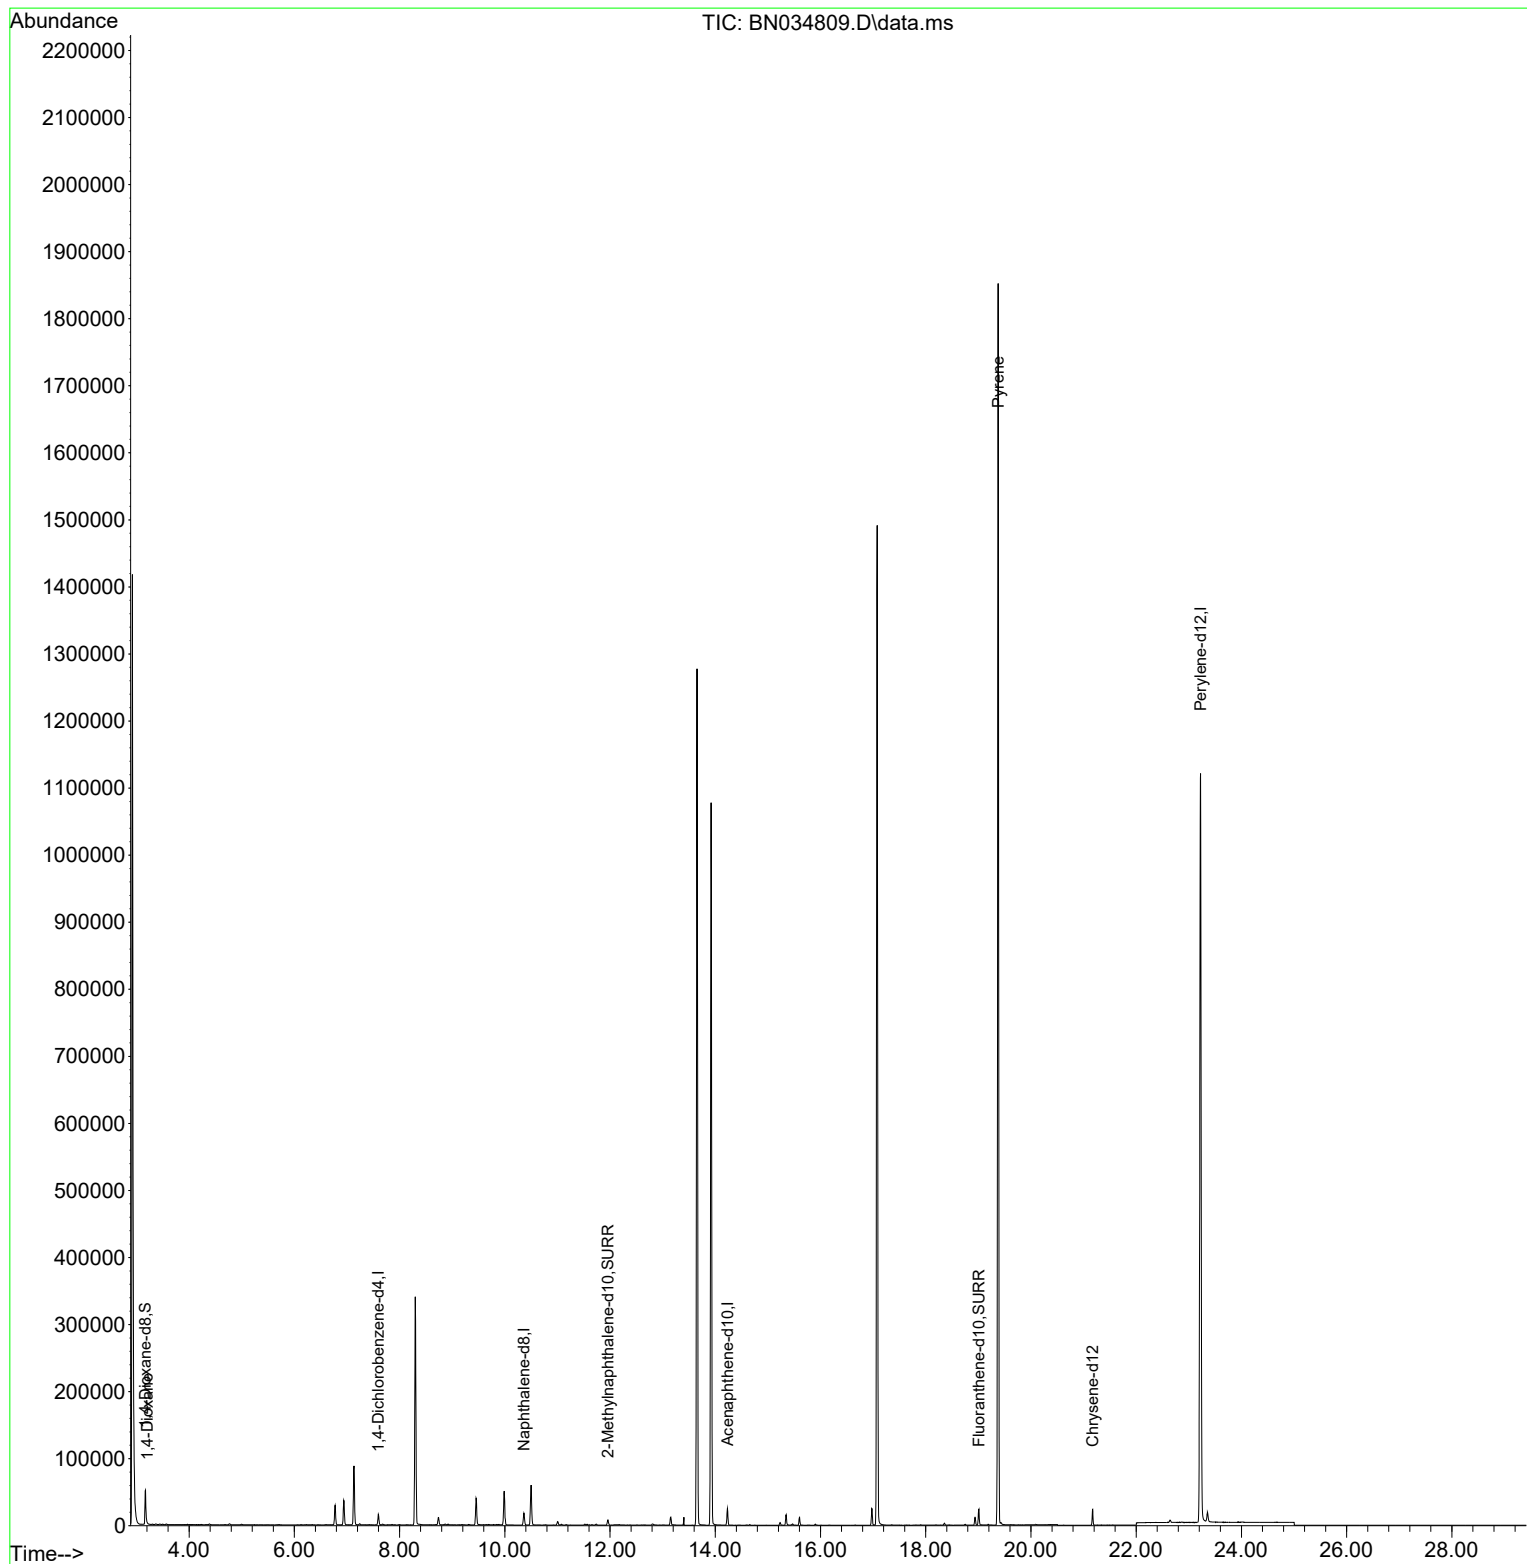

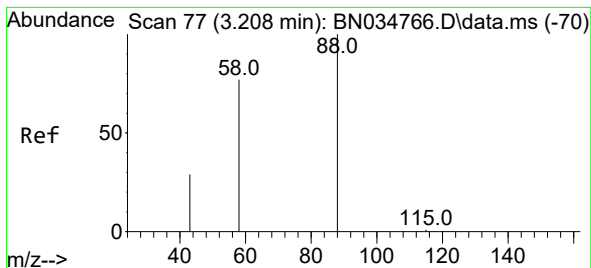

#2

1,4-Dioxane

Concen: 0.055 ng/ul

RT: 3.203 min Scan# 7

Delta R.T. -0.004 min

Lab File: BN034809.D

Acq: 01 Nov 2024 17:48

Instrument :

BNA_N

ClientSampleId :

E1L64





Tgt Ion: 88 Resp: 469

Ion Ratio Lower Upper

88 100

43 69.3 41.9 62.9#

58 41.0 57.5 86.3#

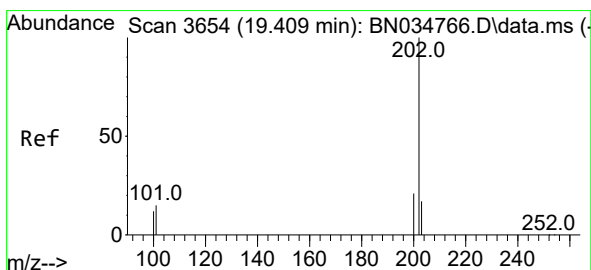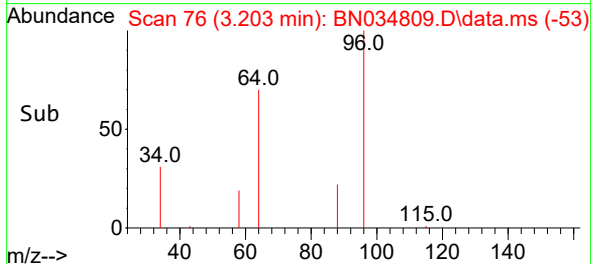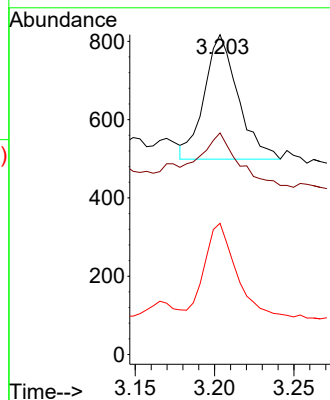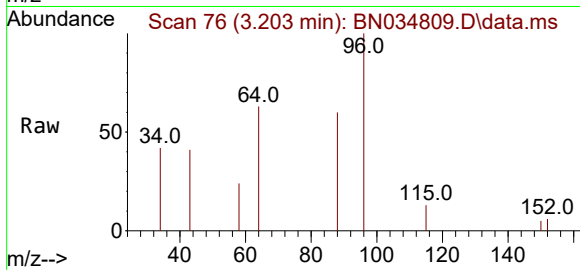

#20

Pyrene

Concen: 0.031 ng/ul

RT: 19.376 min Scan# 3647

Delta R.T. -0.033 min

Lab File: BN034809.D

Acq: 01 Nov 2024 17:48

Tgt Ion: 202 Resp: 3030

Ion Ratio Lower Upper

202 100

101 188.6 12.4 18.6#

100 1316.3 10.0 15.0#

