

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
 Data File : BN034811.D
 Acq On : 01 Nov 2024 19:00
 Operator : RC/JU
 Sample : P4558-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1L79

Quant Time: Nov 03 23:27:35 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 11:13:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.596	152	6663	0.400	ng/ul	0.00
4) Naphthalene-d8	10.361	136	20459	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.231	164	11747	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-16.98
17) Chrysene-d12	21.169	240	17618	0.400	ng/ul	0.00
23) Perylene-d12	23.220	264	1301791	0.400	ng/ul	#-0.14
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.165	96	29278	4.245	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.961	152	10993	0.429	ng/ul	0.00
18) Fluoranthene-d10	19.009	212	26778	0.467	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.230	166	3464	0.076	ng/ul#	17
20) Pyrene	19.376	202	3342	0.038	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034811.D
Acq On : 01 Nov 2024 19:00
Operator : RC/JU
Sample : P4558-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1L79

Quant Time: Nov 03 23:27:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

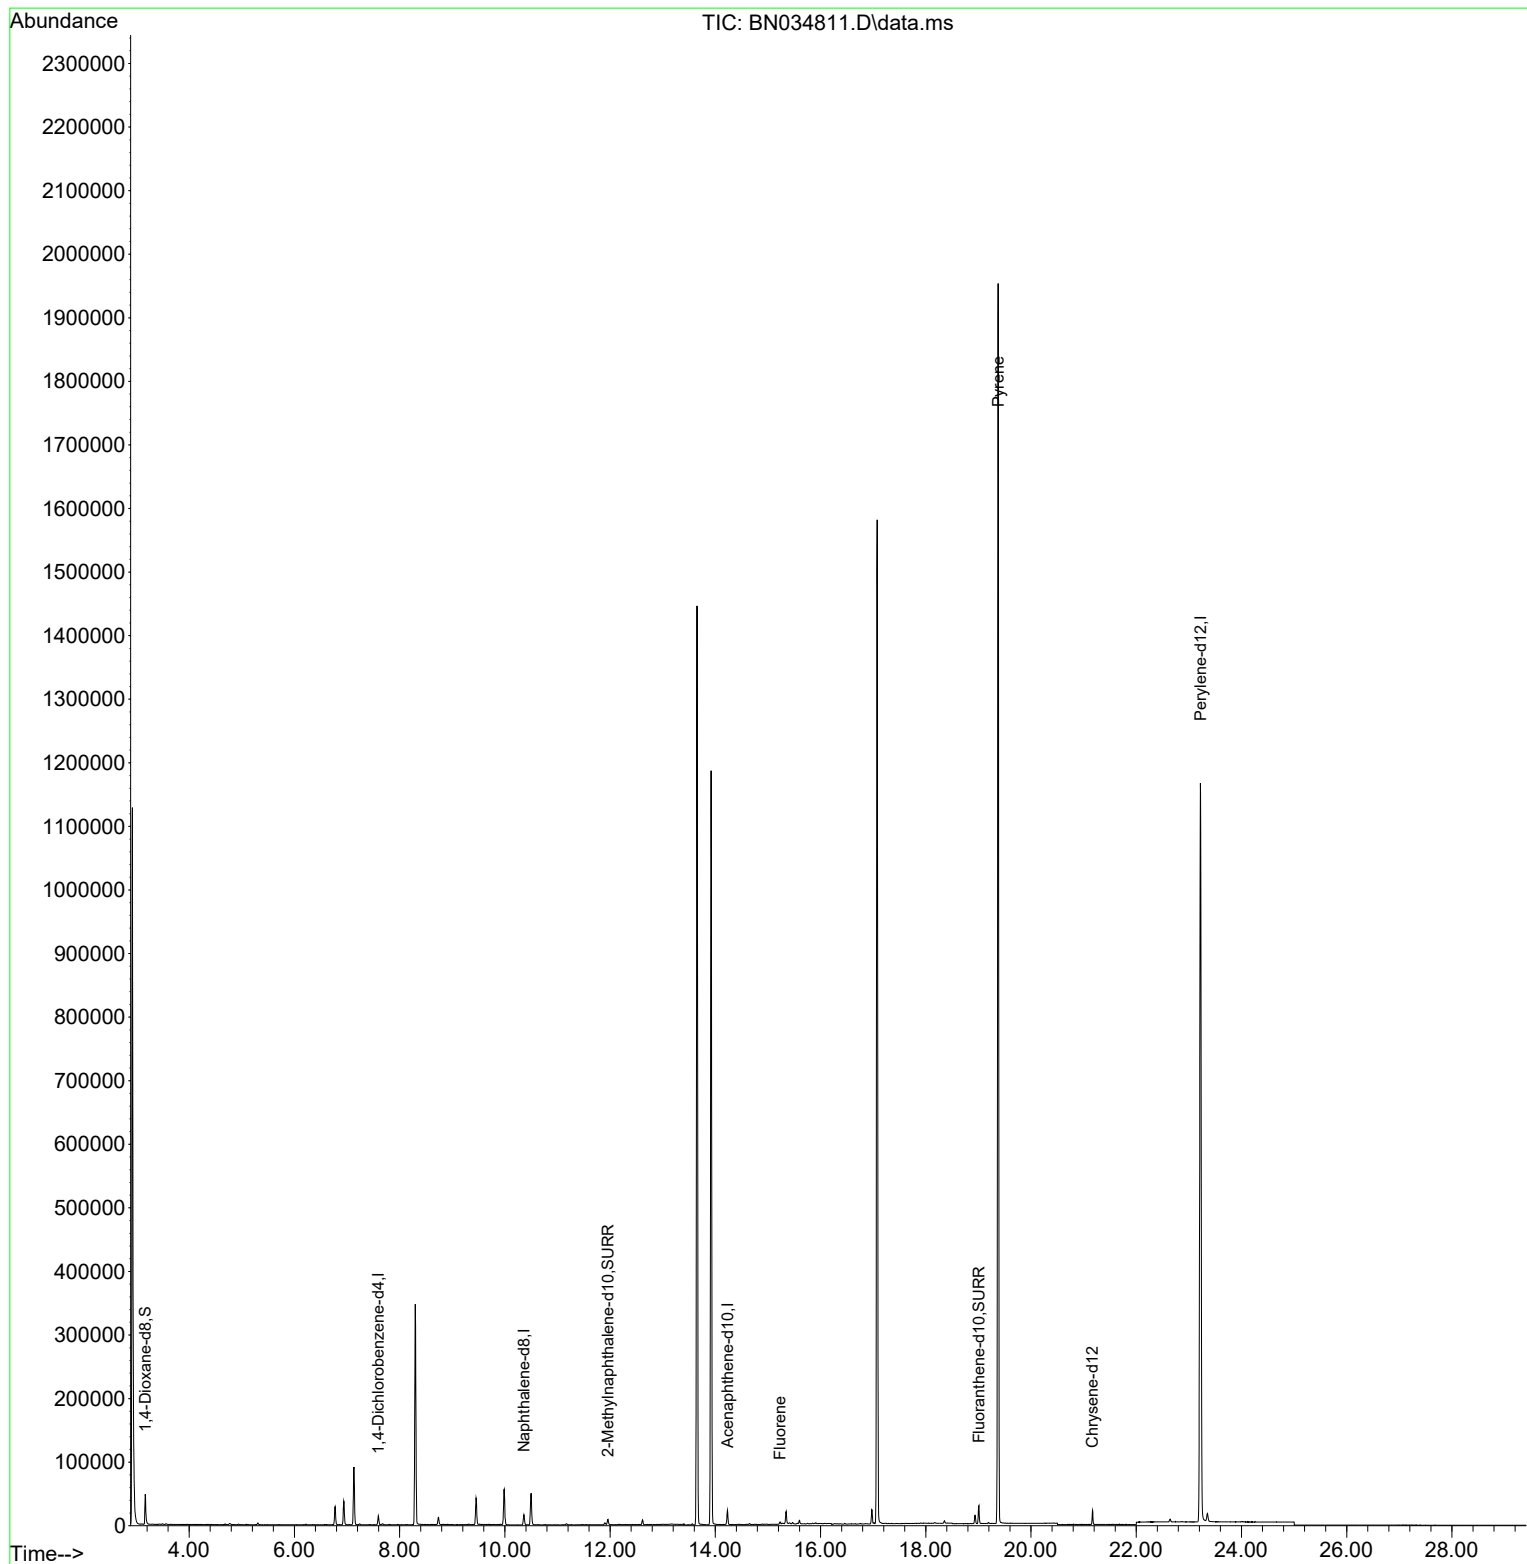

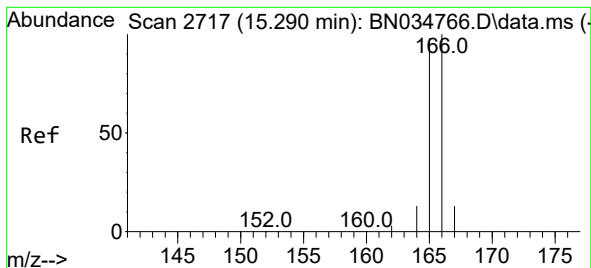

#12

Fluorene

Concen: 0.076 ng/ul

RT: 15.230 min Scan# 21

Delta R.T. -0.060 min

Lab File: BN034811.D

Acq: 01 Nov 2024 19:00

Instrument :

BNA_N

ClientSampleId :

E1L79





Tgt Ion:166 Resp: 3464

Ion Ratio Lower Upper

166 100

165 13.6 79.1 118.7#

167 37.8 11.0 16.4#

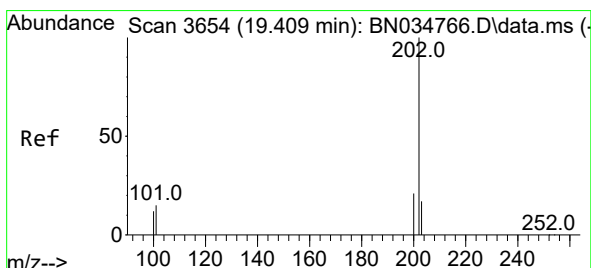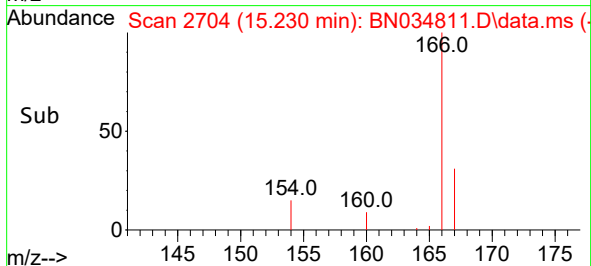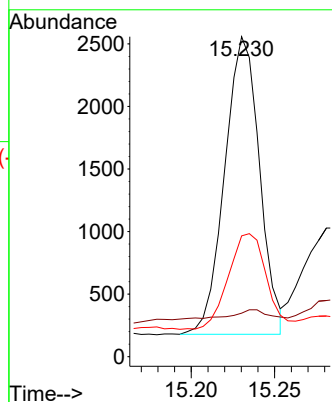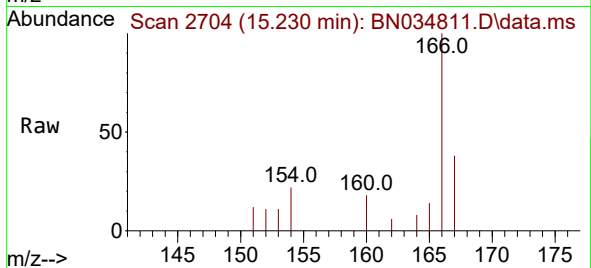

#20

Pyrene

Concen: 0.038 ng/ul

RT: 19.376 min Scan# 3647

Delta R.T. -0.033 min

Lab File: BN034811.D

Acq: 01 Nov 2024 19:00

Tgt Ion:202 Resp: 3342

Ion Ratio Lower Upper

202 100

101 173.7 12.4 18.6#

100 1214.7 10.0 15.0#

