

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
 Data File : BN034812.D
 Acq On : 01 Nov 2024 19:36
 Operator : RC/JU
 Sample : P4534-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1L63

Quant Time: Nov 03 23:27:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 11:13:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.596	152	6530	0.400	ng/ul	0.00
4) Naphthalene-d8	10.361	136	19933	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.231	164	11249	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-16.98
17) Chrysene-d12	21.168	240	15537	0.400	ng/ul	0.00
23) Perylene-d12	23.220	264	1312708	0.400	ng/ul	#-0.14
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.170	96	39078	5.781	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.955	152	10175	0.407	ng/ul	-0.01
18) Fluoranthene-d10	19.004	212	26805	0.530	ng/ul	0.00
Target Compounds						
					Qvalue	
19) Fluoranthene	19.037	202	1640	0.022	ng/ul#	87
20) Pyrene	19.376	202	4582	0.058	ng/ul#	1
22) Chrysene	21.204	228	1391	0.022	ng/ul	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034812.D
Acq On : 01 Nov 2024 19:36
Operator : RC/JU
Sample : P4534-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1L63

Quant Time: Nov 03 23:27:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration




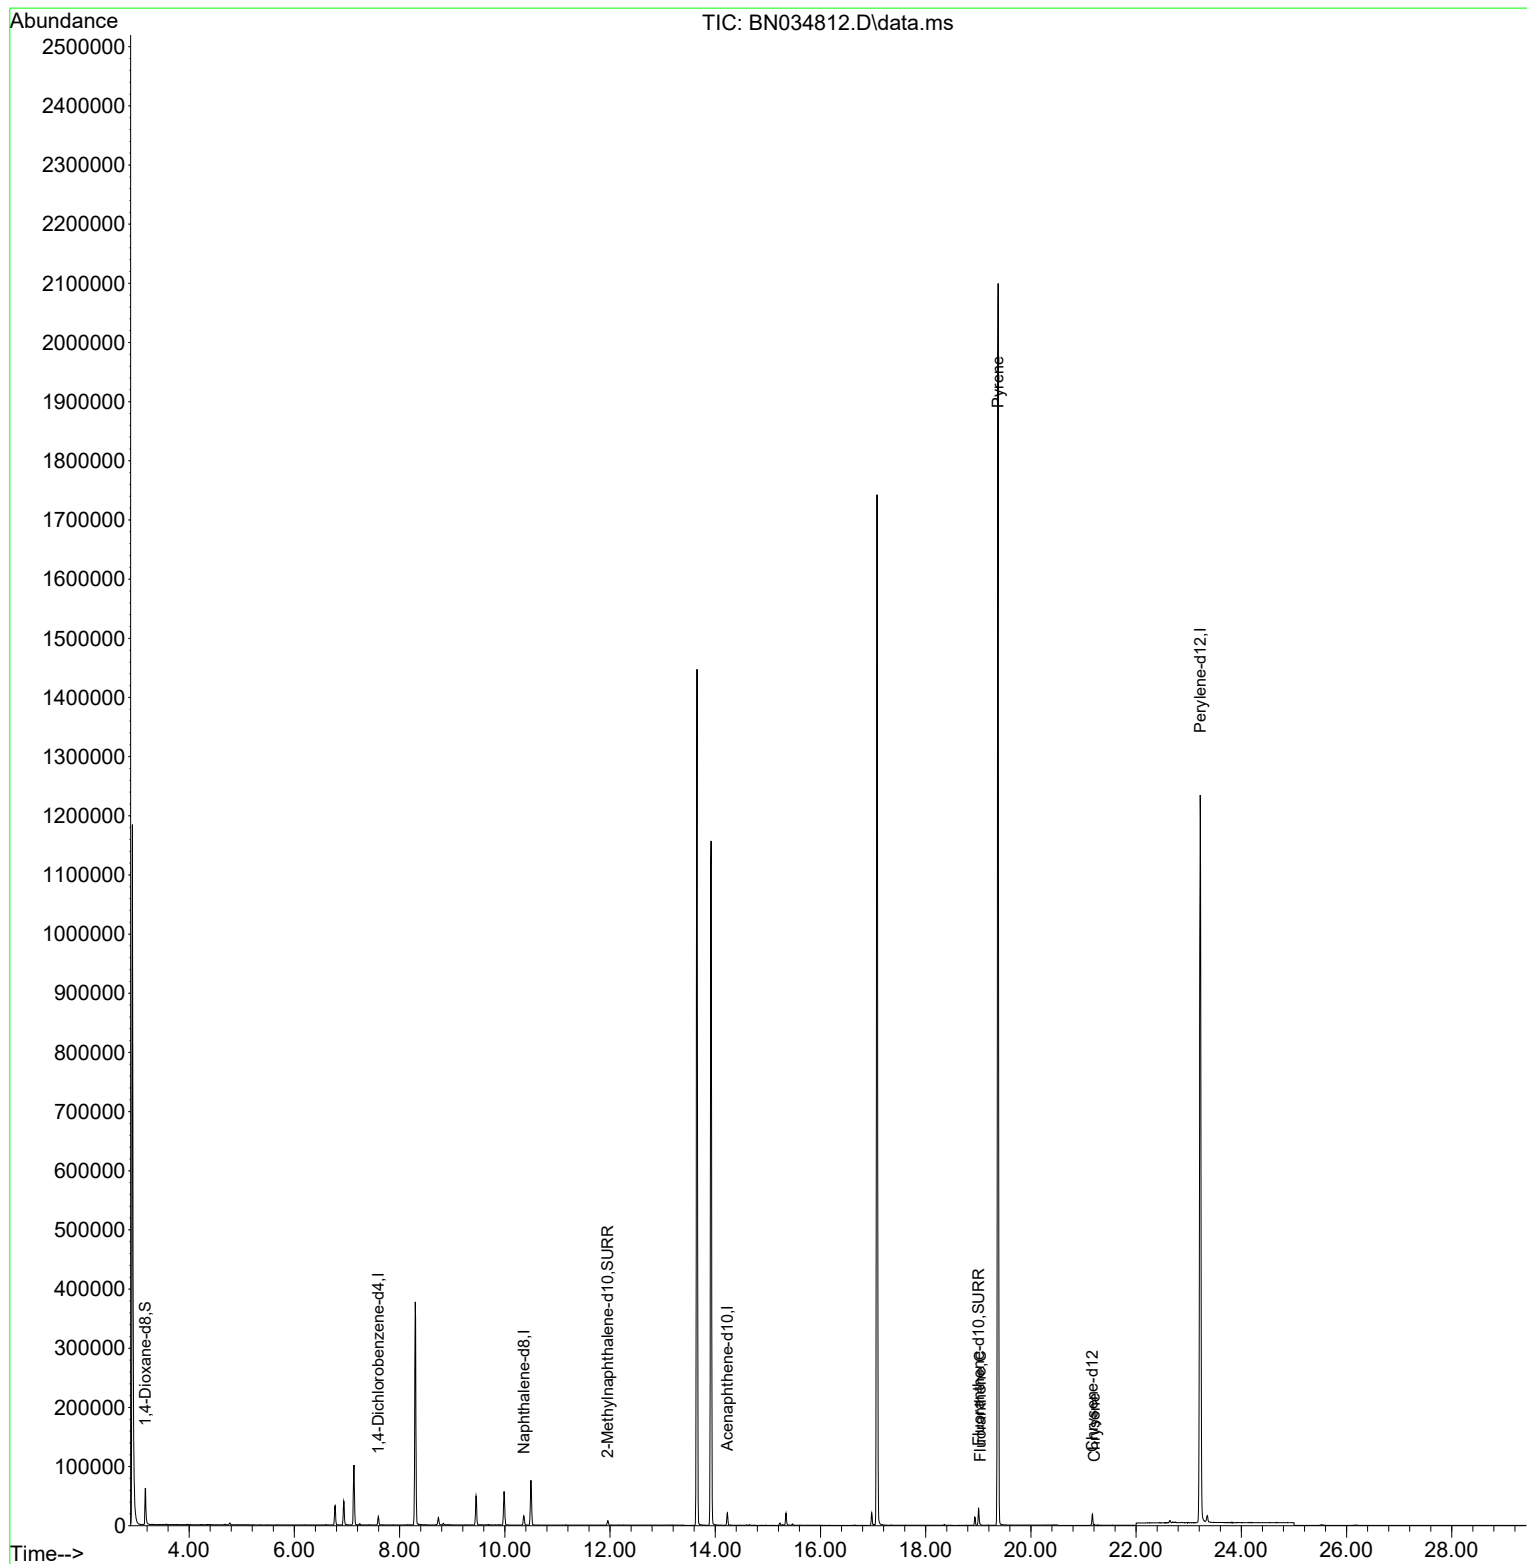


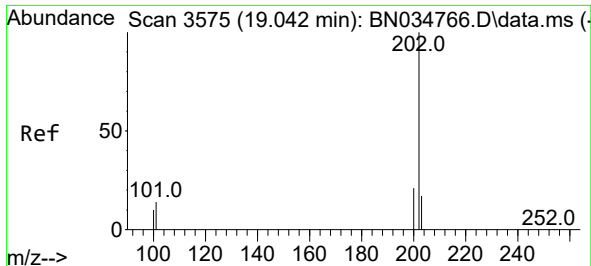

#19
Fluoranthene
Concen: 0.022 ng/ul
RT: 19.037 min Scan# 31
Delta R.T. -0.010 min
Lab File: BN034812.D
Acq: 01 Nov 2024 19:36




Instrument :
BNA_N
ClientSampleId :
E1L63


Tgt Ion:202 Resp: 1640
Ion Ratio Lower Upper
202 100
101 18.7 10.8 16.2#
100 14.9 8.2 12.2#

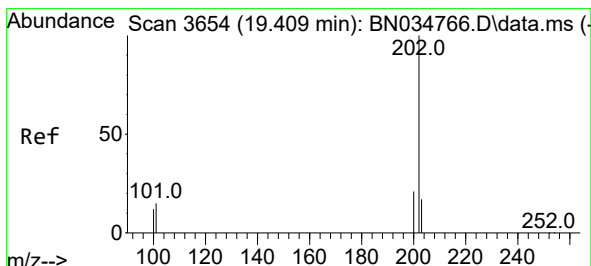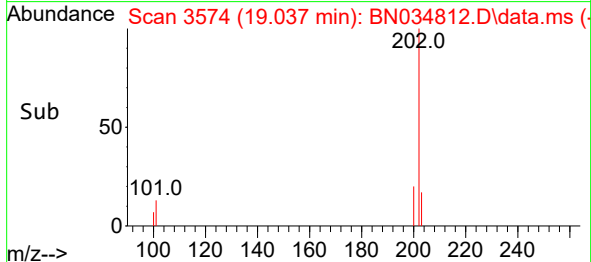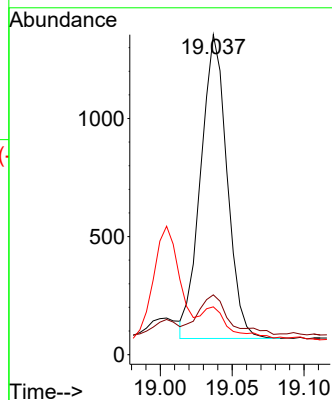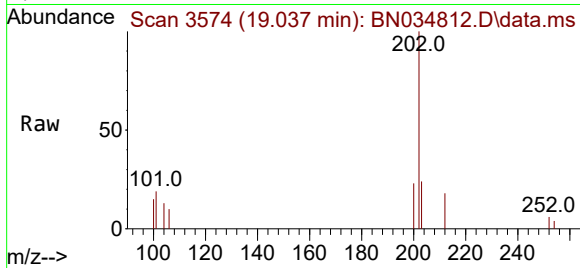

#20
Pyrene
Concen: 0.058 ng/ul
RT: 19.376 min Scan# 3647
Delta R.T. -0.033 min
Lab File: BN034812.D
Acq: 01 Nov 2024 19:36

Tgt Ion:202 Resp: 4582
Ion Ratio Lower Upper
202 100
101 188.0 12.4 18.6#
100 1381.5 10.0 15.0#

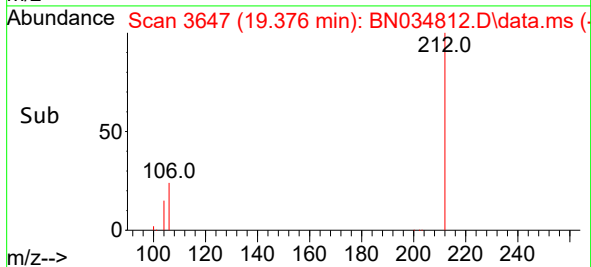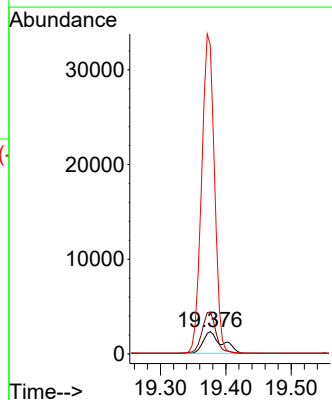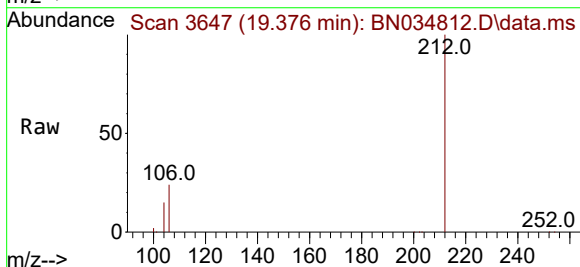

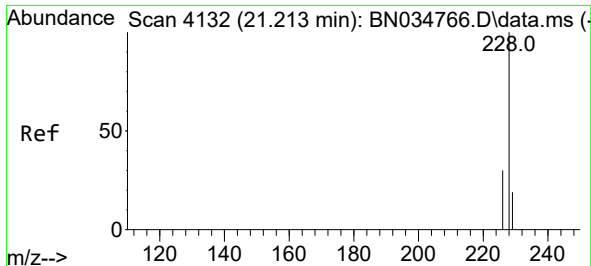

#22

Chrysene

Concen: 0.022 ng/ul

RT: 21.204 min Scan# 41

Delta R.T. -0.009 min

Lab File: BN034812.D


Acq: 01 Nov 2024 19:36

Instrument :

BNA_N

ClientSampleId :

E1L63

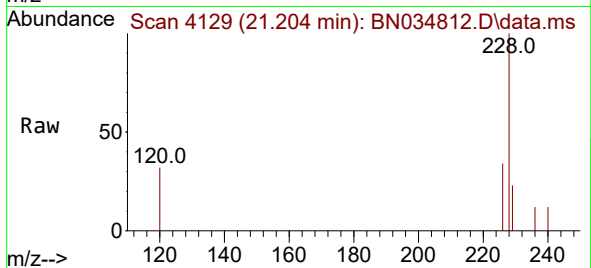

Tgt Ion:228 Resp: 1391

Ion Ratio Lower Upper

228 100

226 34.3 24.3 36.5

229 23.4 15.6 23.4

