

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
 Data File : BN034819.D
 Acq On : 02 Nov 2024 00:24
 Operator : RC/JU
 Sample : PB164447BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK447

Quant Time: Nov 03 23:28:48 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 11:13:08 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.596	152	8004	0.400	ng/ul	0.00
4) Naphthalene-d8	10.361	136	24918	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.231	164	13538	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-16.98
17) Chrysene-d12	21.166	240	16715	0.400	ng/ul	0.00
23) Perylene-d12	23.212	264	821819	0.400	ng/ul	#-0.15
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.170	96	48463	5.849	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.956	152	10354	0.331	ng/ul	-0.01
18) Fluoranthene-d10	19.005	212	18822	0.346	ng/ul	0.00
Target Compounds						
12) Fluorene	15.230	166	3003	0.057	ng/ul#	13
20) Pyrene	19.372	202	2638	0.031	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
 Data File : BN034819.D
 Acq On : 02 Nov 2024 00:24
 Operator : RC/JU
 Sample : PB164447BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK447

Quant Time: Nov 03 23:28:48 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 11:13:08 2024
 Response via : Initial Calibration

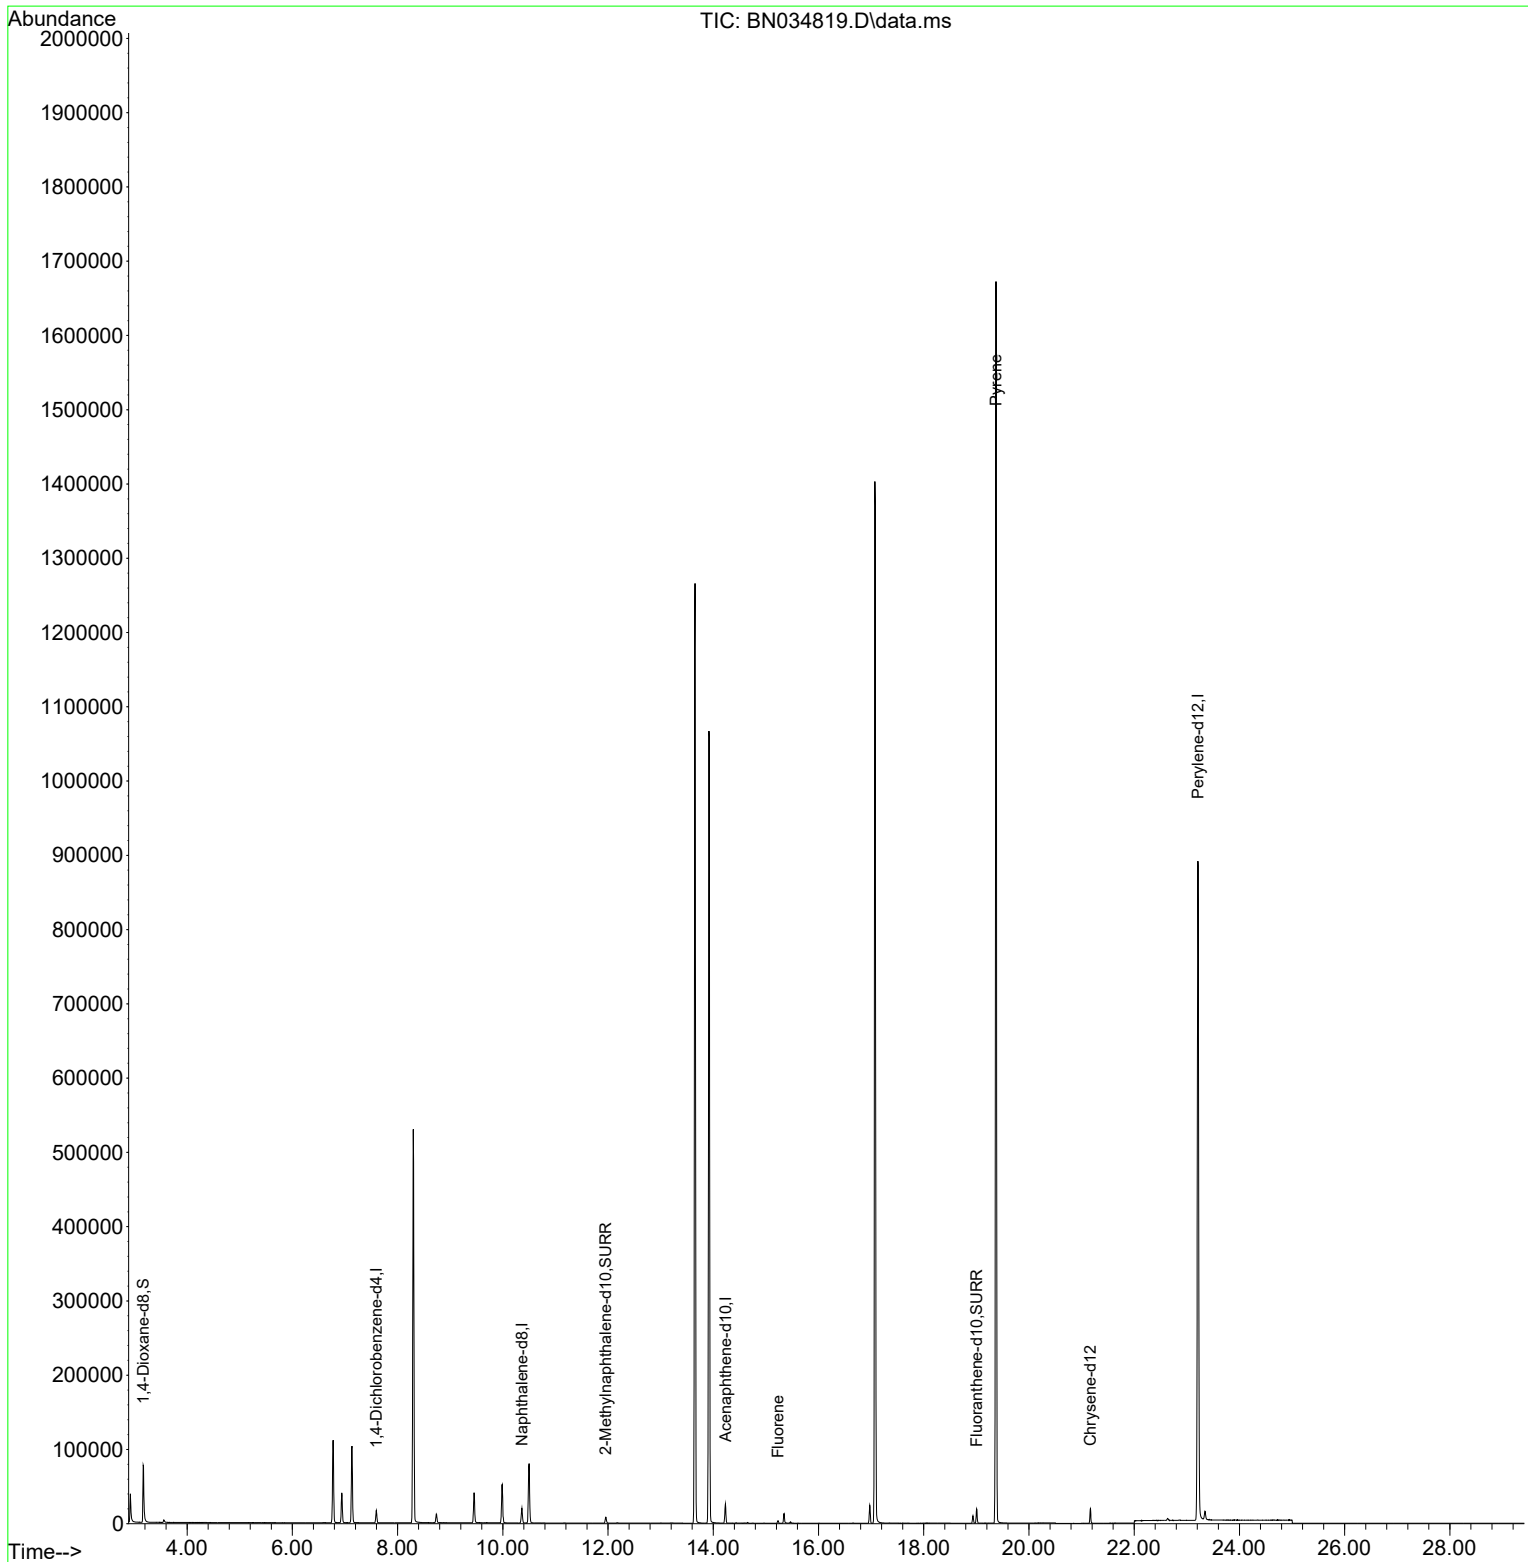




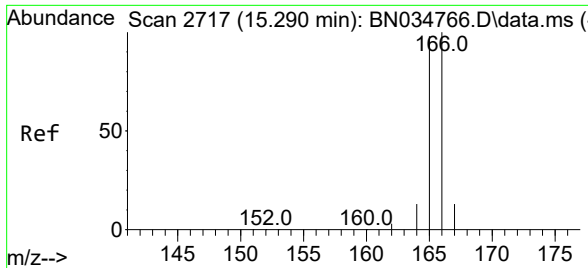


#12
 Fluorene
 Concen: 0.057 ng/u1
 RT: 15.230 min Scan# 21
 Delta R.T. -0.060 min
 Lab File: BN034819.D
 Acq: 02 Nov 2024 00:24

Instrument : BNA_N
 ClientSampleId : SBLK447

Tgt Ion:166 Resp: 3003

Ion	Ratio	Lower	Upper
166	100		
165	7.7	79.1	118.7#
167	36.4	11.0	16.4#

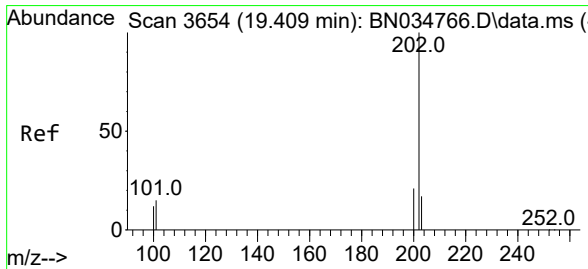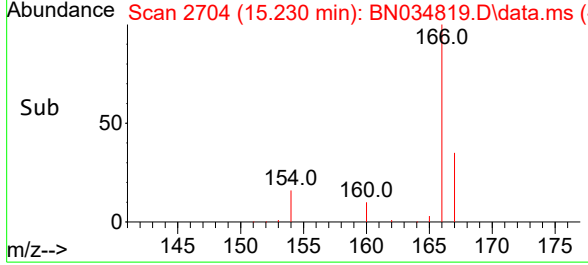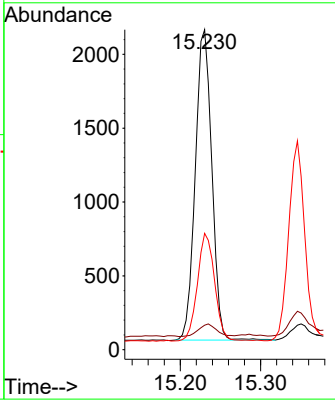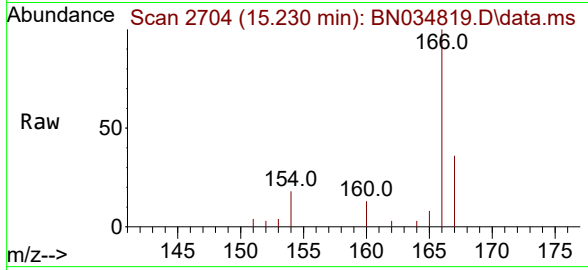

#20
 Pyrene
 Concen: 0.031 ng/u1
 RT: 19.372 min Scan# 3646
 Delta R.T. -0.037 min
 Lab File: BN034819.D
 Acq: 02 Nov 2024 00:24

Tgt Ion:202 Resp: 2638

Ion	Ratio	Lower	Upper
202	100		
101	195.6	12.4	18.6#
100	1482.3	10.0	15.0#

