

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
 Data File : BN034820.D
 Acq On : 02 Nov 2024 01:01
 Operator : RC/JU
 Sample : PB164475BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK475

Quant Time: Nov 03 23:28:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 11:13:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.596	152	6952	0.400	ng/ul	0.00
4) Naphthalene-d8	10.361	136	21489	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.231	164	11862	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-16.98
17) Chrysene-d12	21.166	240	14266	0.400	ng/ul	0.00
23) Perylene-d12	23.211	264	832277	0.400	ng/ul	#-0.15
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.166	96	48228	6.702	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.956	152	10502	0.390	ng/ul	-0.01
18) Fluoranthene-d10	19.005	212	19694	0.424	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.230	166	3139	0.068	ng/ul#	13
20) Pyrene	19.376	202	2692	0.037	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034820.D
Acq On : 02 Nov 2024 01:01
Operator : RC/JU
Sample : PB164475BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK475

Quant Time: Nov 03 23:28:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration




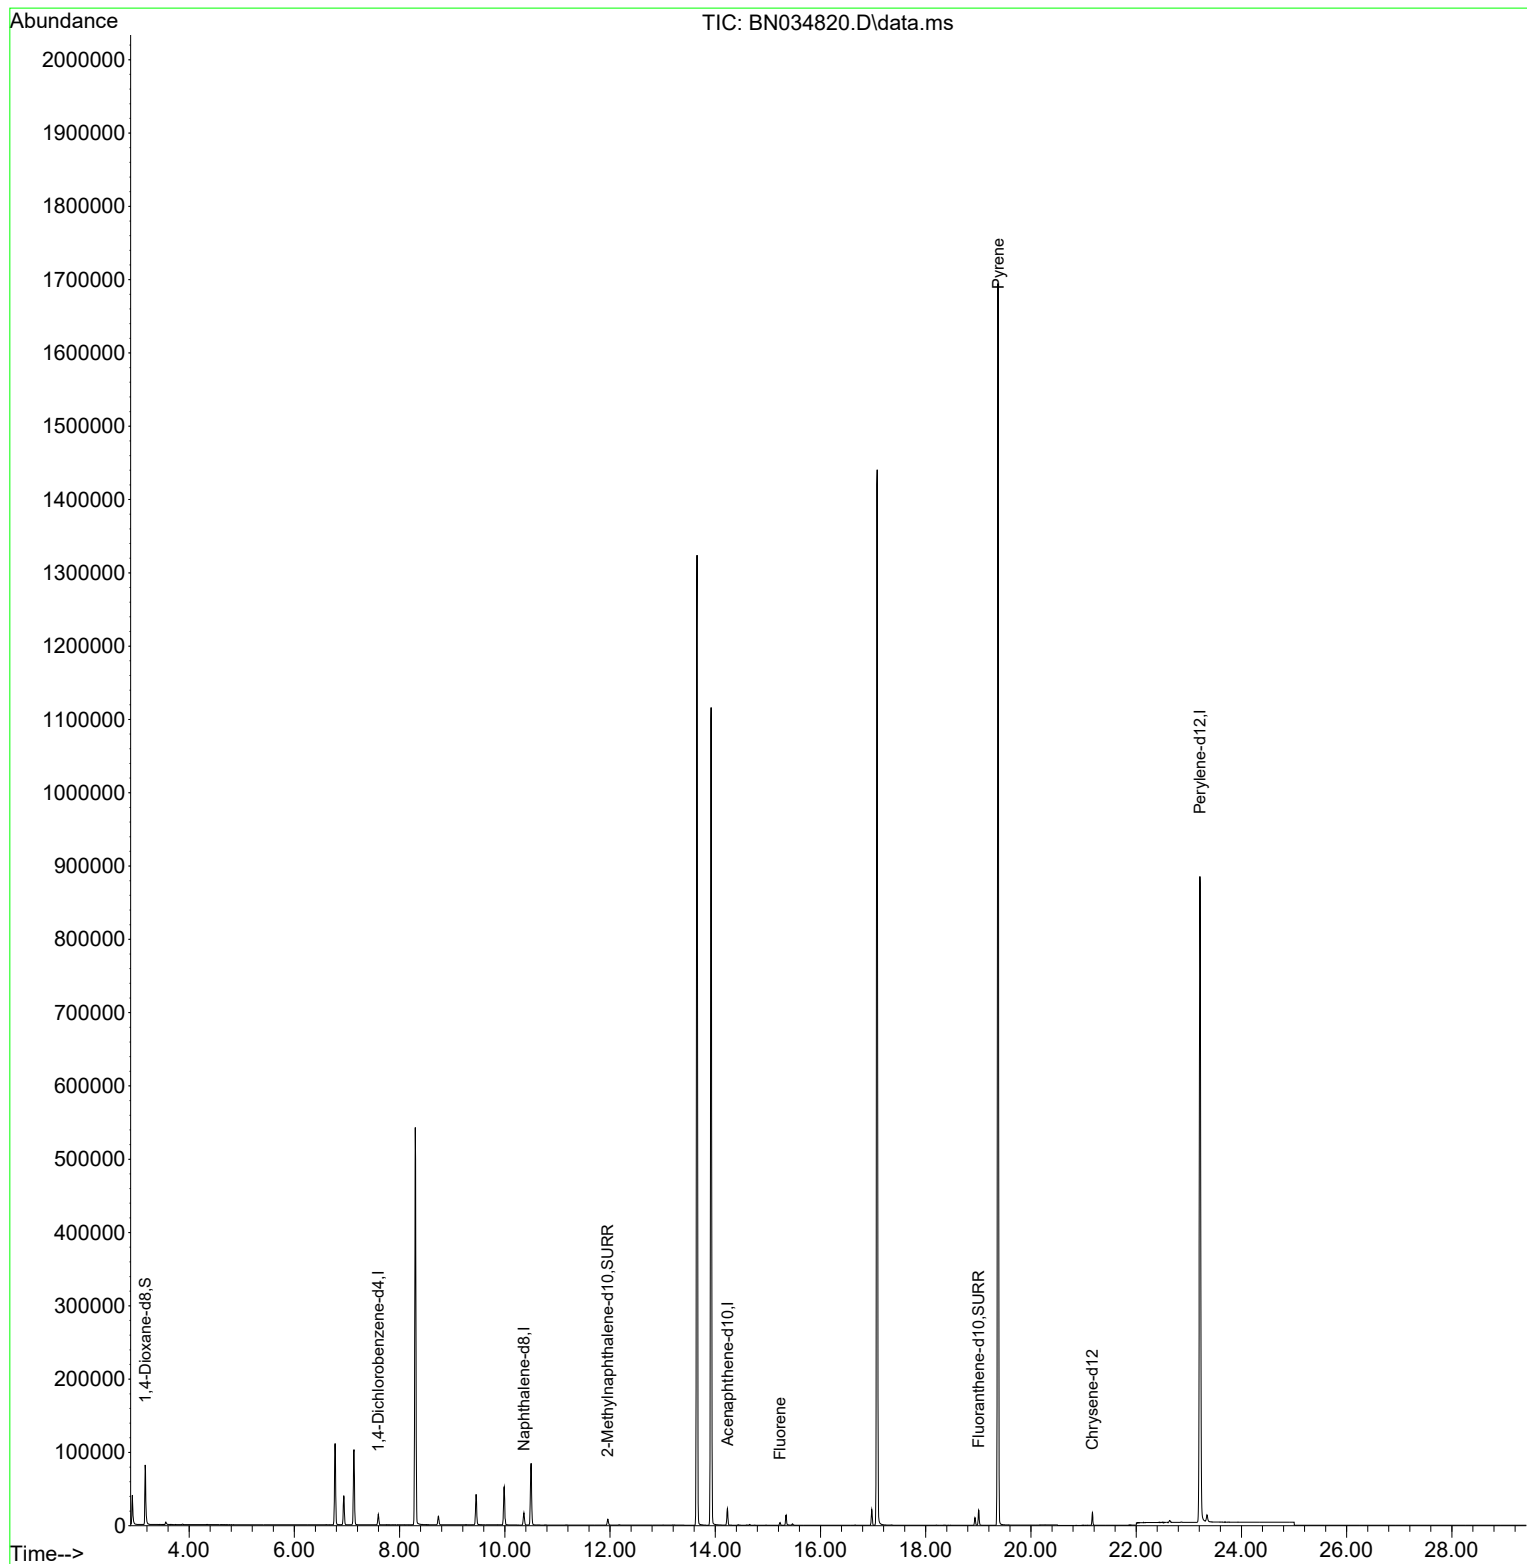


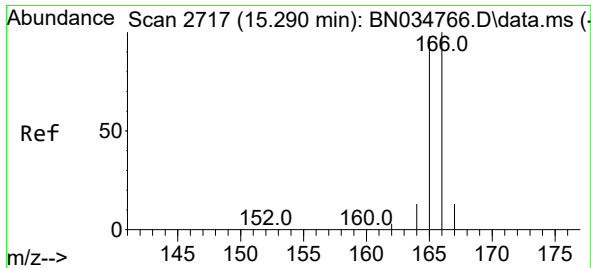

#12
Fluorene
Concen: 0.068 ng/ul
RT: 15.230 min Scan# 21
Delta R.T. -0.060 min
Lab File: BN034820.D
Acq: 02 Nov 2024 01:01

Instrument :
BNA_N
ClientSampleId :
SBLK475

Tgt Ion:166 Resp: 3139
Ion Ratio Lower Upper
166 100
165 7.0 79.1 118.7#
167 33.7 11.0 16.4#

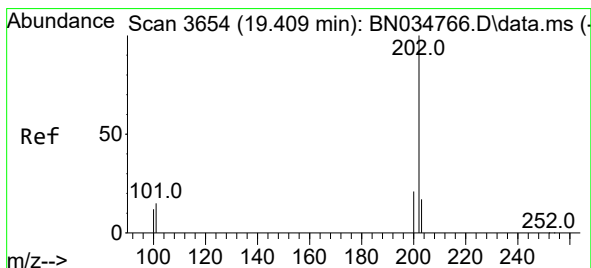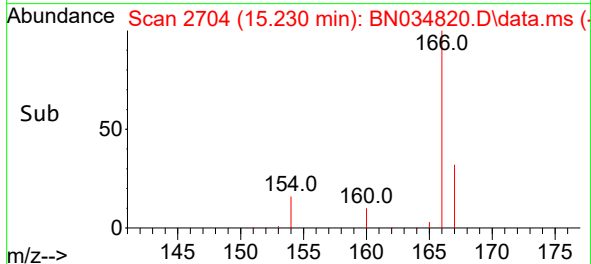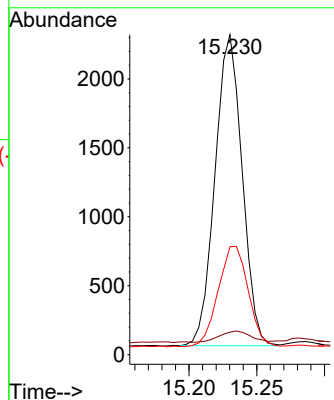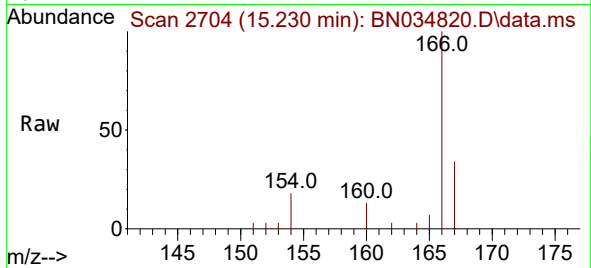

#20
Pyrene
Concen: 0.037 ng/ul
RT: 19.376 min Scan# 3647
Delta R.T. -0.033 min
Lab File: BN034820.D
Acq: 02 Nov 2024 01:01

Tgt Ion:202 Resp: 2692
Ion Ratio Lower Upper
202 100
101 178.1 12.4 18.6#
100 1235.7 10.0 15.0#

